

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
 Data File : PD063235.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2021 11:29
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 13:36:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Mon May 24 13:35:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.971	104.5E6	846.4E6	76.581	73.950
28)	SA Decachlor...	8.195	9.024	91360902	764.3E6	76.312	73.978
Target Compounds							
23)	Chlordane-1	4.308	4.961	33668377	404.4E6	752.892	739.574
24)	Chlordane-2	4.809	5.428	39697154	387.3E6	739.254	748.878
25)	Chlordane-3	5.378	6.074	121.8E6	1642.3E6	761.240	751.491
26)	Chlordane-4	5.436	6.148	99377162	1869.9E6	762.327	749.764
27)	Chlordane-5	6.272	6.951	34008391	332.9E6	693.347	858.293



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
Data File : PD063235.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2021 11:29
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 13:36:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Mon May 24 13:35:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

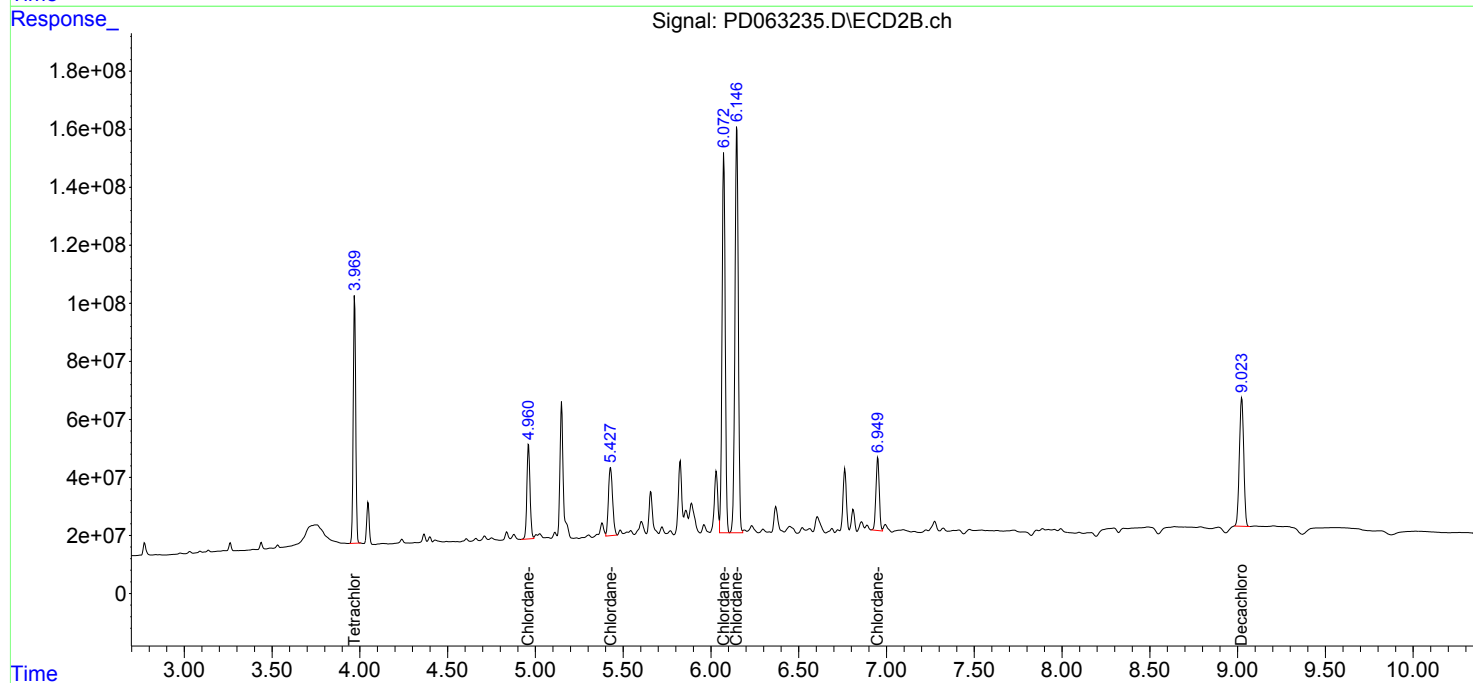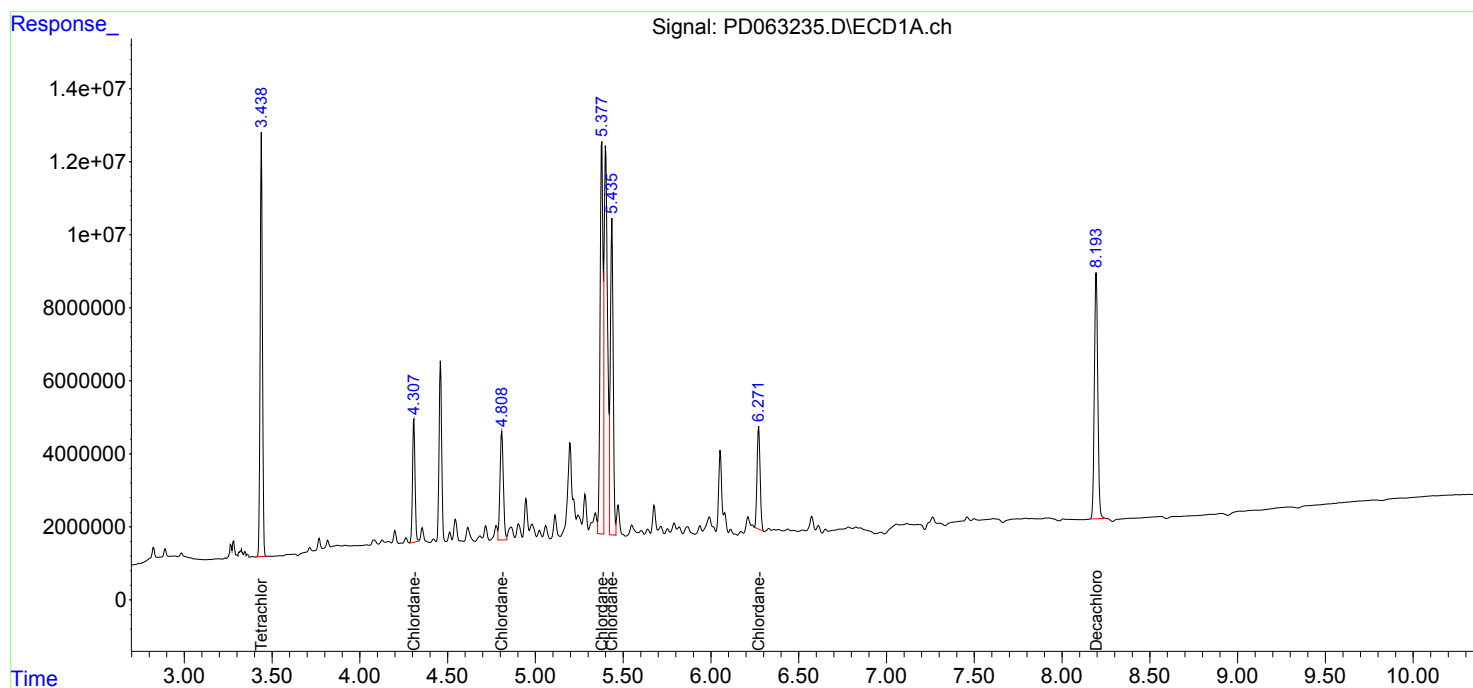


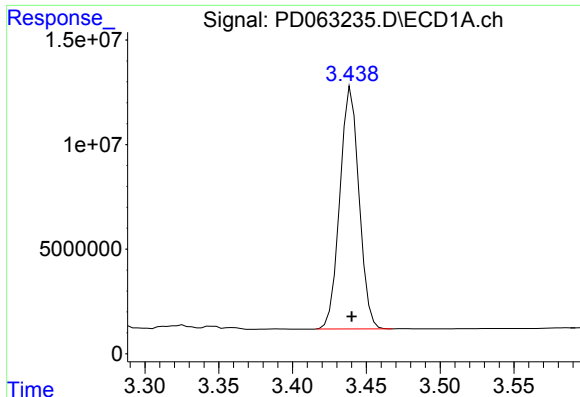

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 104497519
Conc: 76.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

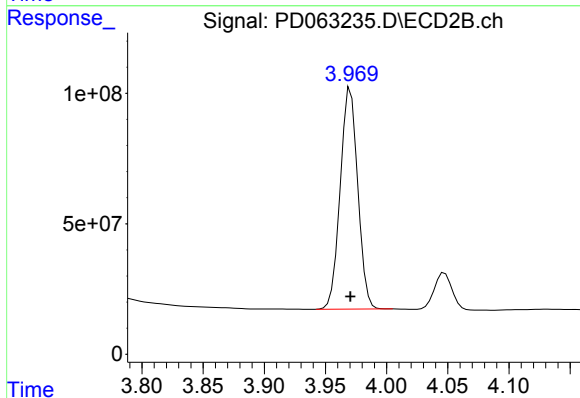


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 846376984
Conc: 73.95 ng/ml

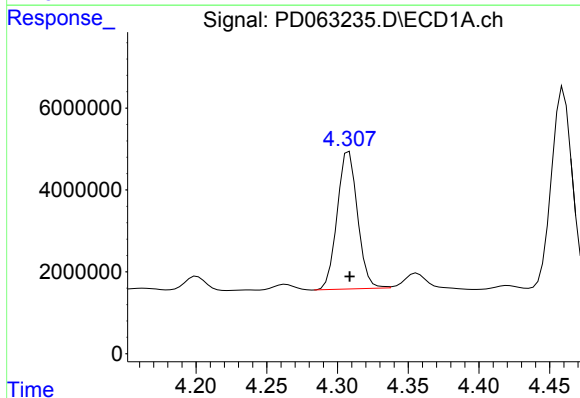


#23 Chlordane-1

R.T.: 4.308 min
Delta R.T.: 0.000 min
Response: 33668377
Conc: 752.89 ng/ml

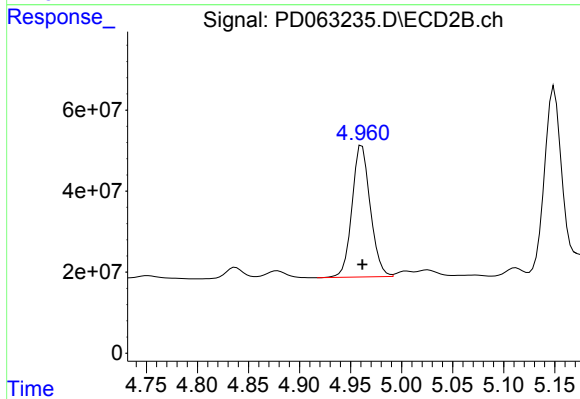

#23 Chlordane-1


R.T.: 4.961 min
Delta R.T.: 0.000 min
Response: 404442135
Conc: 739.57 ng/ml

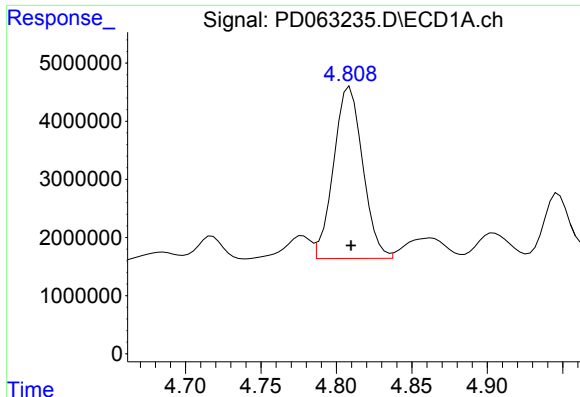

#24 Chlordane-2


R.T.: 4.809 min
Delta R.T.: 0.000 min
Response: 39697154
Conc: 739.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

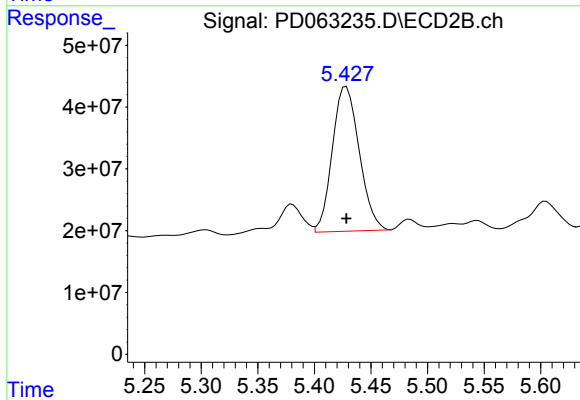


#24 Chlordane-2

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 387333460
Conc: 748.88 ng/ml

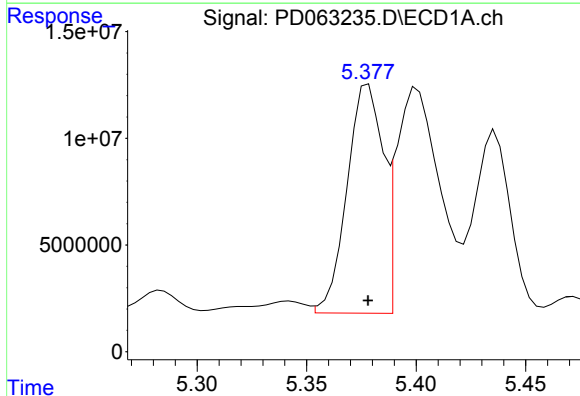


#25 Chlordane-3

R.T.: 5.378 min
Delta R.T.: 0.000 min
Response: 121843526
Conc: 761.24 ng/ml

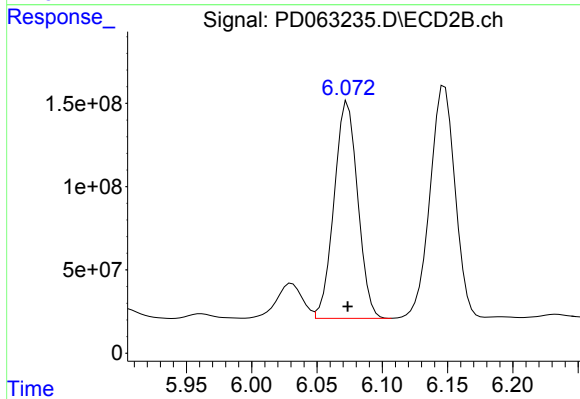

#25 Chlordane-3


R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 1642331620
Conc: 751.49 ng/ml

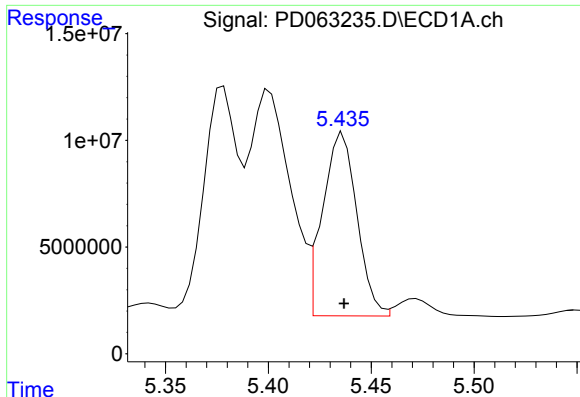

#26 Chlordane-4


R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 99377162
Conc: 762.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

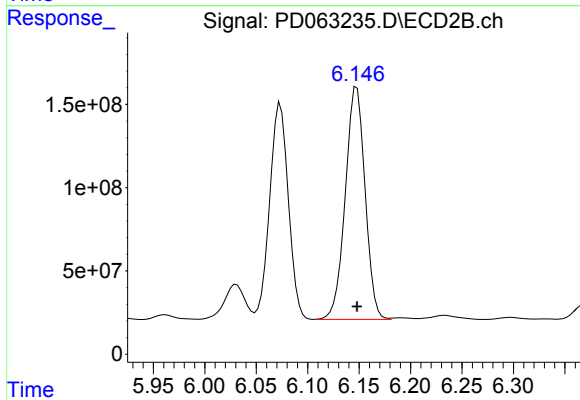


#26 Chlordane-4

R.T.: 6.148 min
Delta R.T.: 0.000 min
Response: 1869900277
Conc: 749.76 ng/ml

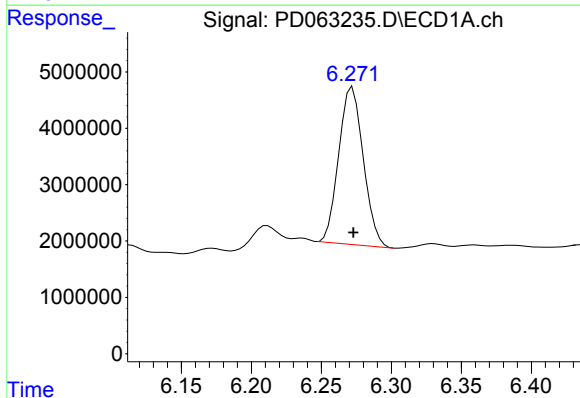


#27 Chlordane-5

R.T.: 6.272 min
Delta R.T.: 0.000 min
Response: 34008391
Conc: 693.35 ng/ml

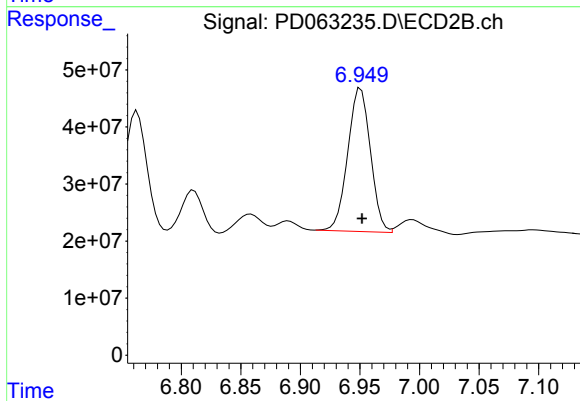

#27 Chlordane-5


R.T.: 6.951 min
Delta R.T.: -0.001 min
Response: 332939907
Conc: 858.29 ng/ml

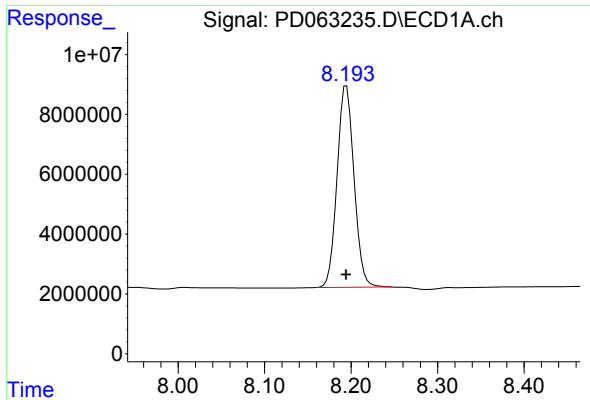

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 91360902
Conc: 76.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

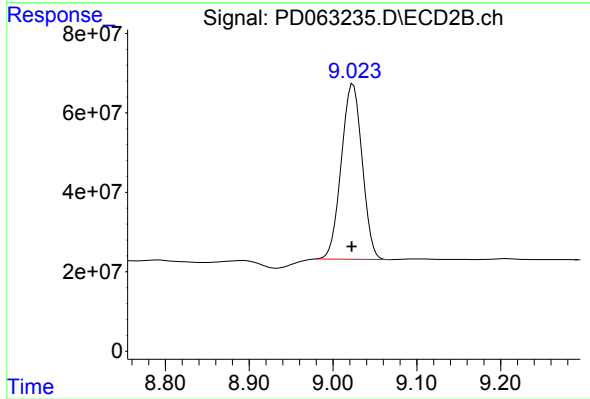

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.002 min
Response: 764263374
Conc: 73.98 ng/ml