

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
 Data File : PD063236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2021 11:43
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 13:36:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Mon May 24 13:35:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	68226825	572.3E6	50.000	50.000
28)	SA Decachlor...	8.194	9.022	59860068	516.5E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.309	4.962	22359366	273.4E6	500.000	500.000
24)	Chlordane-2	4.810	5.428	26849486	258.6E6	500.000	500.000
25)	Chlordane-3	5.378	6.073	80029596	1092.7E6	500.000	500.000
26)	Chlordane-4	5.437	6.148	65180109	1247.0E6	500.000	500.000
27)	Chlordane-5	6.273	6.952	24524801	194.0E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
Data File : PD063236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2021 11:43
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 13:36:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Mon May 24 13:35:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

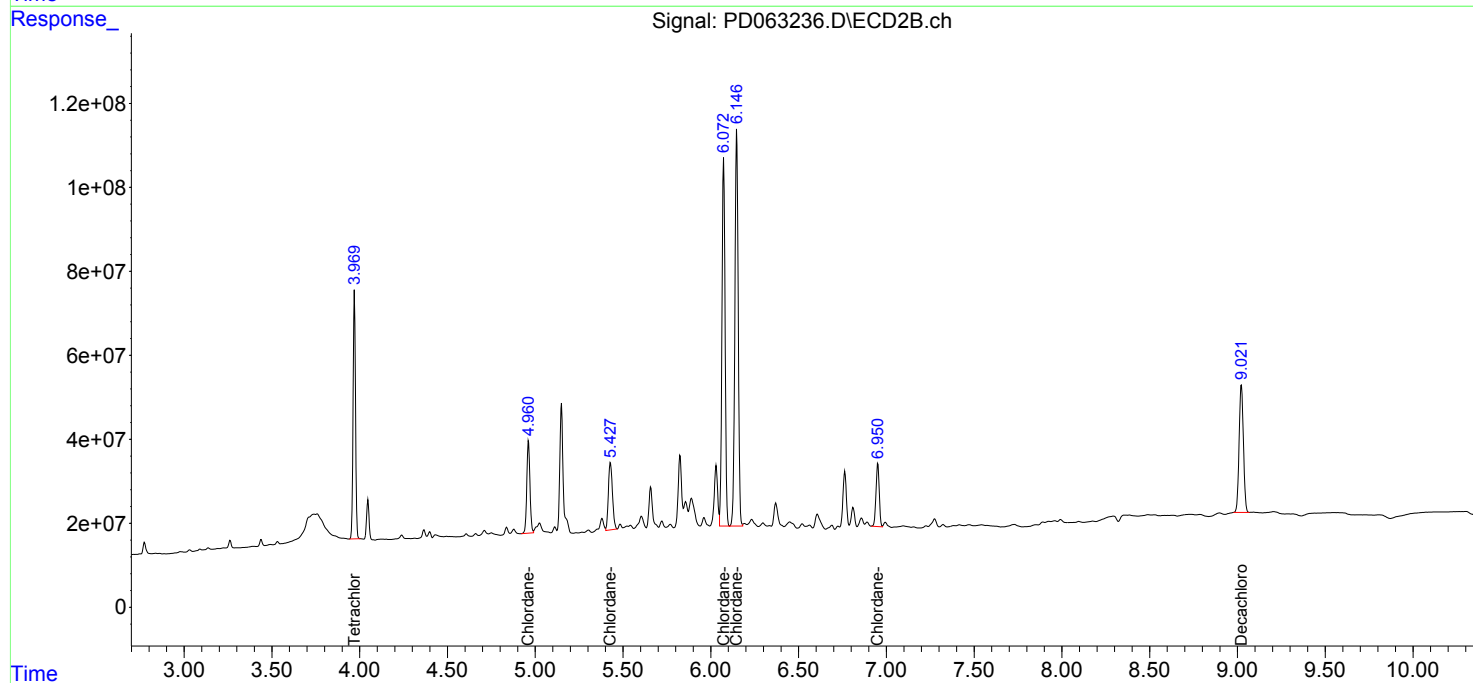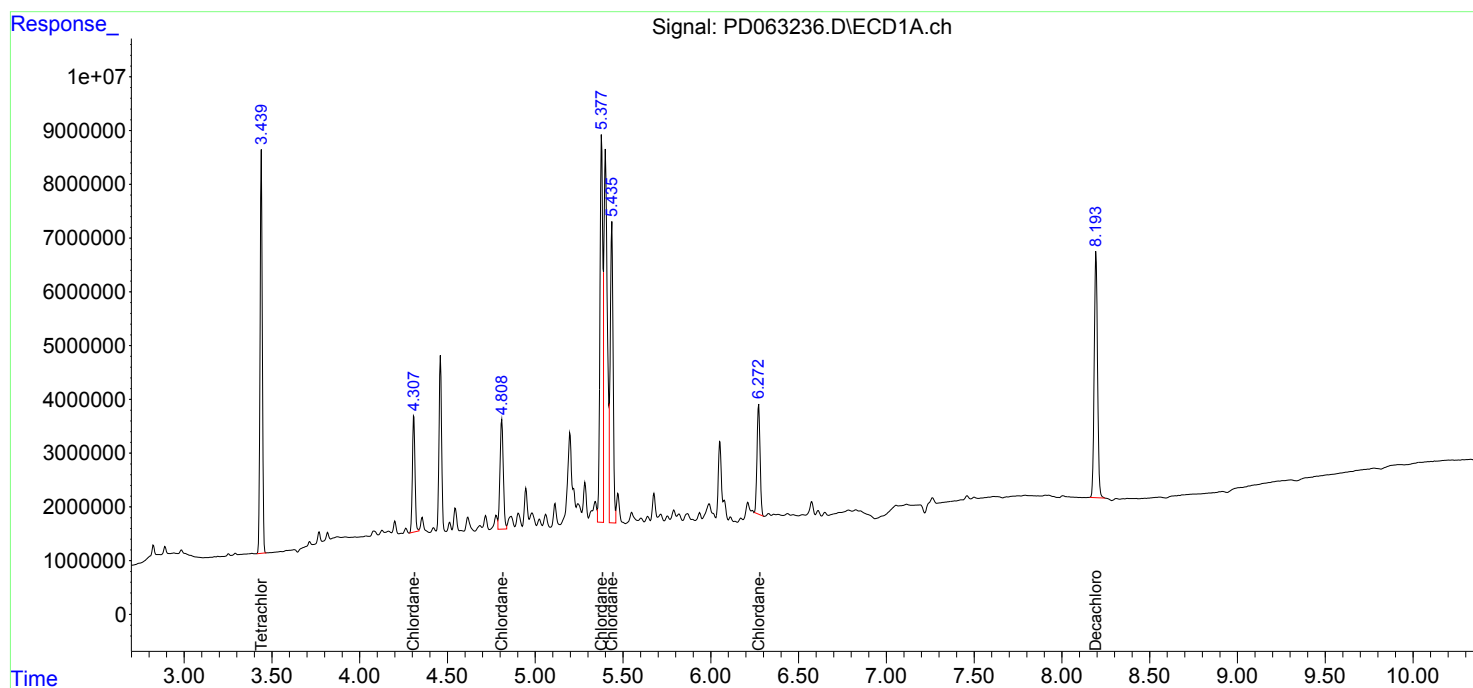


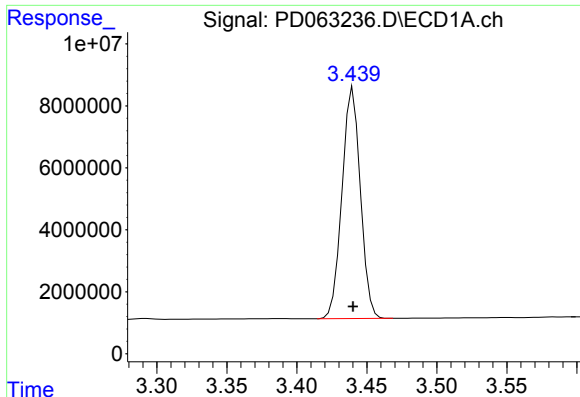

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 68226825
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

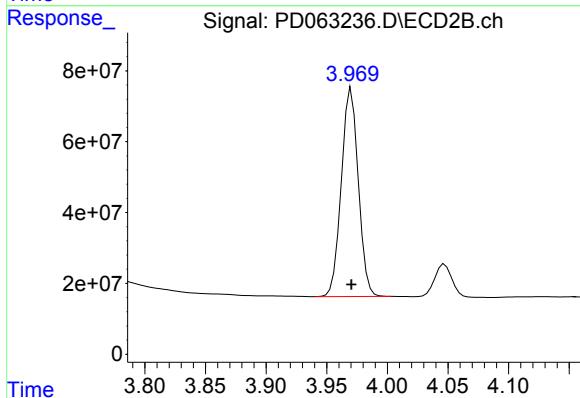


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 572264006
Conc: 50.00 ng/ml

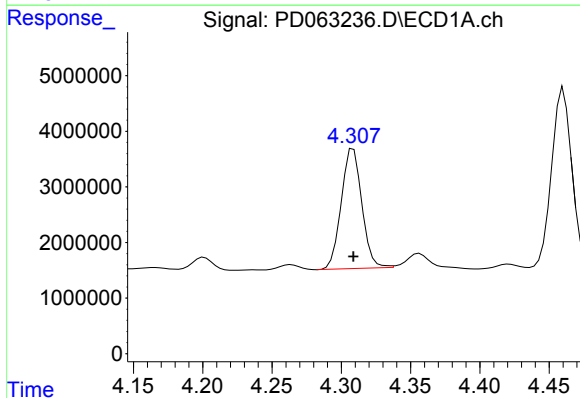


#23 Chlordane-1

R.T.: 4.309 min
Delta R.T.: 0.000 min
Response: 22359366
Conc: 500.00 ng/ml

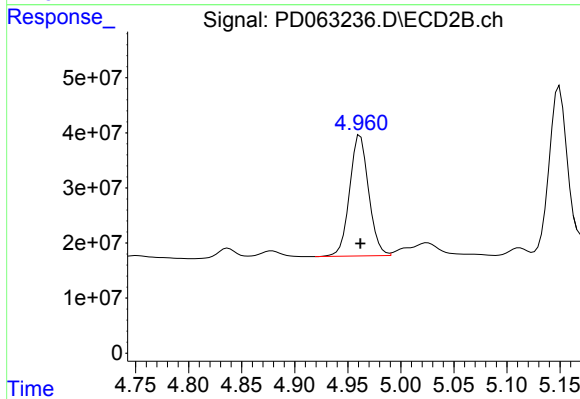

#23 Chlordane-1


R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 273429002
Conc: 500.00 ng/ml

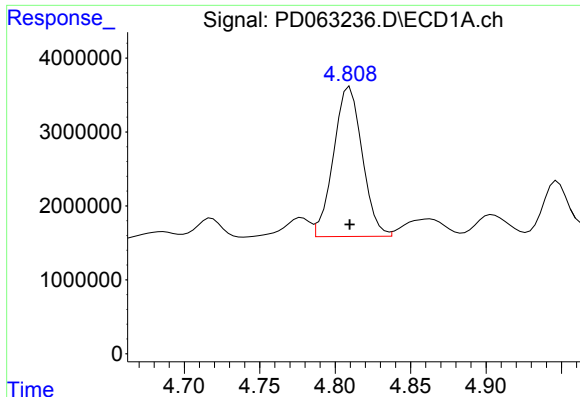

#24 Chlordane-2


R.T.: 4.810 min
Delta R.T.: 0.000 min
Response: 26849486
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

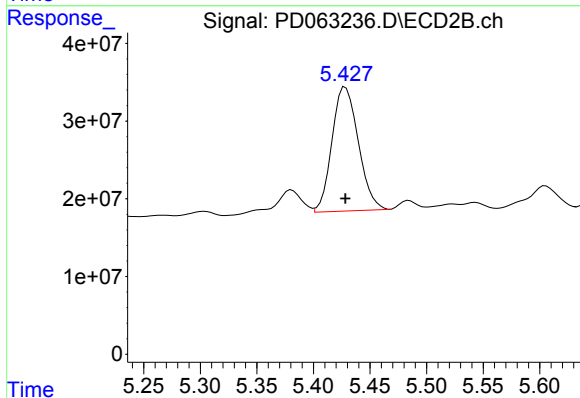


#24 Chlordane-2

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 258609292
Conc: 500.00 ng/ml

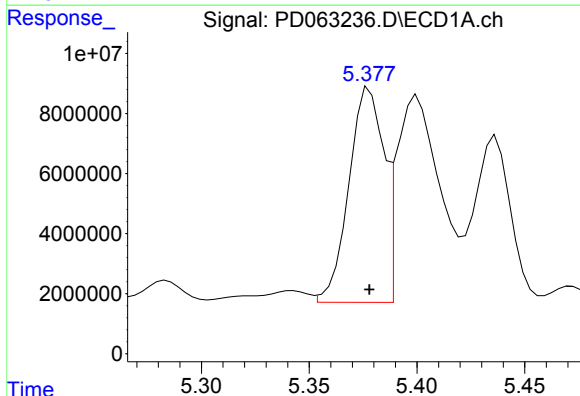


#25 Chlordane-3

R.T.: 5.378 min
Delta R.T.: 0.000 min
Response: 80029596
Conc: 500.00 ng/ml

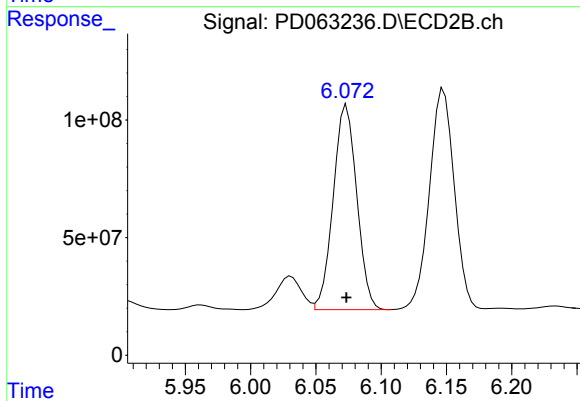

#25 Chlordane-3


R.T.: 6.073 min
Delta R.T.: 0.000 min
Response: 1092715243
Conc: 500.00 ng/ml

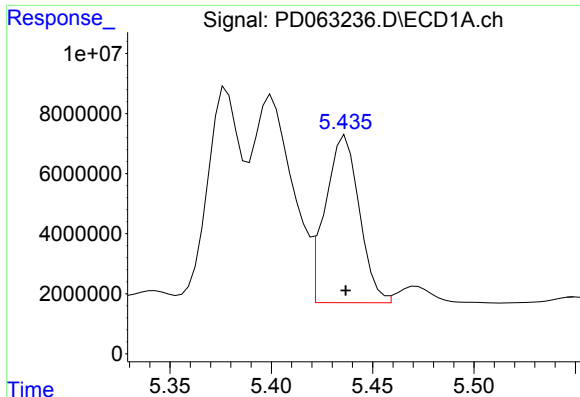

#26 Chlordane-4


R.T.: 5.437 min
Delta R.T.: 0.000 min
Response: 65180109
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

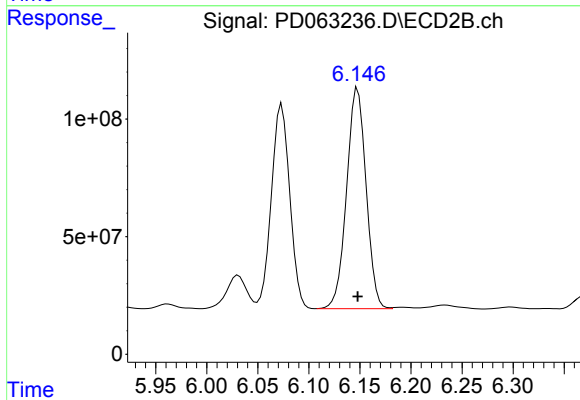


#26 Chlordane-4

R.T.: 6.148 min
Delta R.T.: 0.000 min
Response: 1246992953
Conc: 500.00 ng/ml

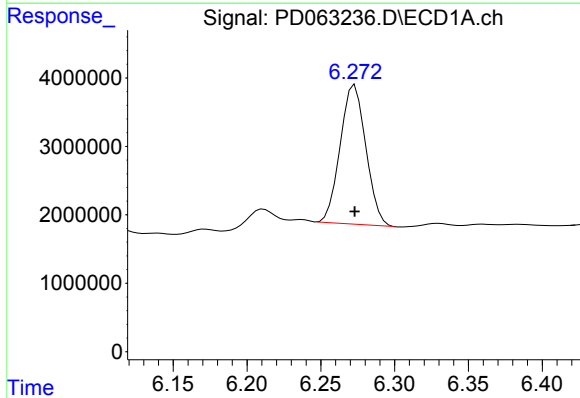


#27 Chlordane-5

R.T.: 6.273 min
Delta R.T.: 0.000 min
Response: 24524801
Conc: 500.00 ng/ml

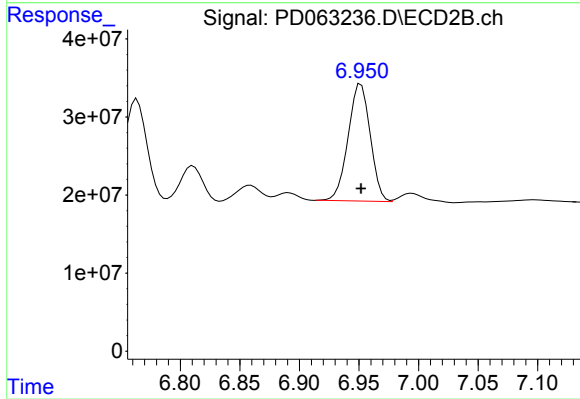

#27 Chlordane-5


R.T.: 6.952 min
Delta R.T.: 0.000 min
Response: 193954783
Conc: 500.00 ng/ml

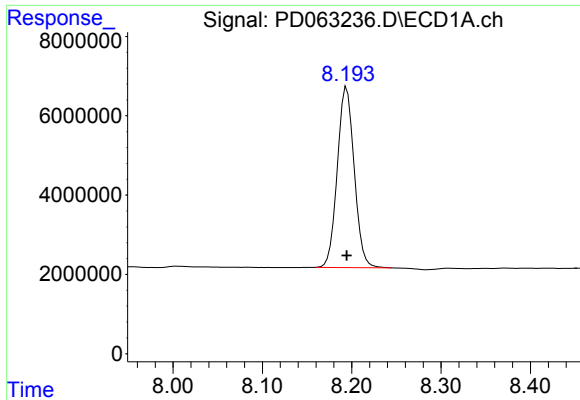

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 59860068
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

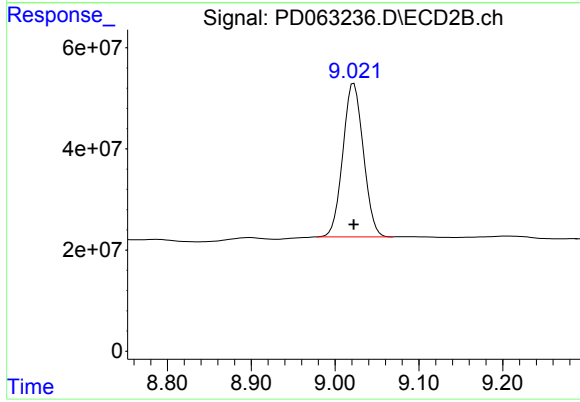

#28 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: 0.000 min
Response: 516548027
Conc: 50.00 ng/ml