

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
 Data File : PD063237.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2021 11:57
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 13:37:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Mon May 24 13:35:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.971	33541838	301.7E6	24.581	26.362
28)	SA Decachlor...	8.195	9.024	32193152	273.1E6	26.890	26.439
Target Compounds							
23)	Chlordane-1	4.308	4.962	11148562	145.8E6	249.304	266.690
24)	Chlordane-2	4.809	5.429	14028785	138.3E6	261.249	267.325
25)	Chlordane-3	5.378	6.074	39208229	575.0E6	244.961	263.124
26)	Chlordane-4	5.436	6.149	32395931	661.8E6	248.511	265.365
27)	Chlordane-5	6.272	6.952	12075597	108.9E6	246.192	280.702



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
Data File : PD063237.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2021 11:57
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 13:37:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Mon May 24 13:35:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

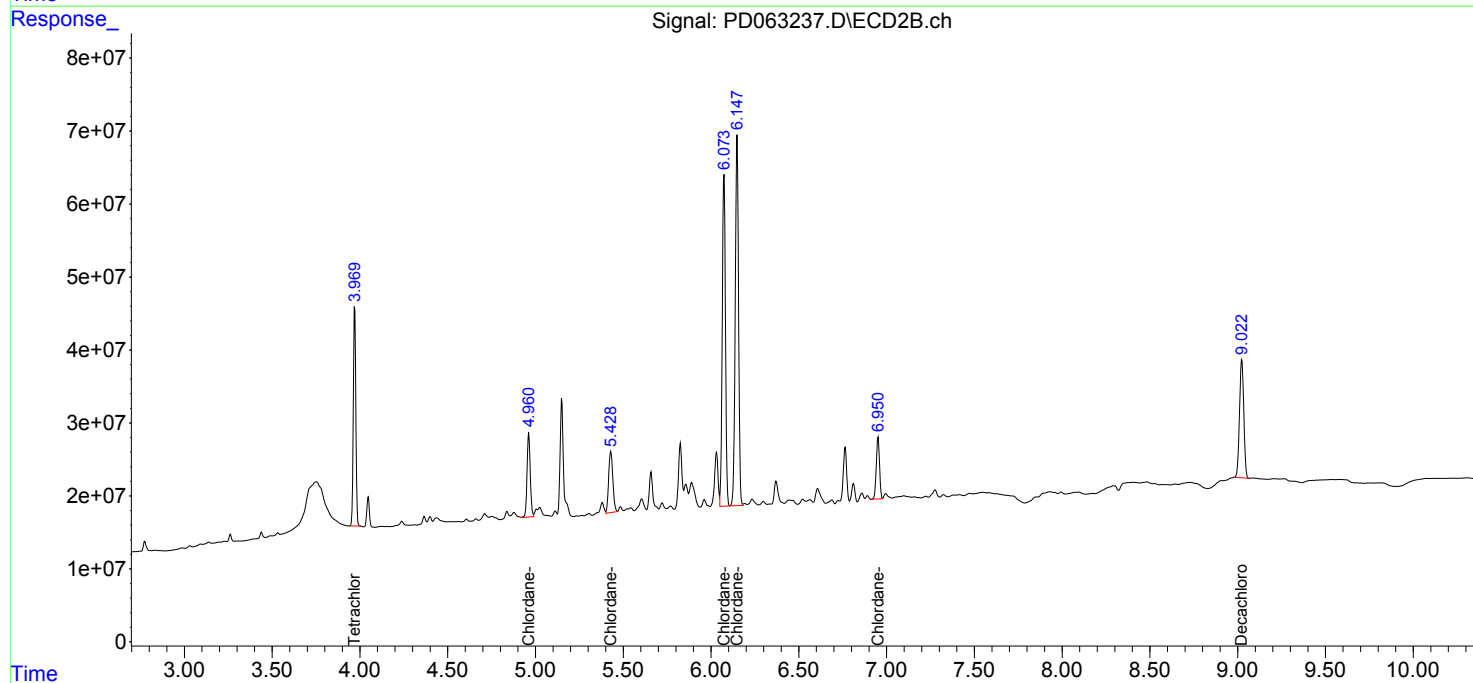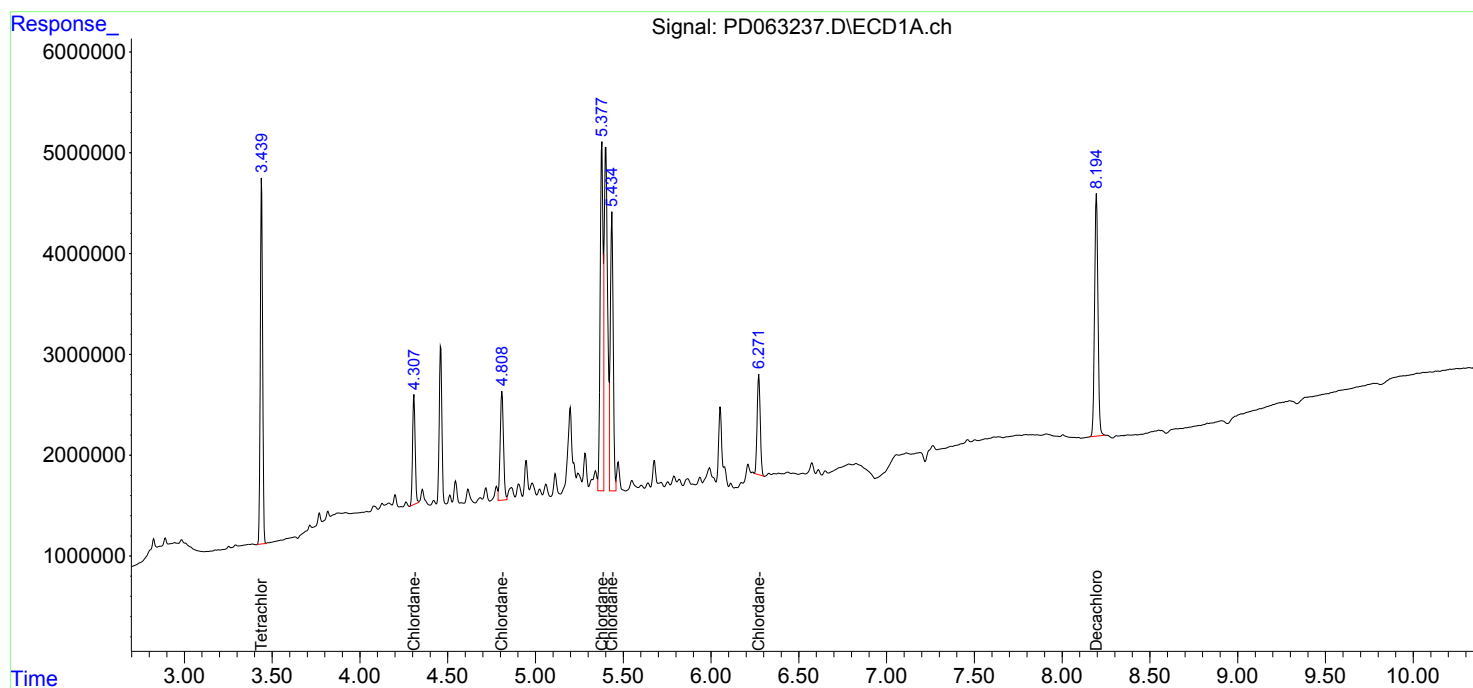


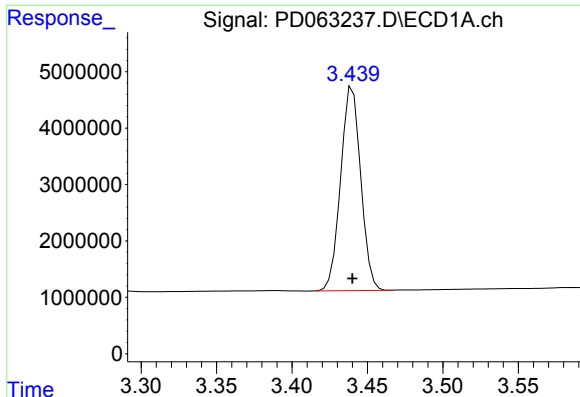

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 33541838
Conc: 24.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

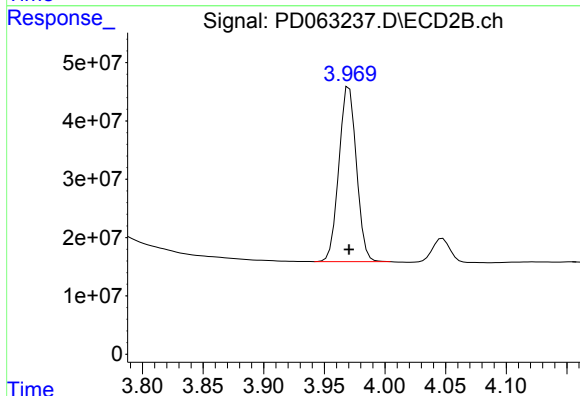


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 301716983
Conc: 26.36 ng/ml

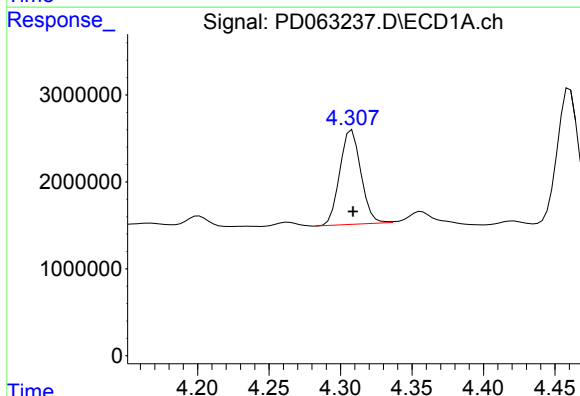


#23 Chlordane-1

R.T.: 4.308 min
Delta R.T.: 0.000 min
Response: 11148562
Conc: 249.30 ng/ml

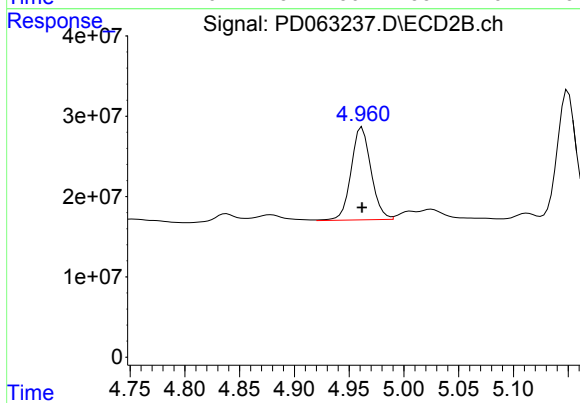

#23 Chlordane-1


R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 145841612
Conc: 266.69 ng/ml

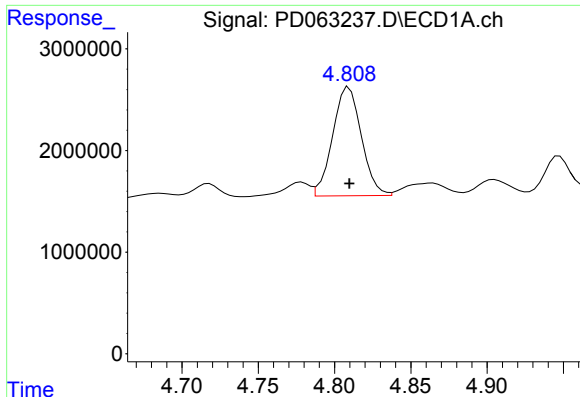

#24 Chlordane-2


R.T.: 4.809 min
Delta R.T.: 0.000 min
Response: 14028785
Conc: 261.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

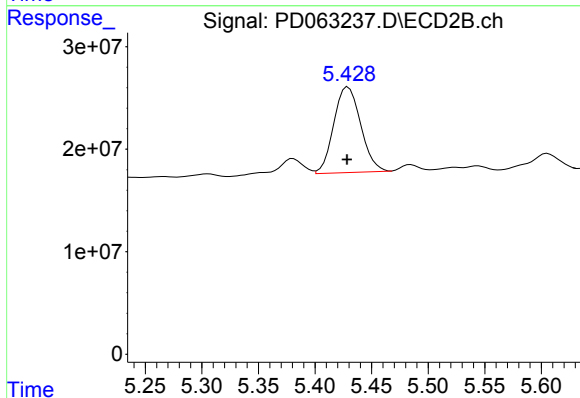


#24 Chlordane-2

R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 138265603
Conc: 267.33 ng/ml

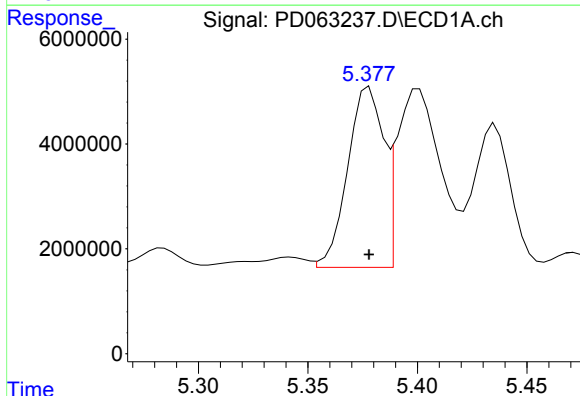


#25 Chlordane-3

R.T.: 5.378 min
Delta R.T.: 0.000 min
Response: 39208229
Conc: 244.96 ng/ml

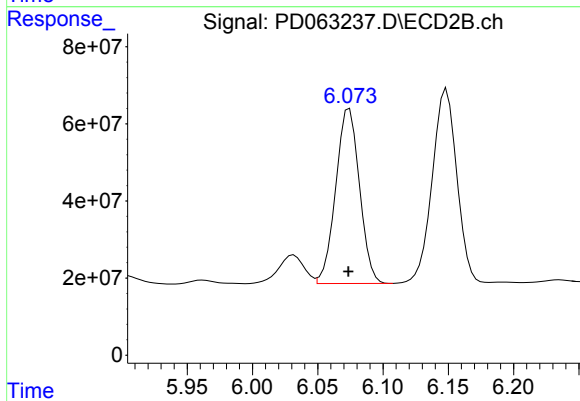

#25 Chlordane-3


R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 575039539
Conc: 263.12 ng/ml

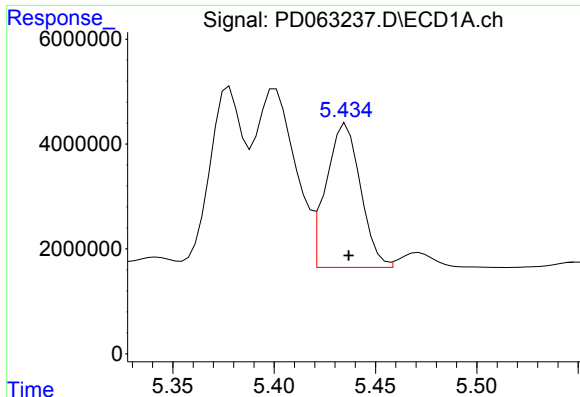

#26 Chlordane-4


R.T.: 5.436 min
Delta R.T.: -0.001 min
Response: 32395931
Conc: 248.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

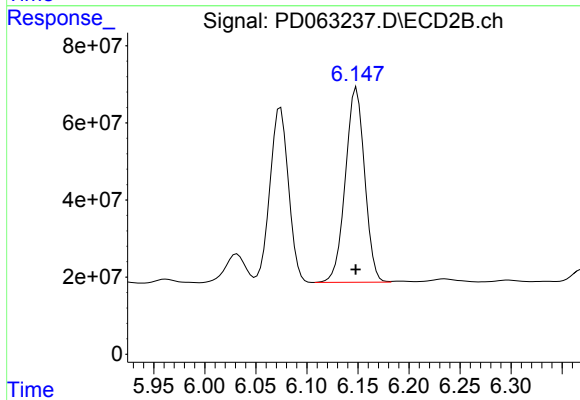


#26 Chlordane-4

R.T.: 6.149 min
Delta R.T.: 0.000 min
Response: 661815945
Conc: 265.36 ng/ml

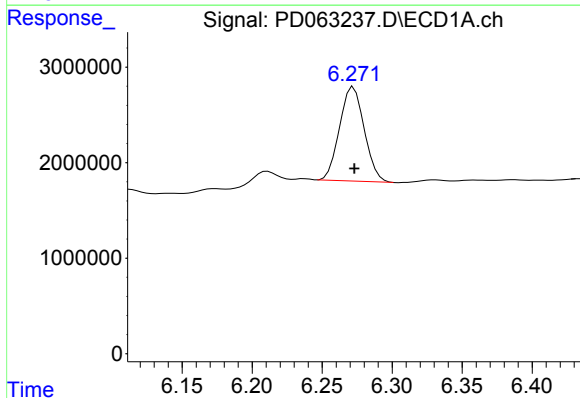


#27 Chlordane-5

R.T.: 6.272 min
Delta R.T.: 0.000 min
Response: 12075597
Conc: 246.19 ng/ml

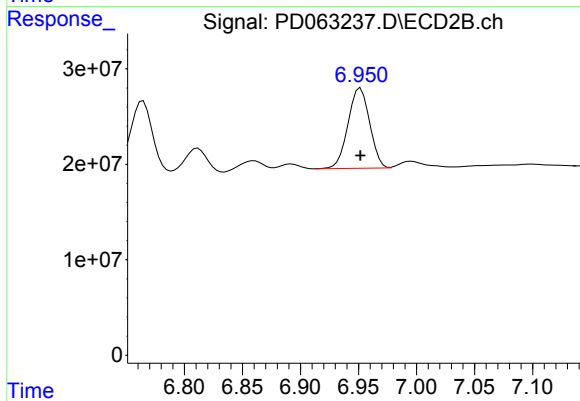

#27 Chlordane-5


R.T.: 6.952 min
Delta R.T.: 0.000 min
Response: 108886994
Conc: 280.70 ng/ml

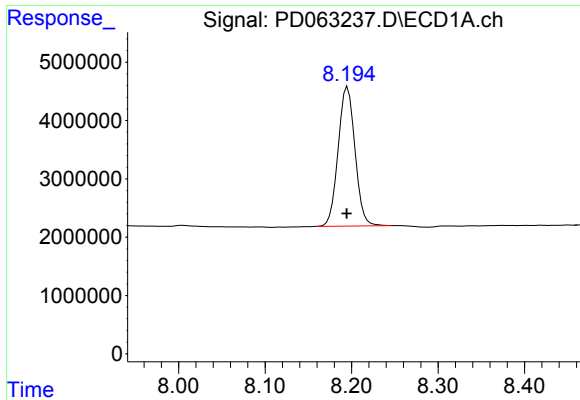

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 32193152
Conc: 26.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

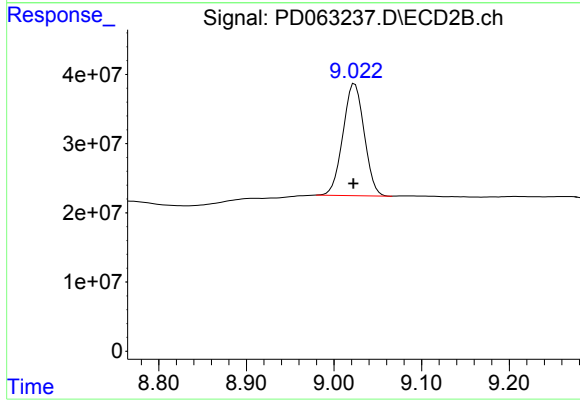

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.001 min
Response: 273142326
Conc: 26.44 ng/ml