

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
 Data File : PD063238.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2021 12:11
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 13:37:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Mon May 24 13:35:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	8190107	75277736	6.002	6.577
28)	SA Decachlor...	8.195	9.024	7905997	68467549	6.604	6.627
Target Compounds							
23)	Chlordane-1	4.308	4.962	2649959	34677616	59.258	63.412
24)	Chlordane-2	4.809	5.428	3420621	36591868	63.700	70.747
25)	Chlordane-3	5.377	6.074	8862157	146.9E6	55.368	67.228
26)	Chlordane-4	5.436	6.148	7306111	169.5E6	56.046	67.947
27)	Chlordane-5	6.273	6.952	2796149	26329800	57.007	67.876



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
Data File : PD063238.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2021 12:11
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 13:37:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Mon May 24 13:35:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

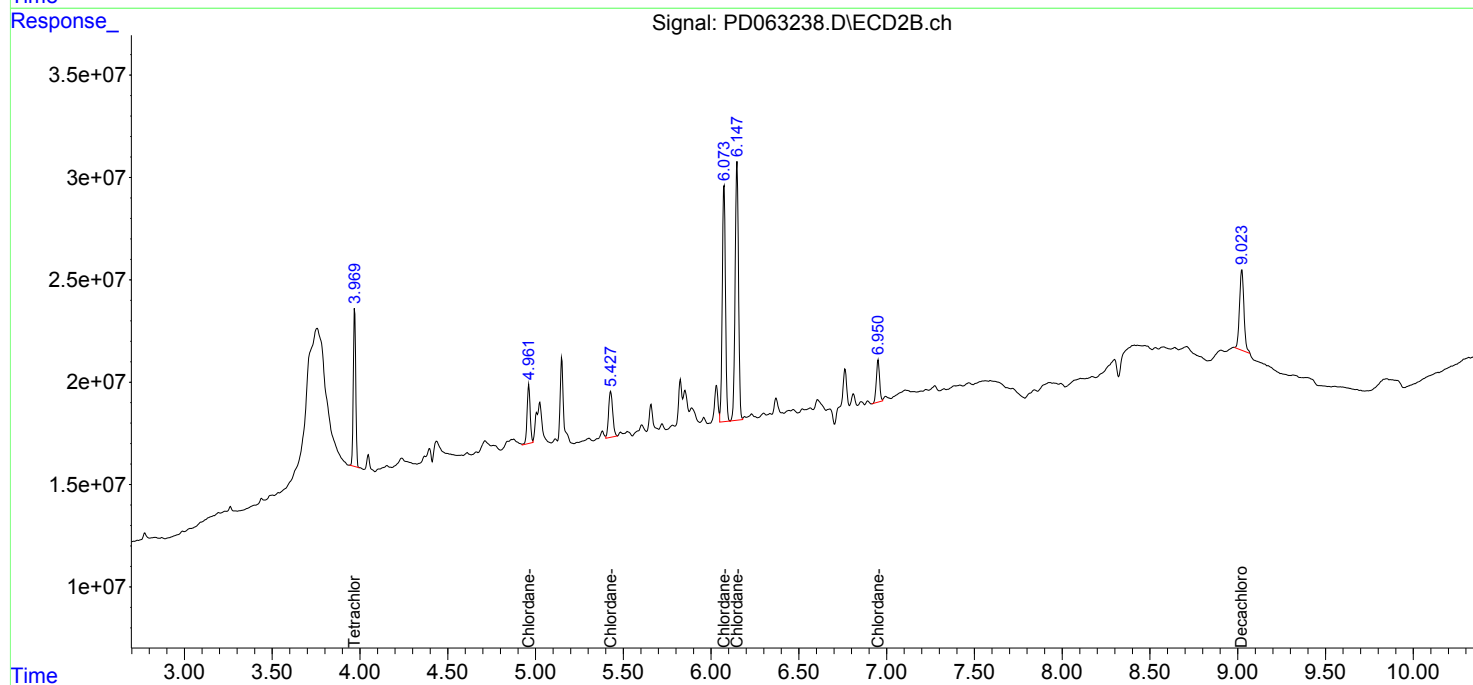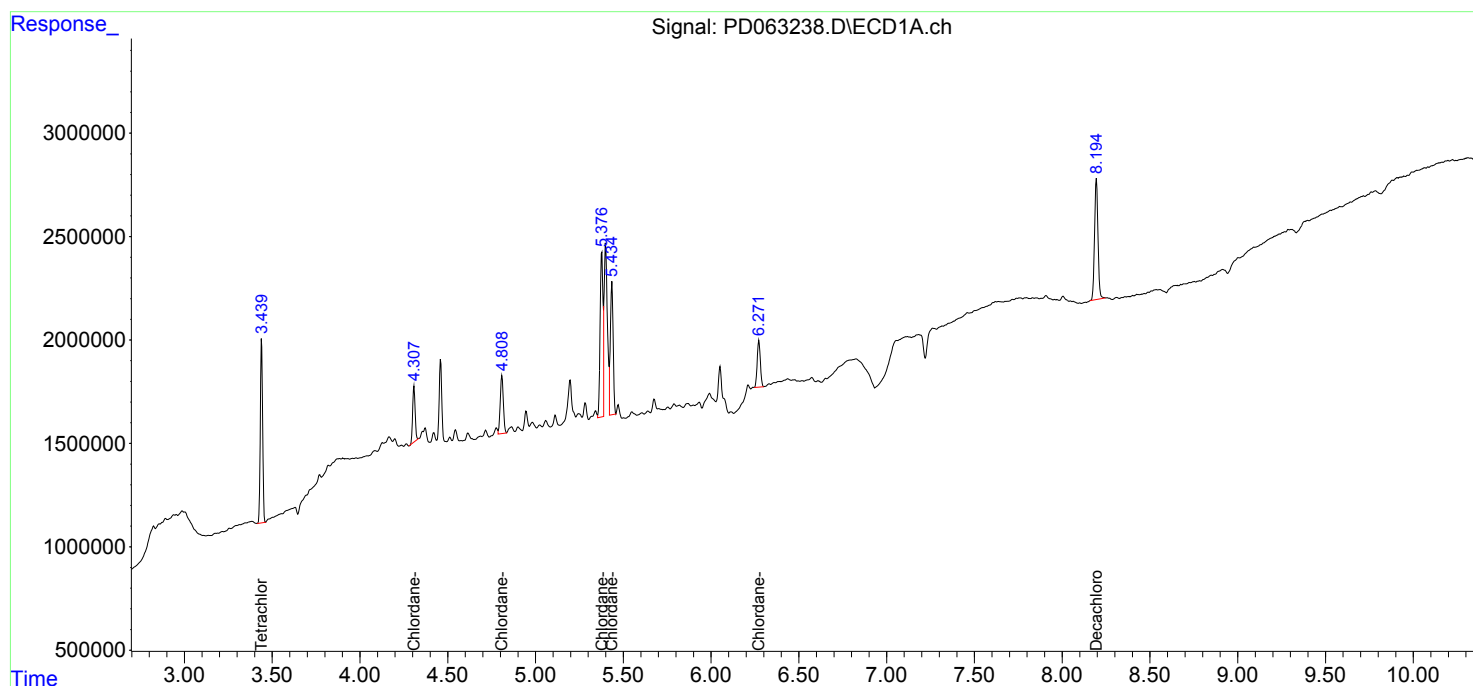


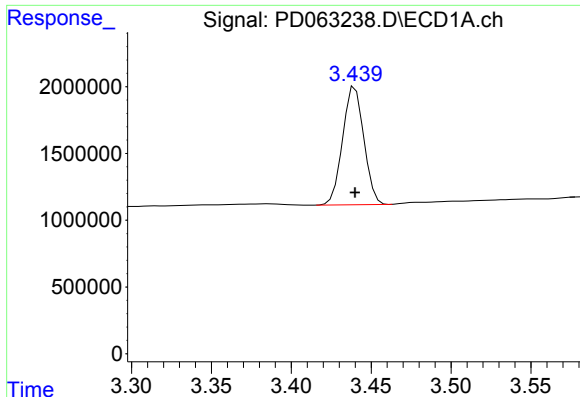

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 8190107
Conc: 6.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

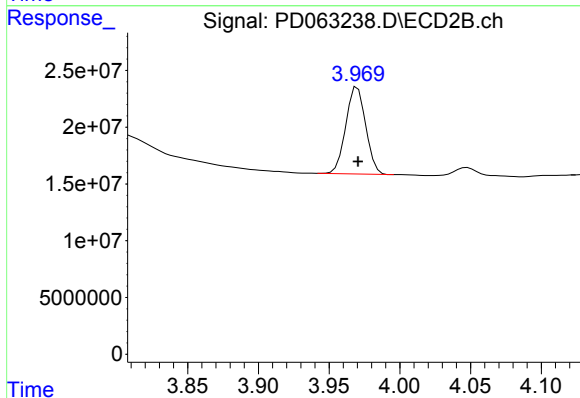


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 75277736
Conc: 6.58 ng/ml

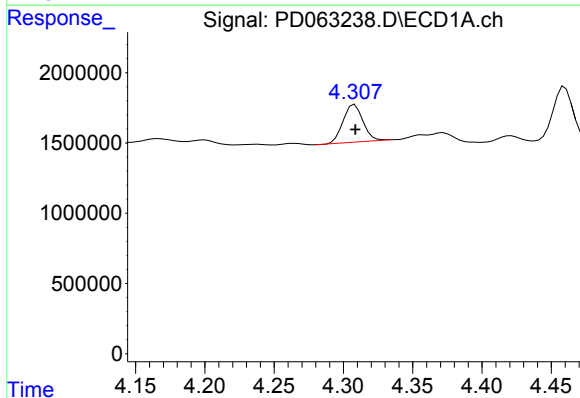


#23 Chlordane-1

R.T.: 4.308 min
Delta R.T.: 0.000 min
Response: 2649959
Conc: 59.26 ng/ml

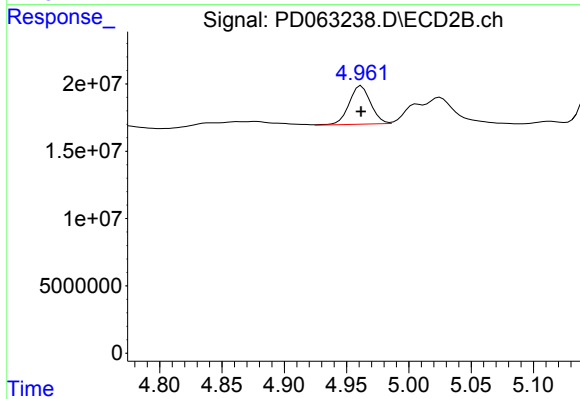

#23 Chlordane-1


R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 34677616
Conc: 63.41 ng/ml

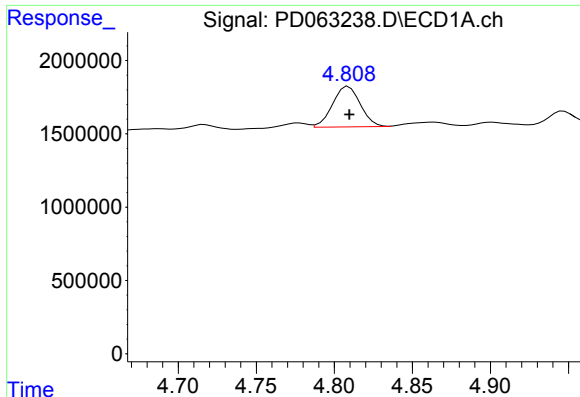

#24 Chlordane-2


R.T.: 4.809 min
Delta R.T.: 0.000 min
Response: 3420621
Conc: 63.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

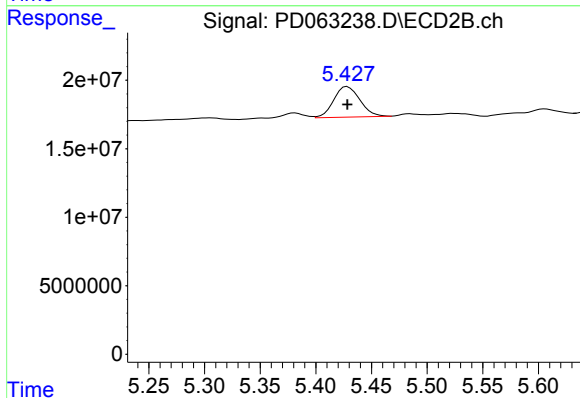


#24 Chlordane-2

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 36591868
Conc: 70.75 ng/ml

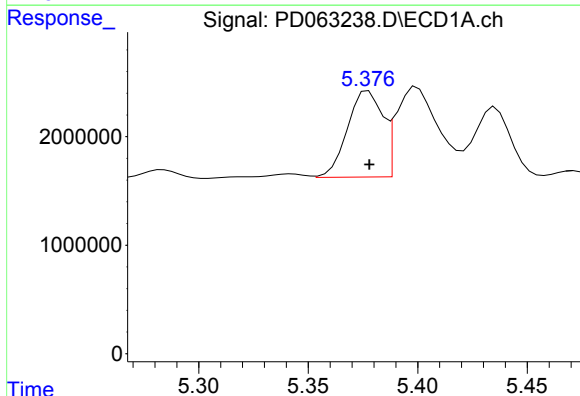


#25 Chlordane-3

R.T.: 5.377 min
Delta R.T.: 0.000 min
Response: 8862157
Conc: 55.37 ng/ml

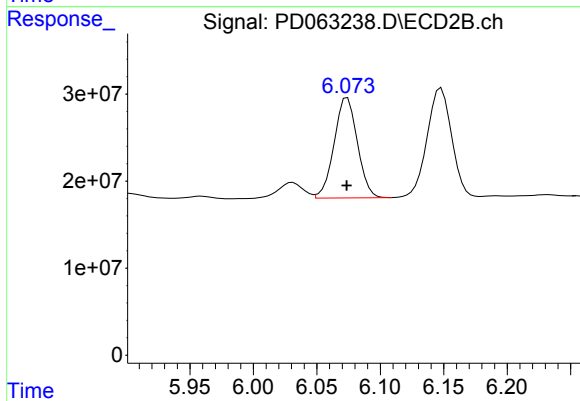

#25 Chlordane-3


R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 146922233
Conc: 67.23 ng/ml

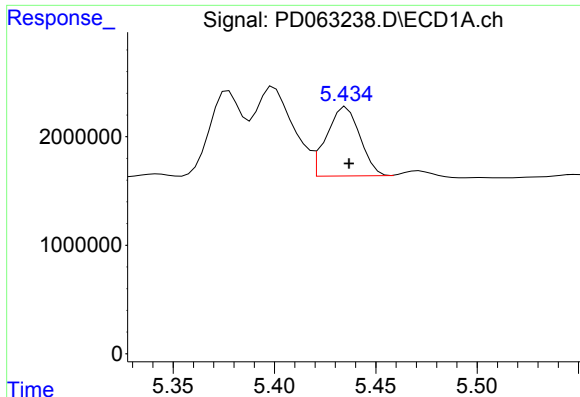

#26 Chlordane-4


R.T.: 5.436 min
Delta R.T.: -0.001 min
Response: 7306111
Conc: 56.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

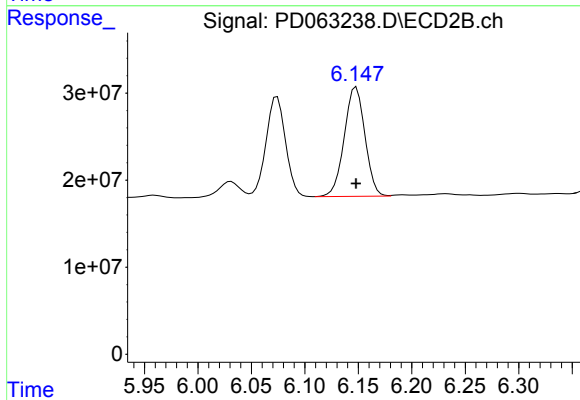


#26 Chlordane-4

R.T.: 6.148 min
Delta R.T.: 0.000 min
Response: 169459361
Conc: 67.95 ng/ml

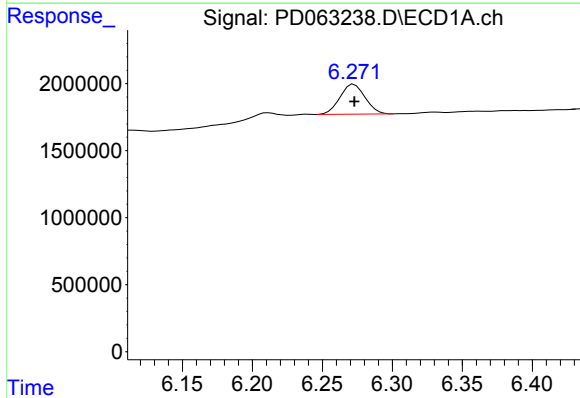


#27 Chlordane-5

R.T.: 6.273 min
Delta R.T.: 0.000 min
Response: 2796149
Conc: 57.01 ng/ml

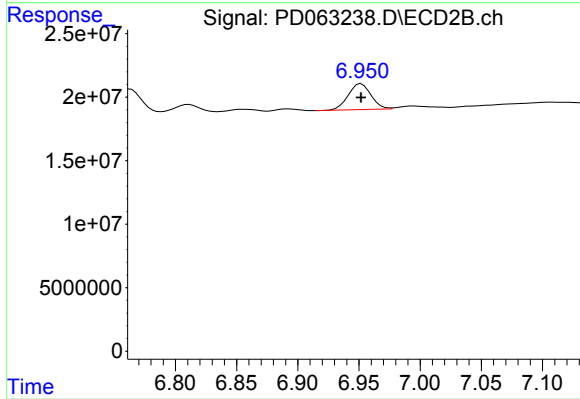

#27 Chlordane-5


R.T.: 6.952 min
Delta R.T.: 0.000 min
Response: 26329800
Conc: 67.88 ng/ml

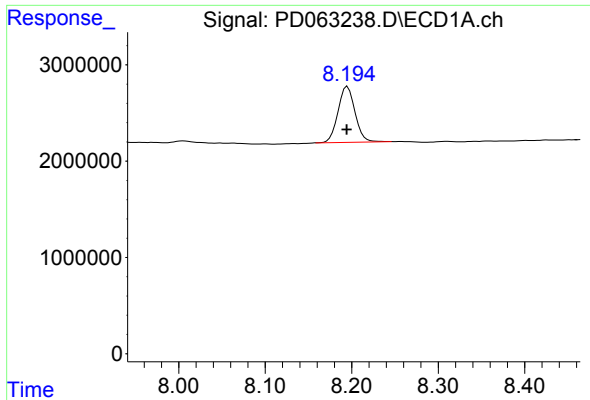

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 7905997
Conc: 6.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

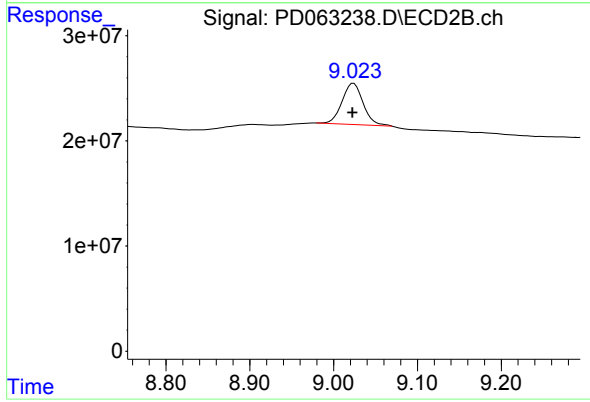

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.002 min
Response: 68467549
Conc: 6.63 ng/ml