

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
 Data File : PD063244.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2021 14:24
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD052421

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 14:41:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Mon May 24 13:43:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	67067601	568.3E6	46.753	46.482
28)	SA Decachlor...	8.196	9.024	62625311	532.0E6	48.203	48.048
Target Compounds							
23)	Chlordane-1	4.308	4.962	22089409	273.5E6	474.403	471.582
24)	Chlordane-2	4.810	5.429	26719359	260.8E6	469.978	461.009
25)	Chlordane-3	5.378	6.074	78991098	1115.9E6	479.139	472.472
26)	Chlordane-4	5.436	6.148	64801288	1278.2E6	479.440	472.667
27)	Chlordane-5	6.273	6.952	23898594	226.1E6	479.381	505.936



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
Data File : PD063244.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2021 14:24
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD052421

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 14:41:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Mon May 24 13:43:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

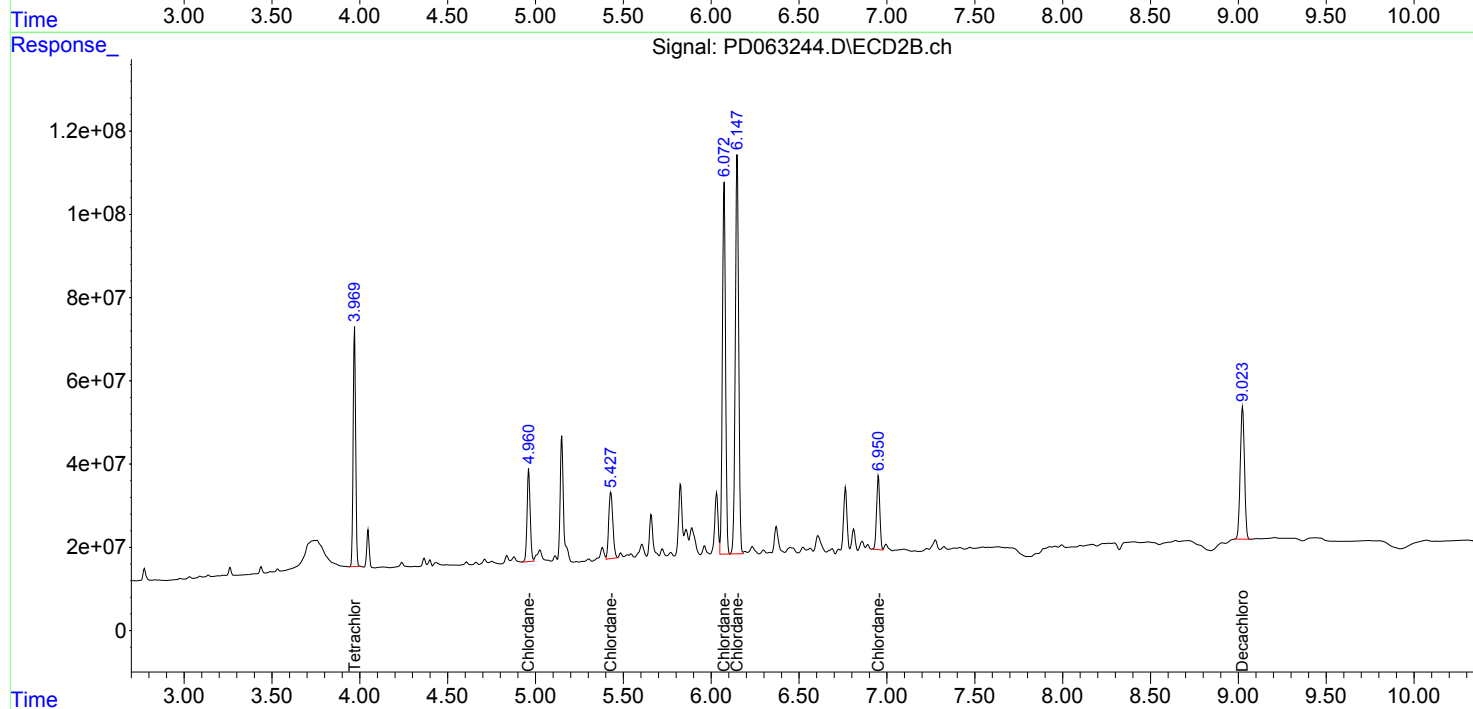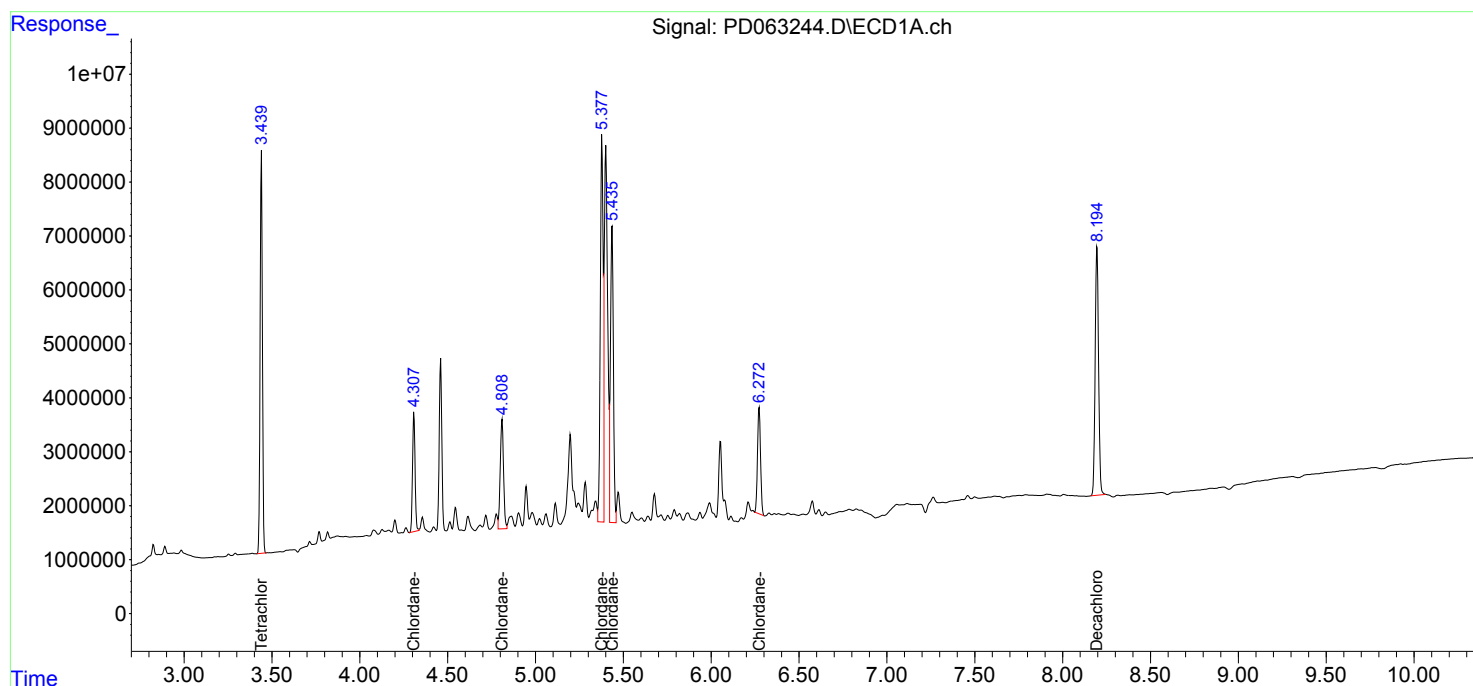


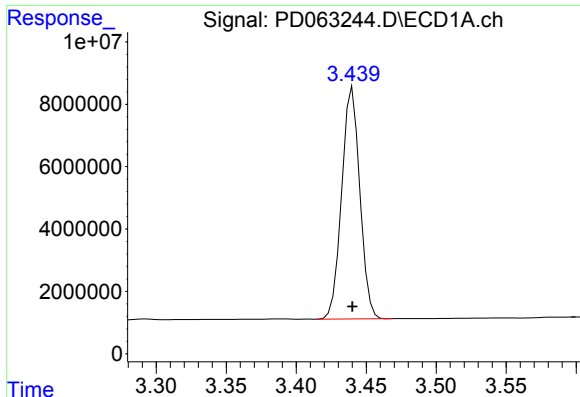

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 67067601
Conc: 46.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD052421

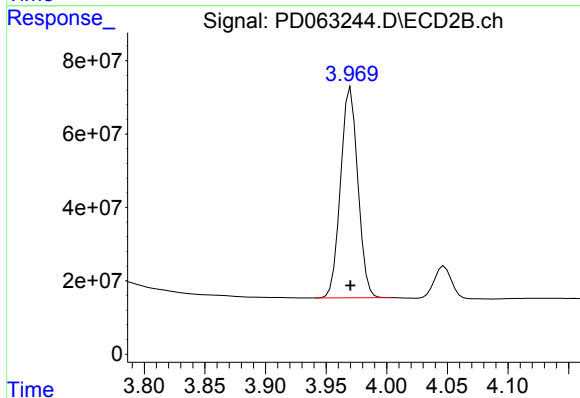


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 568300495
Conc: 46.48 ng/ml

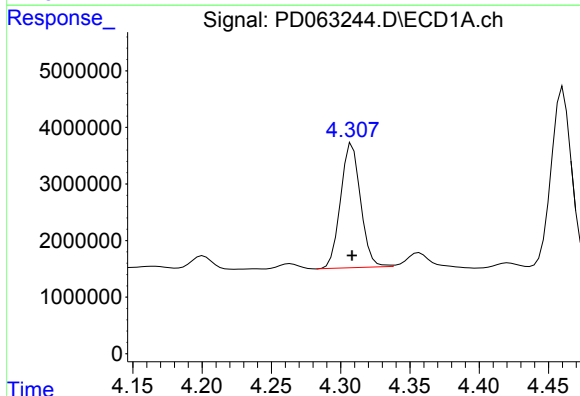


#23 Chlordane-1

R.T.: 4.308 min
Delta R.T.: 0.000 min
Response: 22089409
Conc: 474.40 ng/ml

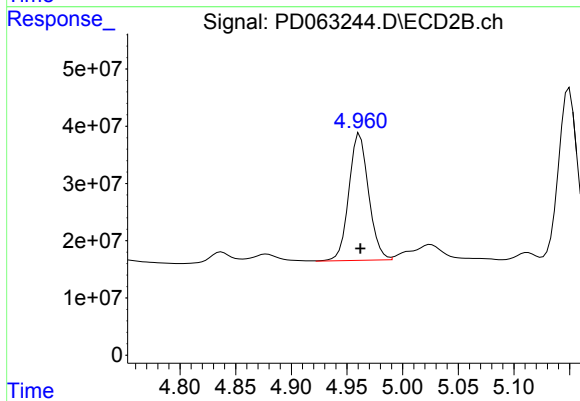

#23 Chlordane-1


R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 273545281
Conc: 471.58 ng/ml

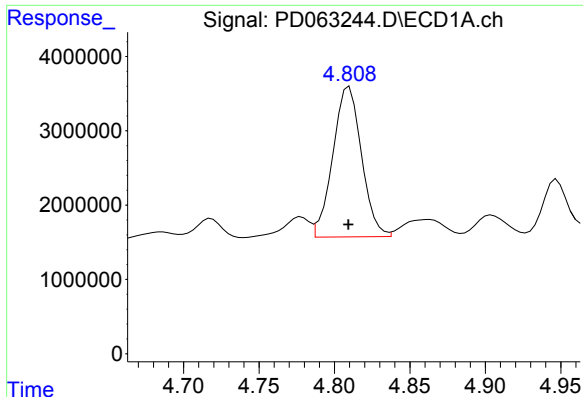

#24 Chlordane-2


R.T.: 4.810 min
Delta R.T.: 0.000 min
Response: 26719359
Conc: 469.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD052421

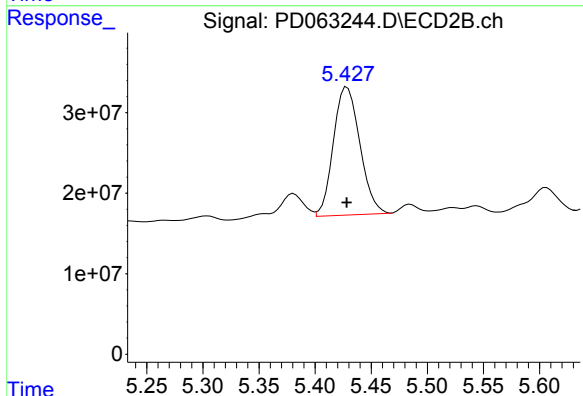


#24 Chlordane-2

R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 260773367
Conc: 461.01 ng/ml

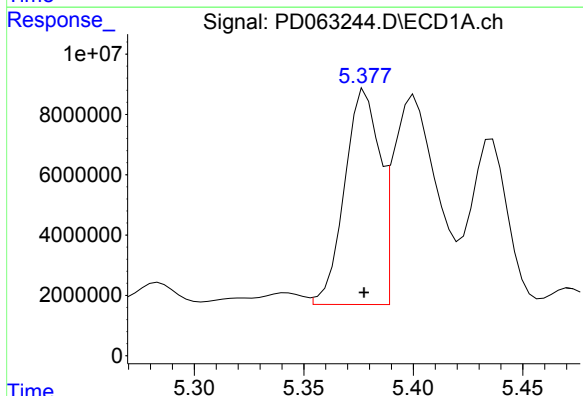


#25 Chlordane-3

R.T.: 5.378 min
Delta R.T.: 0.000 min
Response: 78991098
Conc: 479.14 ng/ml

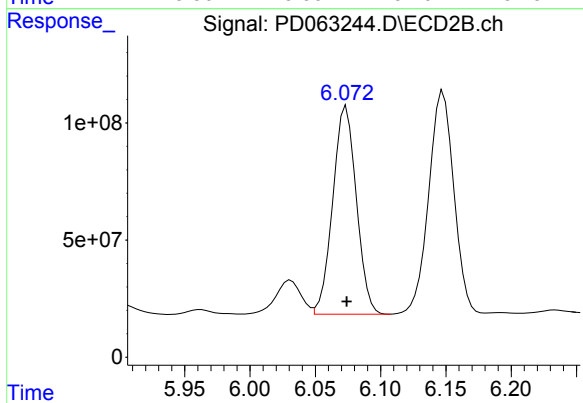

#25 Chlordane-3


R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 1115870211
Conc: 472.47 ng/ml

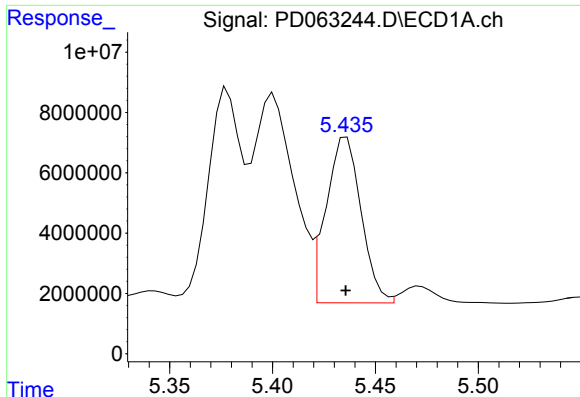

#26 Chlordane-4


R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 64801288
Conc: 479.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD052421

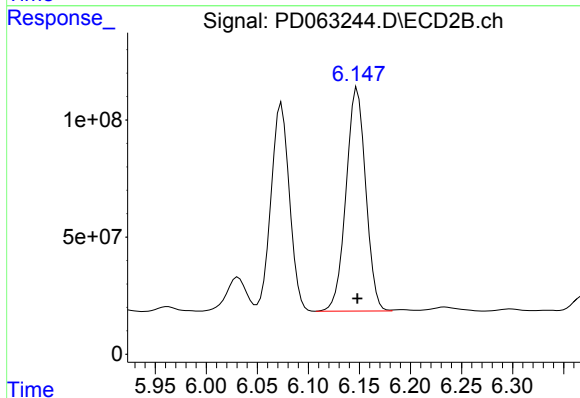


#26 Chlordane-4

R.T.: 6.148 min
Delta R.T.: 0.000 min
Response: 1278219300
Conc: 472.67 ng/ml

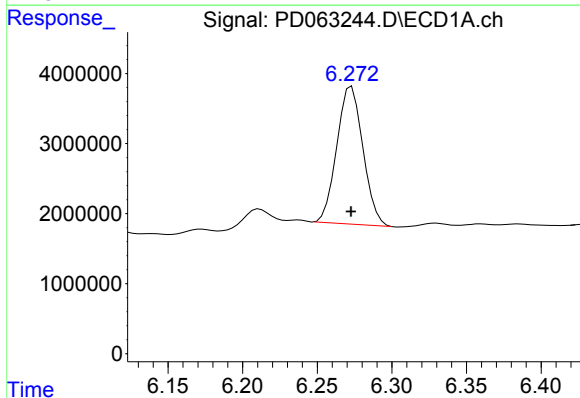


#27 Chlordane-5

R.T.: 6.273 min
Delta R.T.: 0.000 min
Response: 23898594
Conc: 479.38 ng/ml

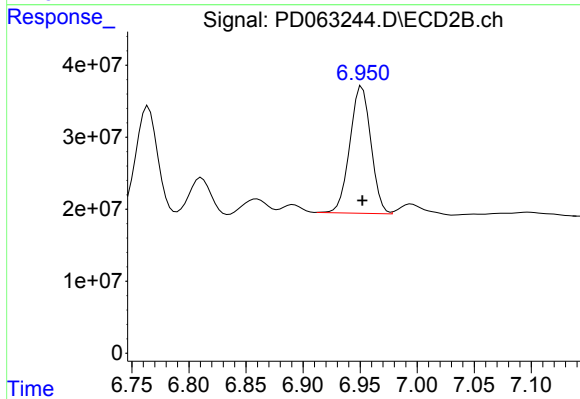

#27 Chlordane-5


R.T.: 6.952 min
Delta R.T.: 0.000 min
Response: 226143578
Conc: 505.94 ng/ml

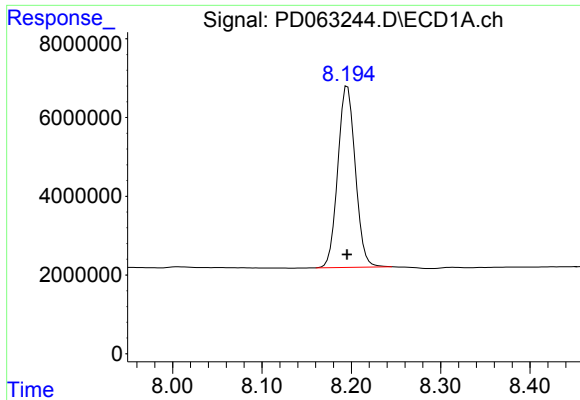

#28 Decachlorobiphenyl

R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 62625311
Conc: 48.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD052421

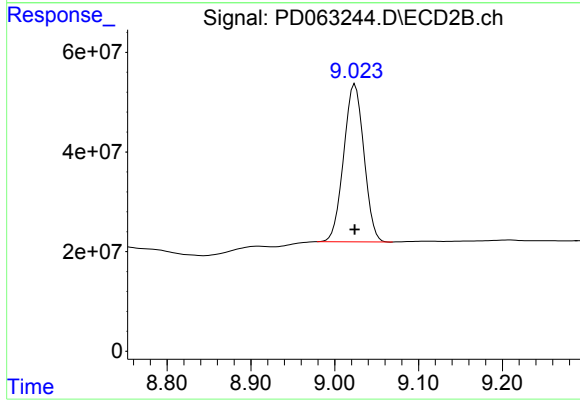

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 532022241
Conc: 48.05 ng/ml