

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
 Data File : PD063253.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2021 17:50
 Operator : AR\AJ
 Sample : M2490-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 72-11986

Manual Integrations
 APPROVED

Ankita
 5/25/2021 4:06:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 01:25:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Mon May 24 14:48:18 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.971	15635838	163.5E6	14.195	14.110
28)	SA Decachlor...	8.194	9.024	18929803	160.6E6	15.041m	15.744
Target Compounds							
17)	MA 4,4'-DDT	6.355	7.091	786102	5959933	0.688	0.529m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052421\
Data File : PD063253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2021 17:50
Operator : AR\AJ
Sample : M2490-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
72-11986


Manual Integrations
APPROVED

Ankita
5/25/2021 4:06:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 01:25:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Mon May 24 14:48:18 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

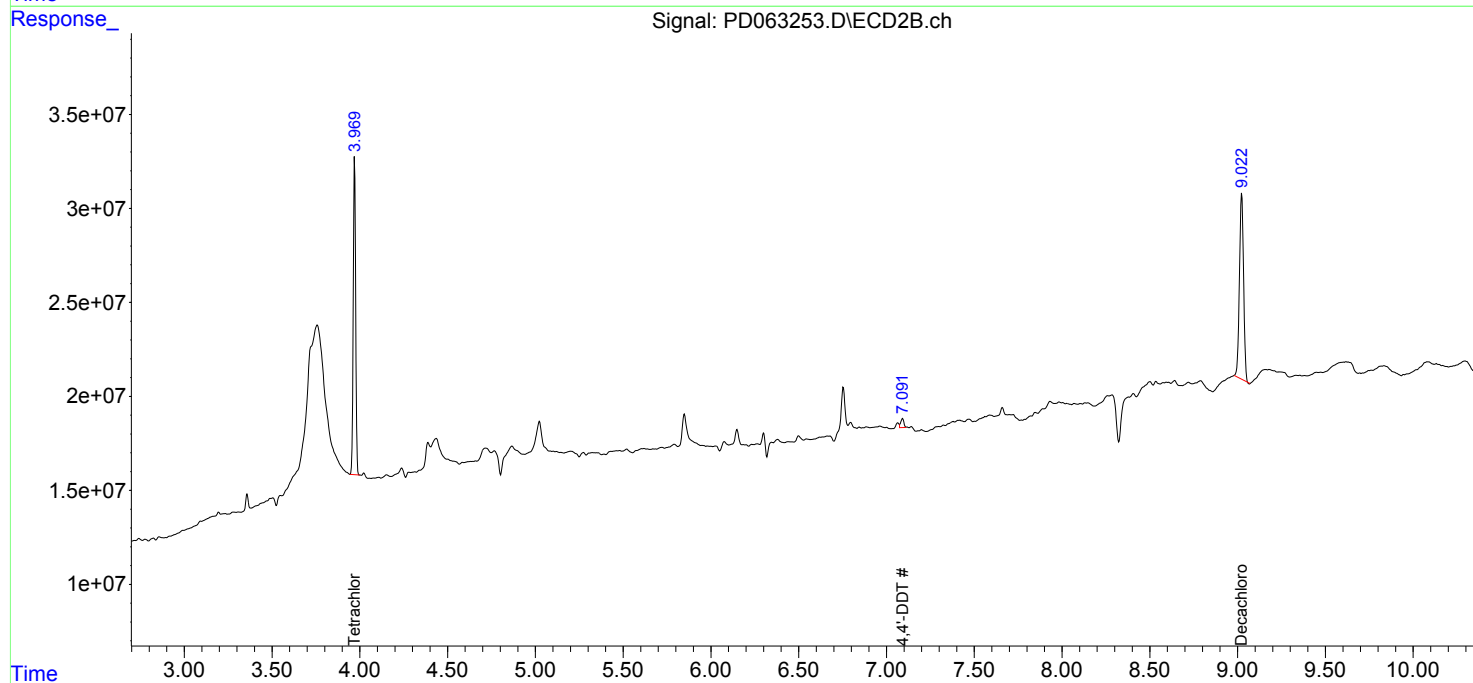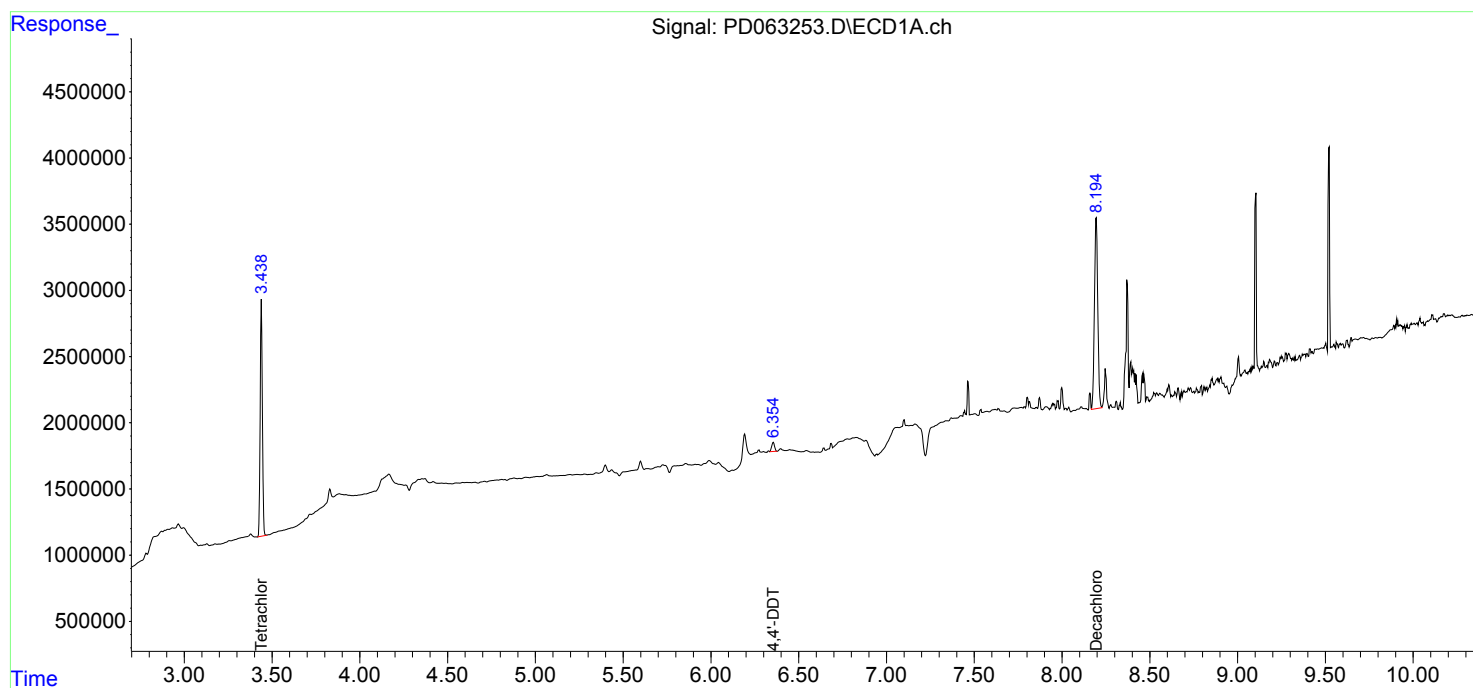

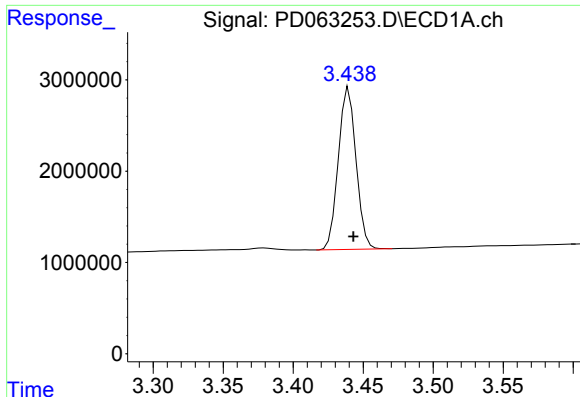


#1 Tetrachloro-m-xylene

R.T.: 3.440 min
Delta R.T.: -0.003 min
Response: 15635838
Conc: 14.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
72-11986


Manual Integrations
APPROVED

Ankita
5/25/2021 4:06:04 PM

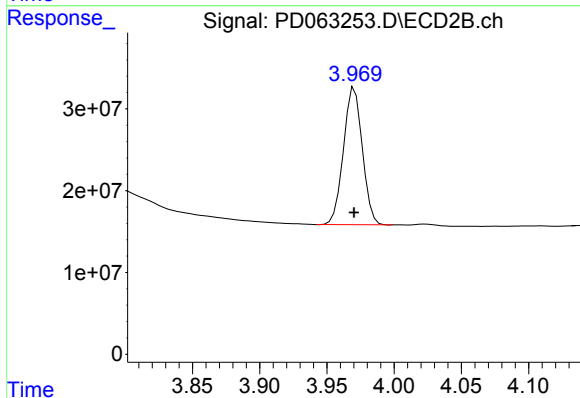


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 163506078
Conc: 14.11 ng/ml

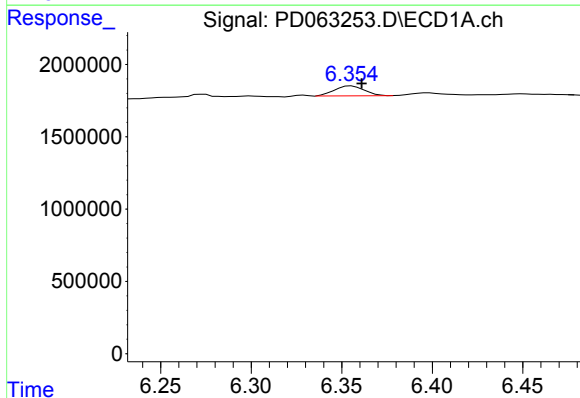


#17 4,4'-DDT

R.T.: 6.355 min
Delta R.T.: -0.006 min
Response: 786102
Conc: 0.69 ng/ml

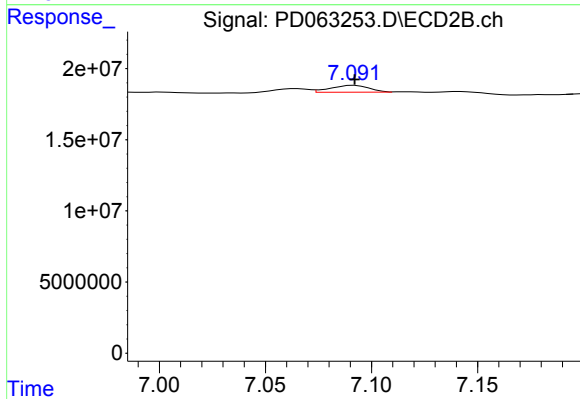

#17 4,4'-DDT

R.T.: 7.091 min
Delta R.T.: -0.002 min
Response: 5959933
Conc: 0.53 ng/ml m

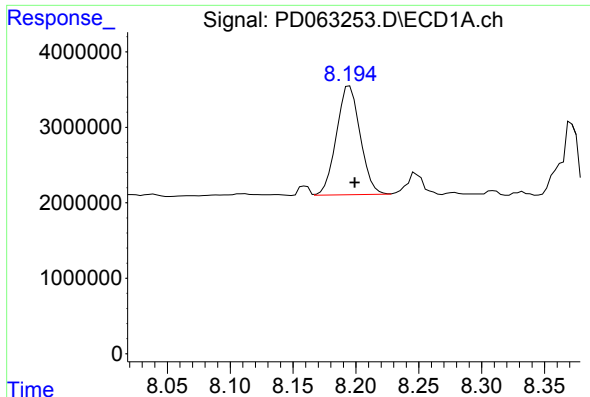


#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: -0.005 min
Response: 18929803
Conc: 15.04 ng/ml m

Instrument :
ECD_D
ClientSampleId :
72-11986

Manual Integrations
APPROVED

Ankita
5/25/2021 4:06:04 PM

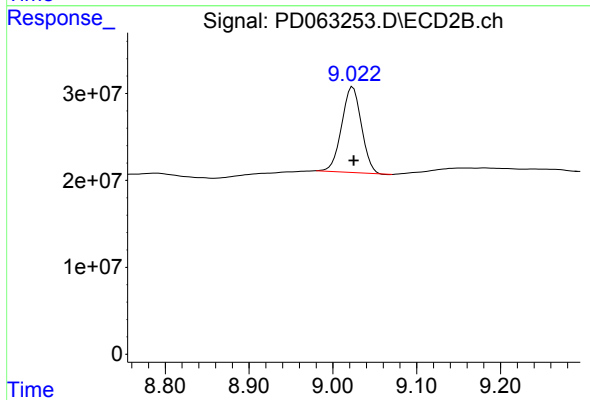

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: -0.001 min
Response: 160617008
Conc: 15.74 ng/ml