

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052422\
 Data File : PD069803.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2022 21:15
 Operator : AR\AJ
 Sample : N2894-17
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P008-SS002-1824-01

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/24/2022
 Supervised By : Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 02:43:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Mon May 23 02:08:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	4.169	20335351	189.3E6	20.293	19.815m
28)	SA Decachlor...	8.194	9.363	14089960	99016125	13.063	16.522m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052422\
Data File : PD069803.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2022 21:15
Operator : AR\AJ
Sample : N2894-17
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
P008-SS002-1824-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/24/2022
Supervised By : Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 02:43:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Mon May 23 02:08:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

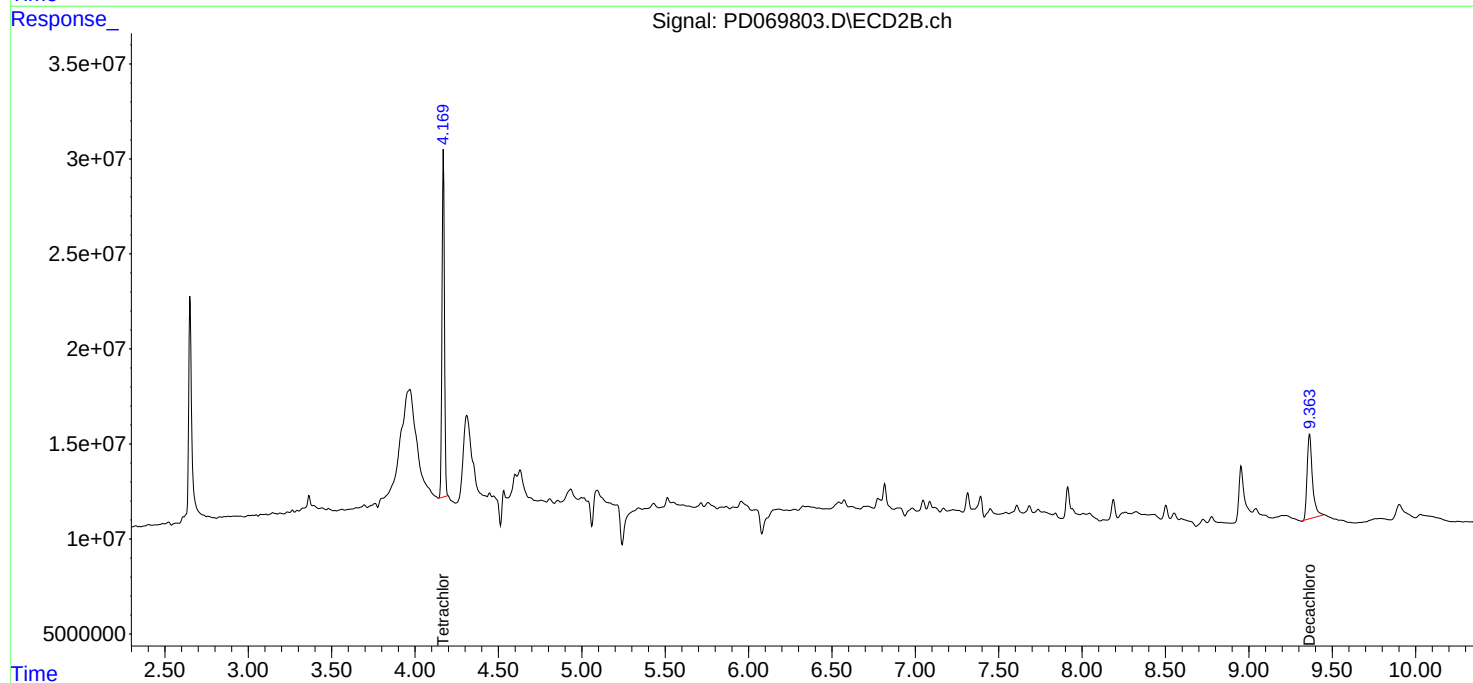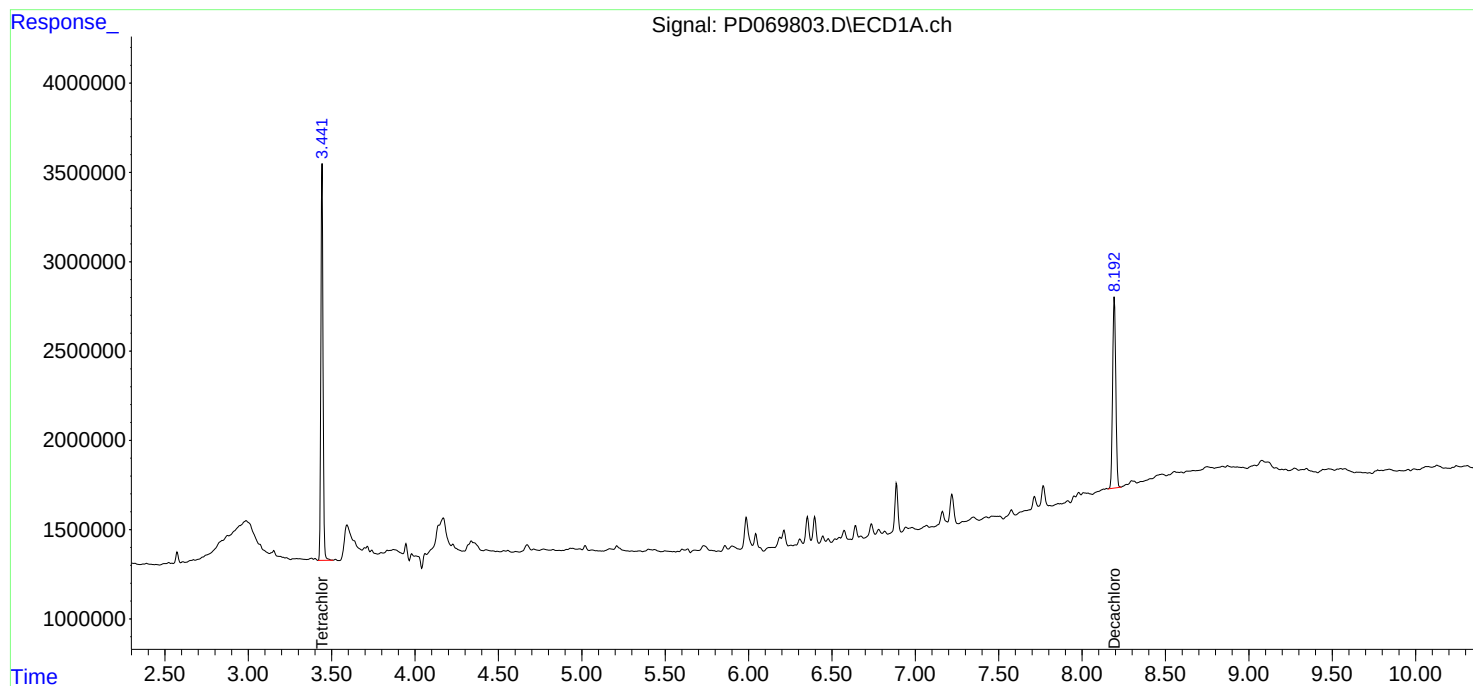

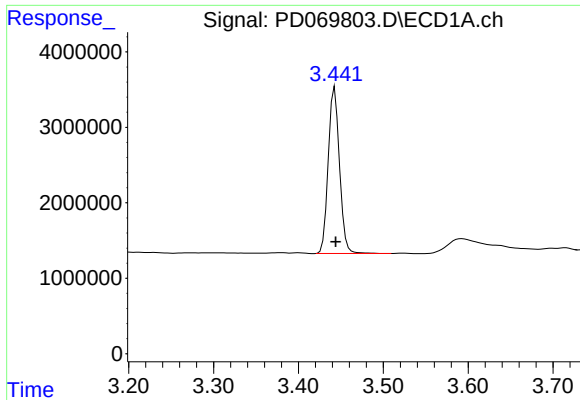


#1 Tetrachloro-m-xylene

R.T.: 3.443 min
Delta R.T.: -0.001 min
Response: 20335351
Conc: 20.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
P008-SS002-1824-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/24/2022
Supervised By :Ankita Jodhani 05/24/2022

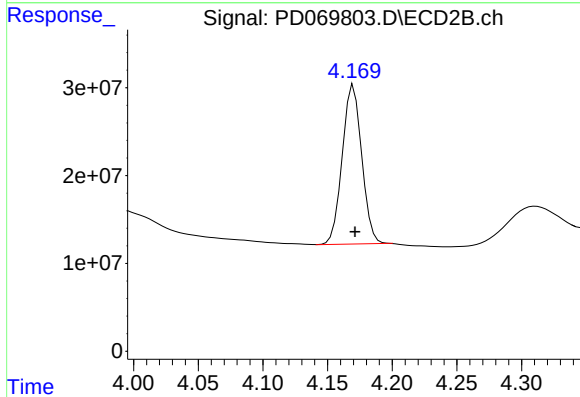


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: -0.003 min
Response: 189309892
Conc: 19.81 ng/ml m

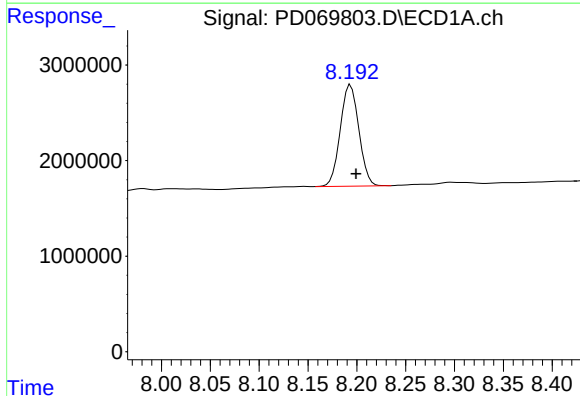

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: -0.006 min
Response: 14089960
Conc: 13.06 ng/ml

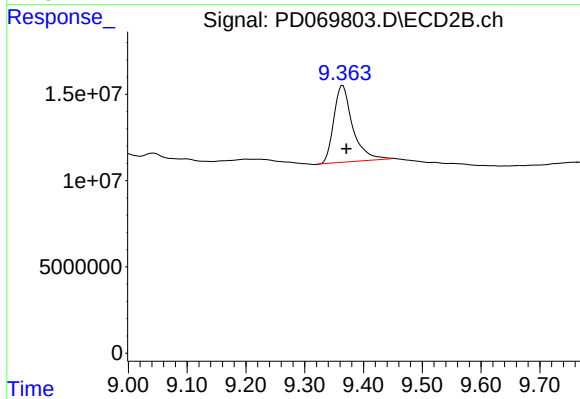

#28 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: -0.007 min
Response: 99016125
Conc: 16.52 ng/ml m