

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052422\
 Data File : PD069805.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2022 21:43
 Operator : AR\AJ
 Sample : N2894-19
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P008-SS003-0006-01

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/24/2022
 Supervised By :Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 02:44:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Mon May 23 02:08:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.443	4.169	21042323	196.4E6	20.999	20.560m
2) SA Decachlor...	8.194	9.363	33351790	199.2E6	30.920	33.239
Target Compounds						
12) B 4,4'-DDE	5.602	6.545	1409262	16128965	1.218	1.625m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052422\
Data File : PD069805.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2022 21:43
Operator : AR\AJ
Sample : N2894-19
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
P008-SS003-0006-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/24/2022
Supervised By :Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 02:44:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Mon May 23 02:08:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

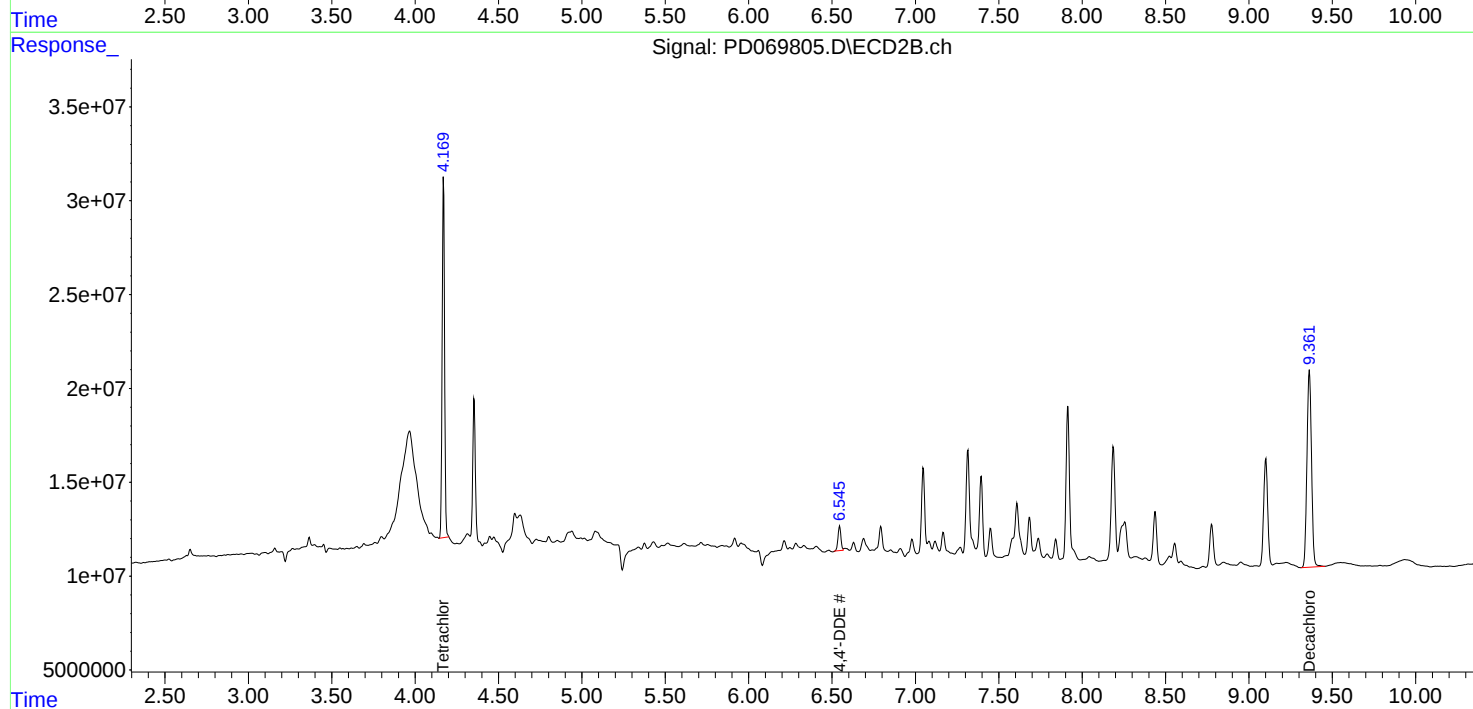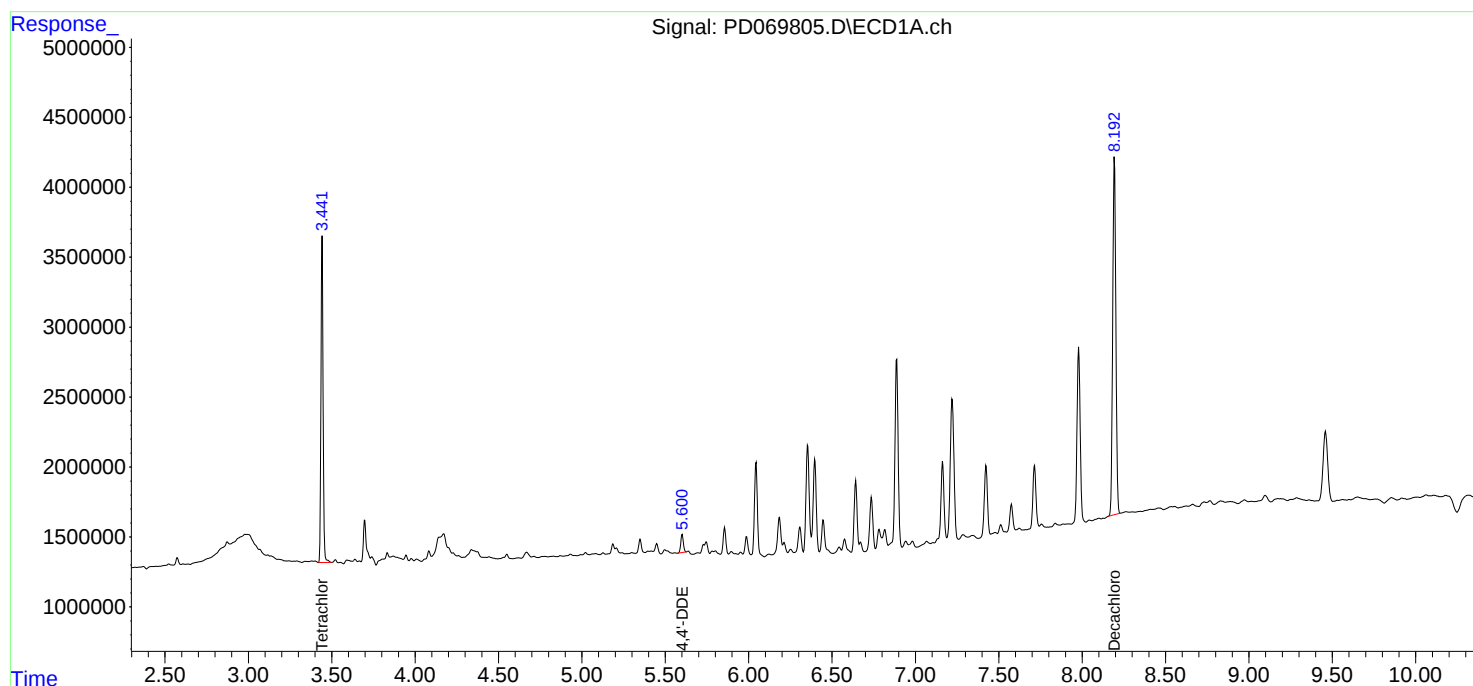

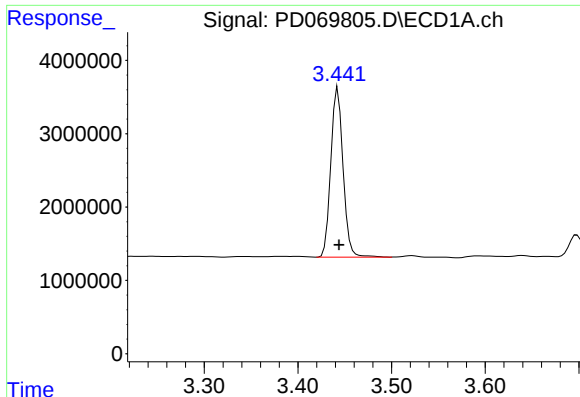


#1 Tetrachloro-m-xylene

R.T.: 3.443 min
Delta R.T.: -0.001 min
Response: 21042323
Conc: 21.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
P008-SS003-0006-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/24/2022
Supervised By :Ankita Jodhani 05/24/2022

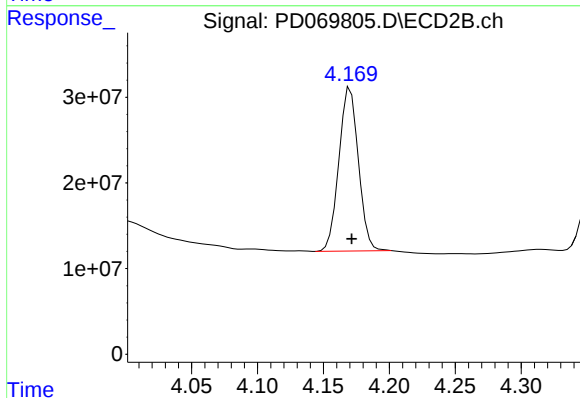


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: -0.002 min
Response: 196429004
Conc: 20.56 ng/ml m

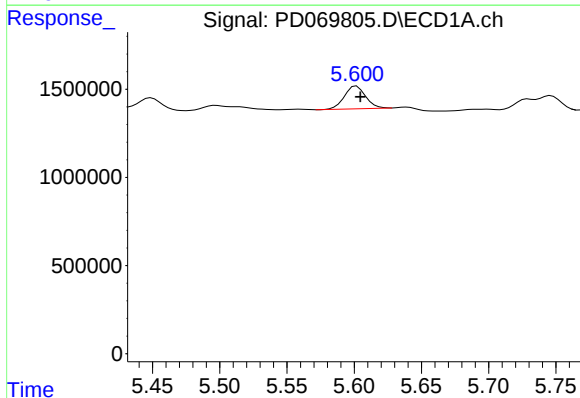


#12 4,4'-DDE

R.T.: 5.602 min
Delta R.T.: -0.003 min
Response: 1409262
Conc: 1.22 ng/ml

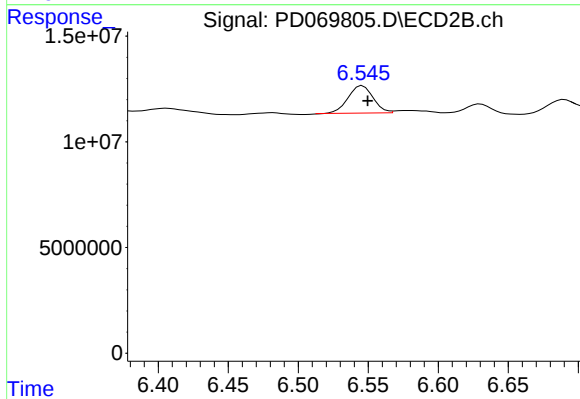

#12 4,4'-DDE

R.T.: 6.545 min
Delta R.T.: -0.005 min
Response: 16128965
Conc: 1.62 ng/ml m

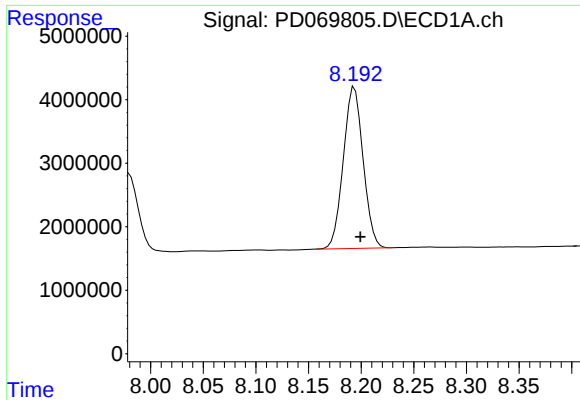


#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: -0.006 min
Response: 33351790
Conc: 30.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
P008-SS003-0006-01

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/24/2022
Supervised By :Ankita Jodhani 05/24/2022

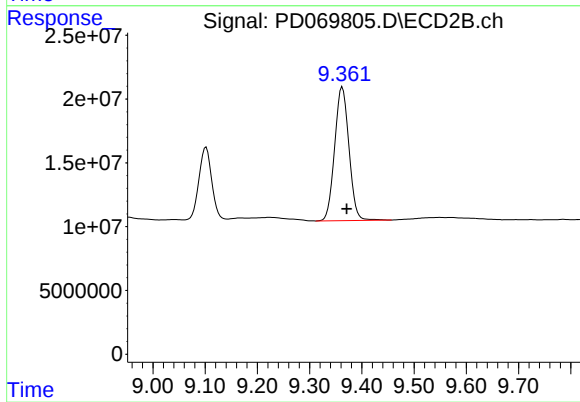

#28 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: -0.008 min
Response: 199196730
Conc: 33.24 ng/ml