

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052422\
 Data File : PD069806.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2022 21:57
 Operator : AR\AJ
 Sample : N2895-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P030-SS001-0006-01

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/24/2022
 Supervised By :Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 02:44:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Mon May 23 02:08:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.168	10314434	102.9E6	10.293	10.767m
28)	SA Decachlor...	8.195	9.361	13423629	76931203	12.445	12.837m
Target Compounds							
12)	B 4,4'-DDE	5.600	6.545	495796	6481447	0.428m	0.653m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052422\
Data File : PD069806.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2022 21:57
Operator : AR\AJ
Sample : N2895-05
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
P030-SS001-0006-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/24/2022
Supervised By : Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 02:44:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Mon May 23 02:08:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

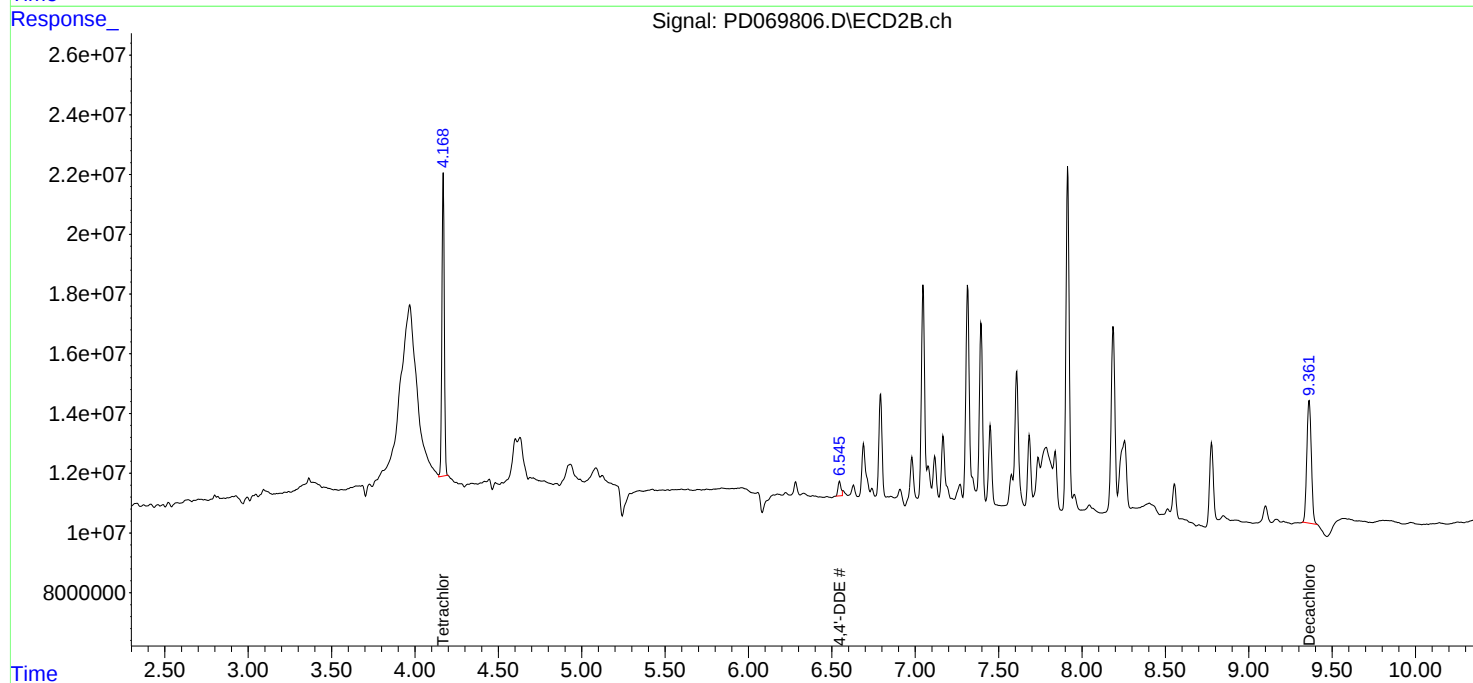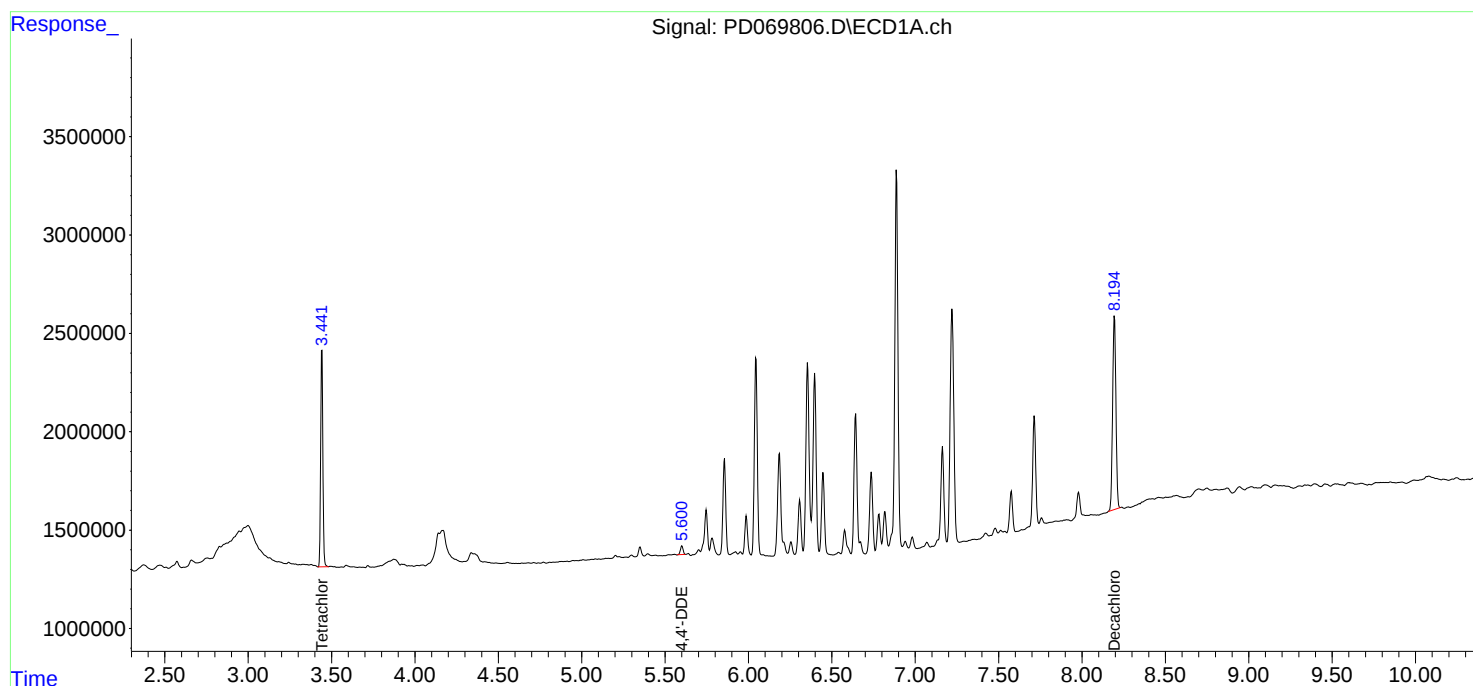

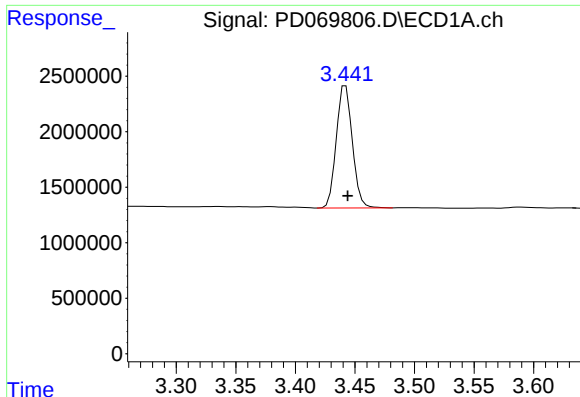


#1 Tetrachloro-m-xylene

R.T.: 3.442 min
Delta R.T.: -0.002 min
Response: 10314434
Conc: 10.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
P030-SS001-0006-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/24/2022
Supervised By :Ankita Jodhani 05/24/2022

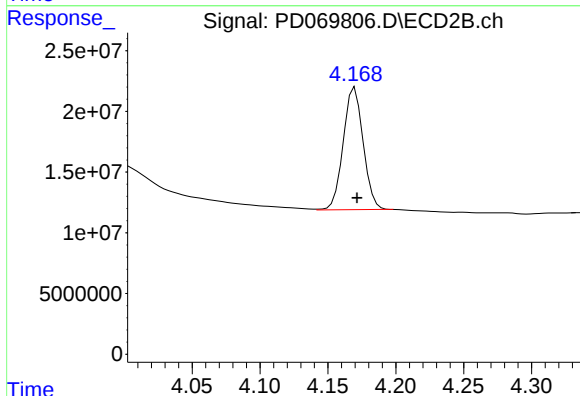


#1 Tetrachloro-m-xylene

R.T.: 4.168 min
Delta R.T.: -0.003 min
Response: 102866958
Conc: 10.77 ng/ml m

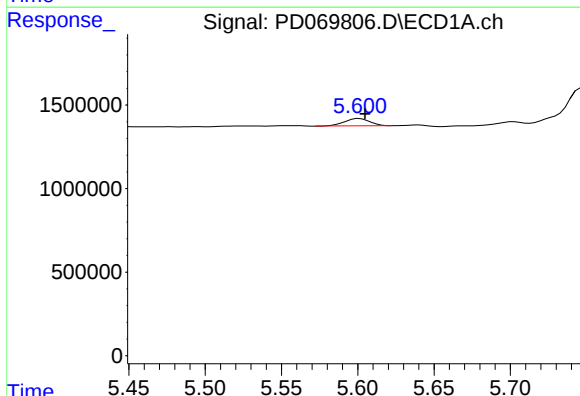


#12 4,4'-DDE

R.T.: 5.600 min
Delta R.T.: -0.005 min
Response: 495796
Conc: 0.43 ng/ml m

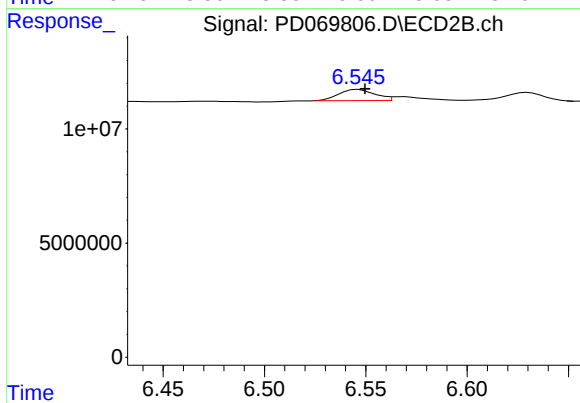

#12 4,4'-DDE

R.T.: 6.545 min
Delta R.T.: -0.005 min
Response: 6481447
Conc: 0.65 ng/ml m

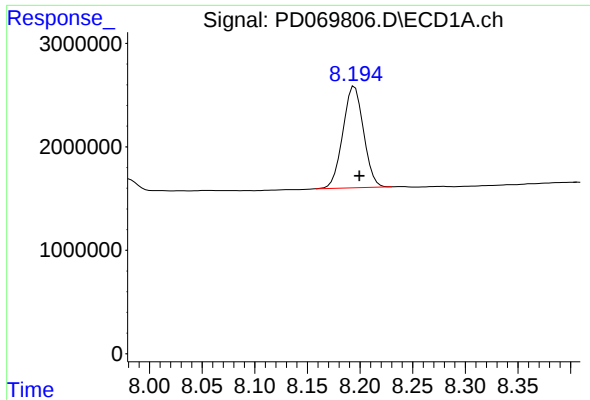


#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: -0.004 min
Response: 13423629
Conc: 12.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
P030-SS001-0006-01

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/24/2022
Supervised By :Ankita Jodhani 05/24/2022

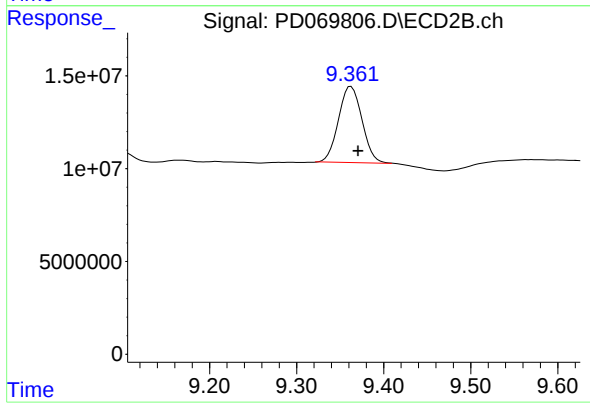

#28 Decachlorobiphenyl

R.T.: 9.361 min
Delta R.T.: -0.010 min
Response: 76931203
Conc: 12.84 ng/ml m