

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052422\
 Data File : PD069808.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2022 22:25
 Operator : AR\AJ
 Sample : N2894-24
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P008-SS004-0006-01

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/24/2022
 Supervised By :Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 02:45:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Mon May 23 02:08:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	4.169	9699183	97037703	9.679	10.157m
28)	SA Decachlor...	8.194	9.362	10041525	61842183	9.309	10.319
Target Compounds							
12)	B 4,4'-DDE	5.601	6.545	634161	6694044	0.548	0.674m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052422\
Data File : PD069808.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2022 22:25
Operator : AR\AJ
Sample : N2894-24
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
P008-SS004-0006-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/24/2022
Supervised By : Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 02:45:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Mon May 23 02:08:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

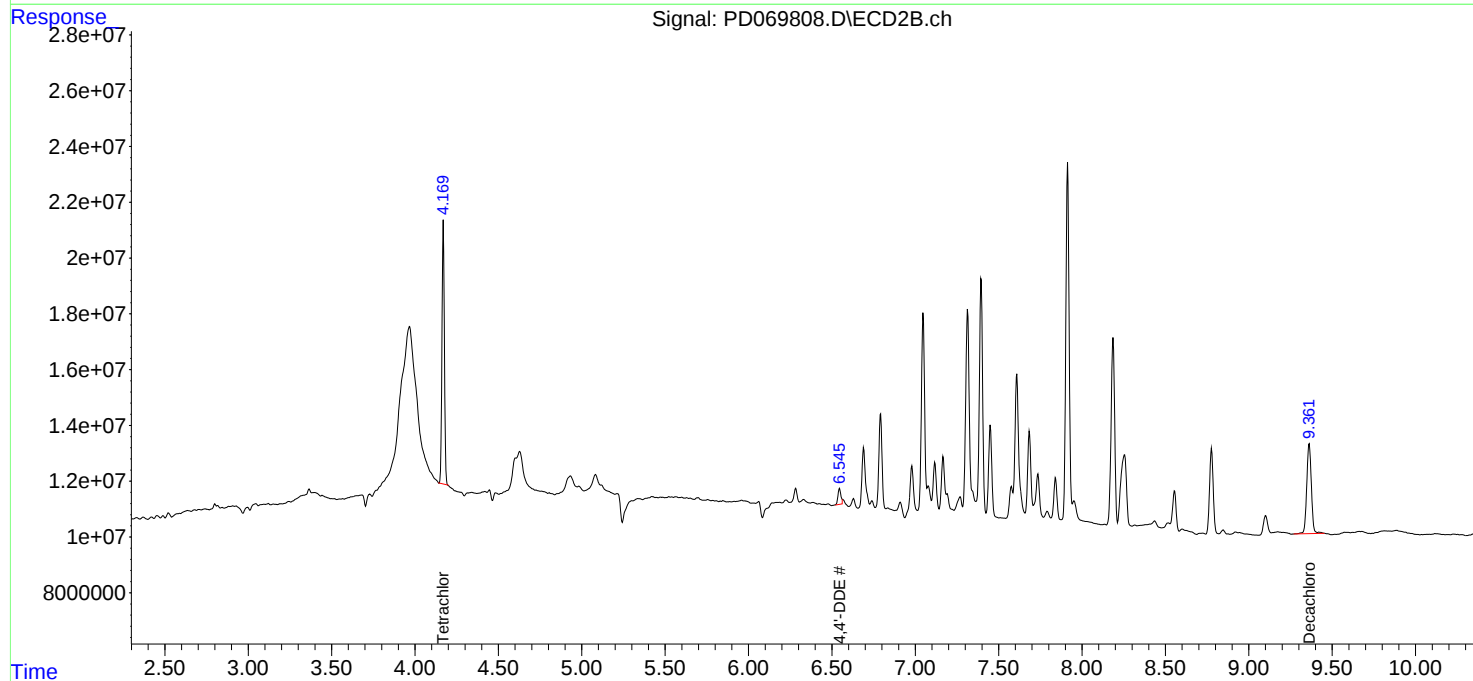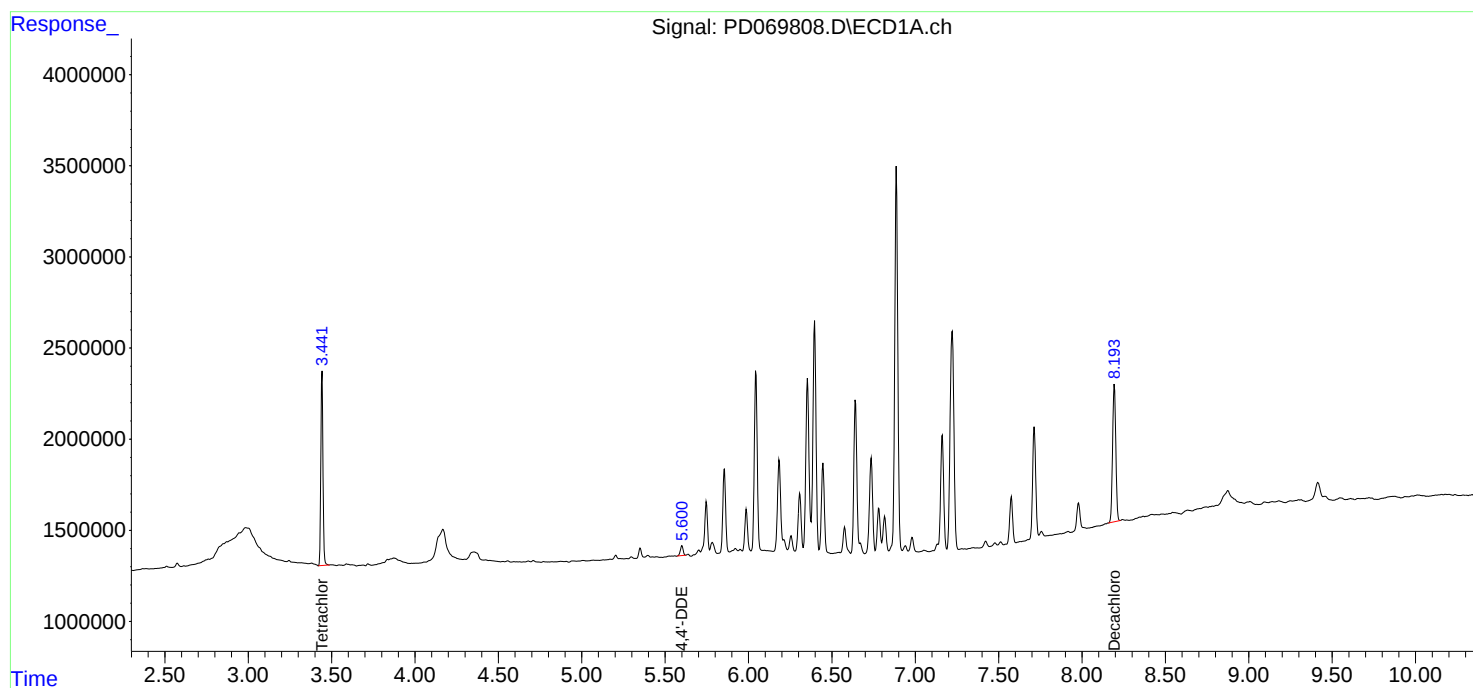

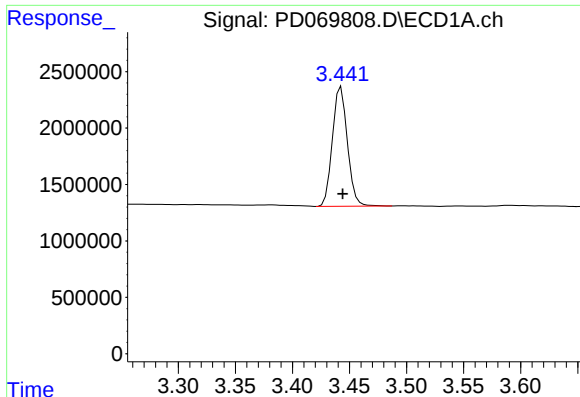


#1 Tetrachloro-m-xylene

R.T.: 3.443 min
Delta R.T.: -0.001 min
Response: 9699183
Conc: 9.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
P008-SS004-0006-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/24/2022
Supervised By :Ankita Jodhani 05/24/2022

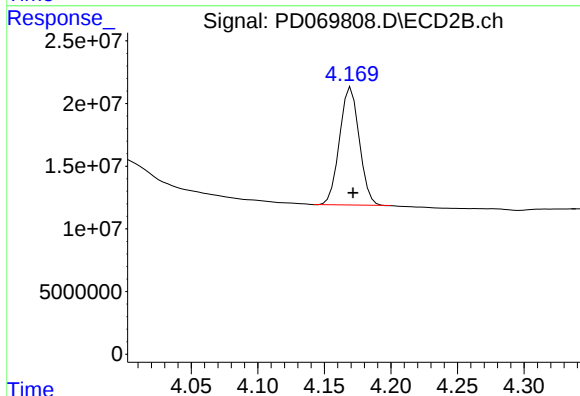


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: -0.003 min
Response: 97037703
Conc: 10.16 ng/ml m

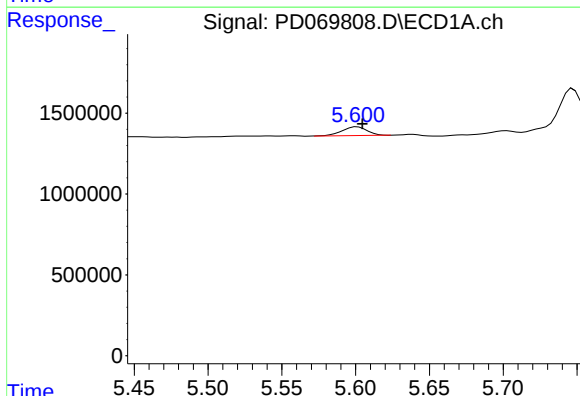


#12 4,4'-DDE

R.T.: 5.601 min
Delta R.T.: -0.003 min
Response: 634161
Conc: 0.55 ng/ml

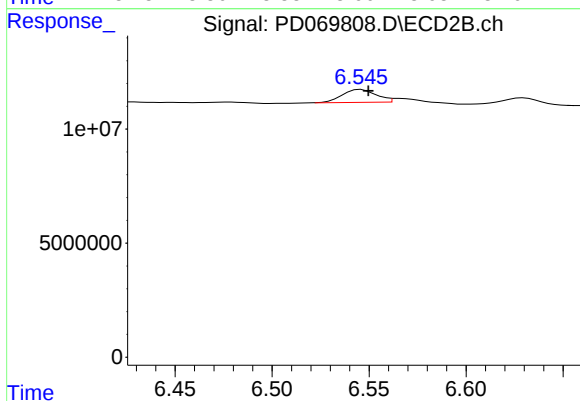

#12 4,4'-DDE

R.T.: 6.545 min
Delta R.T.: -0.005 min
Response: 6694044
Conc: 0.67 ng/ml m

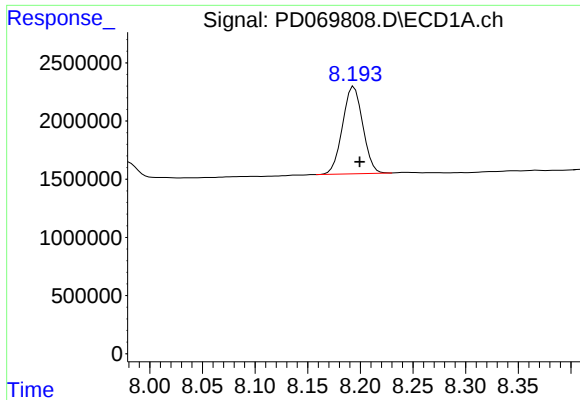


#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: -0.005 min
Response: 10041525
Conc: 9.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
P008-SS004-0006-01

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/24/2022
Supervised By :Ankita Jodhani 05/24/2022

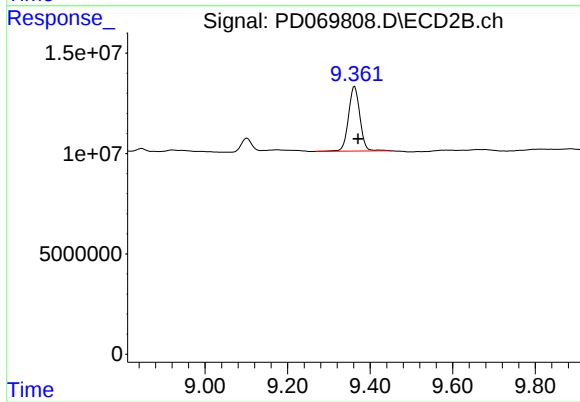

#28 Decachlorobiphenyl

R.T.: 9.362 min
Delta R.T.: -0.009 min
Response: 61842183
Conc: 10.32 ng/ml