

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052422\
 Data File : PD069811.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2022 23:21
 Operator : AR\AJ
 Sample : N2895-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P030-SS001-1218-01

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/24/2022
 Supervised By : Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 02:47:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Mon May 23 02:08:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.169	18301698	176.1E6	18.264	18.427m
28)	SA Decachlor...	8.194	9.363	15382115	89966168	14.261	15.012
Target Compounds							
12)	B 4,4'-DDE	5.601	6.544	782211	8376690	0.676	0.844m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052422\
Data File : PD069811.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2022 23:21
Operator : AR\AJ
Sample : N2895-07
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
P030-SS001-1218-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/24/2022
Supervised By : Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 02:47:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Mon May 23 02:08:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

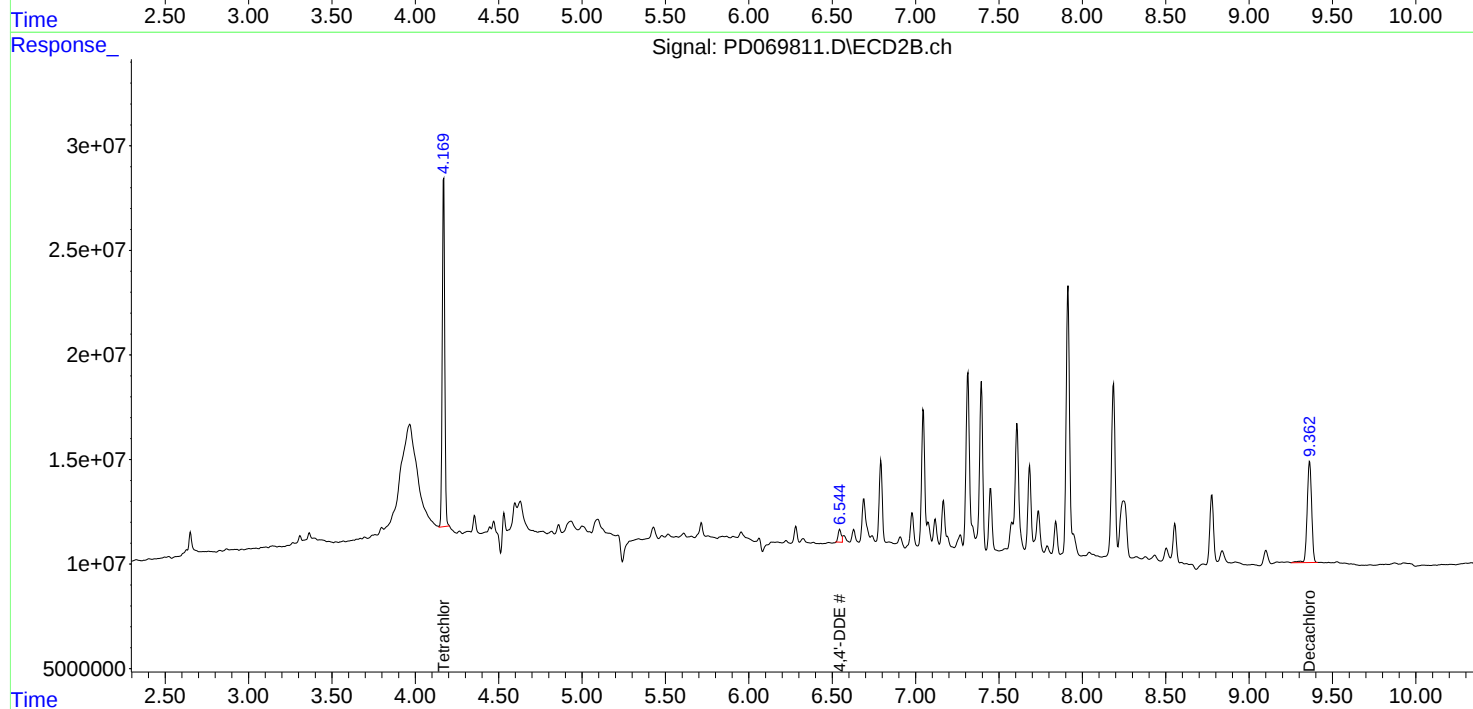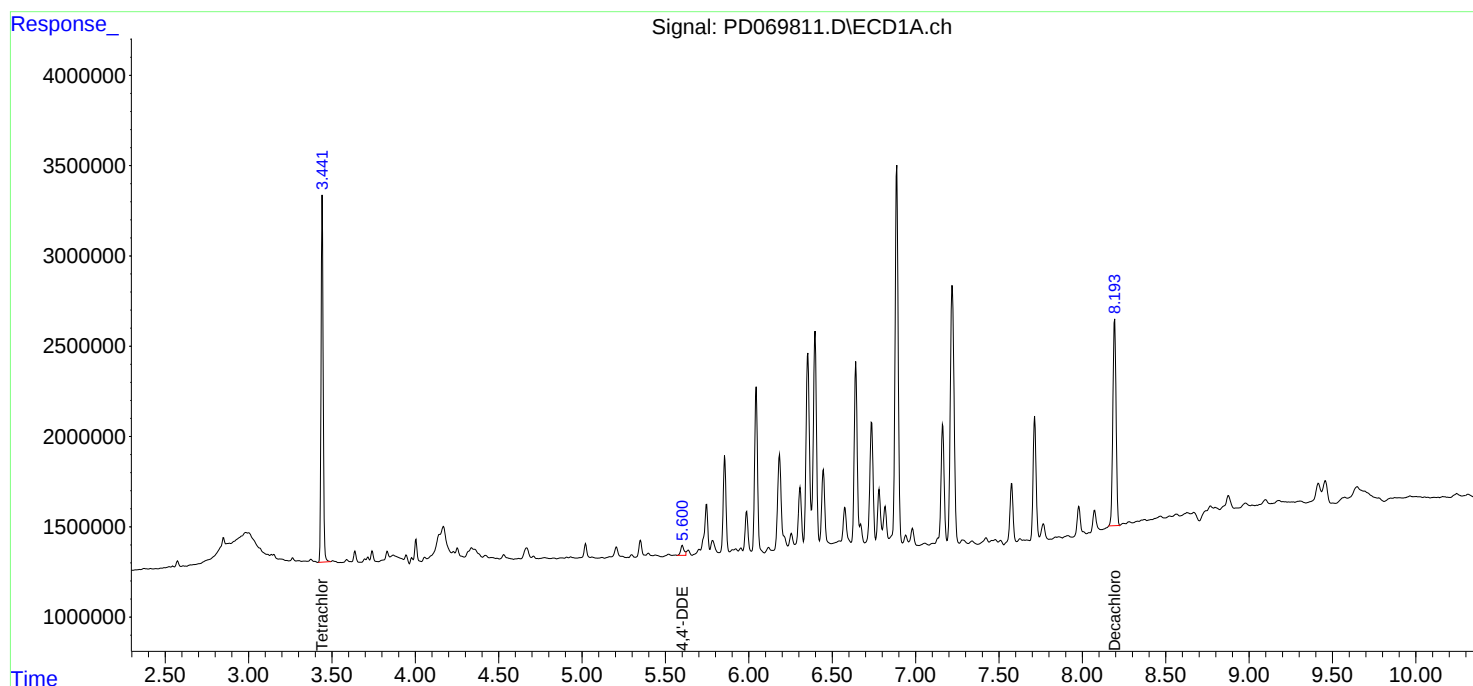

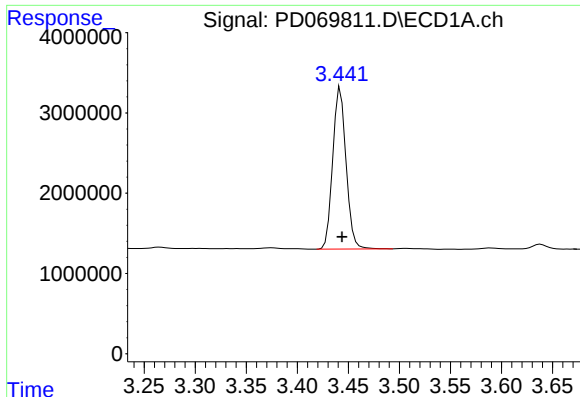


#1 Tetrachloro-m-xylene

R.T.: 3.442 min
Delta R.T.: -0.002 min
Response: 18301698
Conc: 18.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
P030-SS001-1218-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/24/2022
Supervised By :Ankita Jodhani 05/24/2022

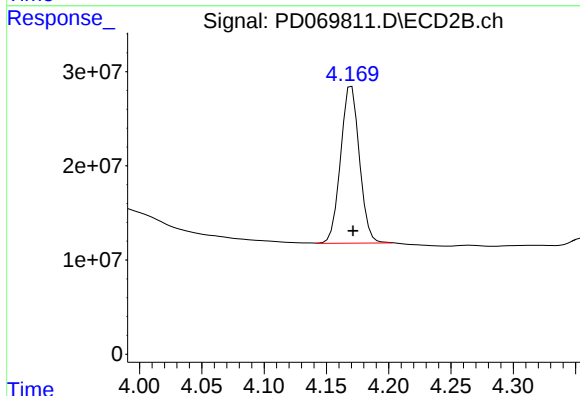


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: -0.003 min
Response: 176053542
Conc: 18.43 ng/ml m

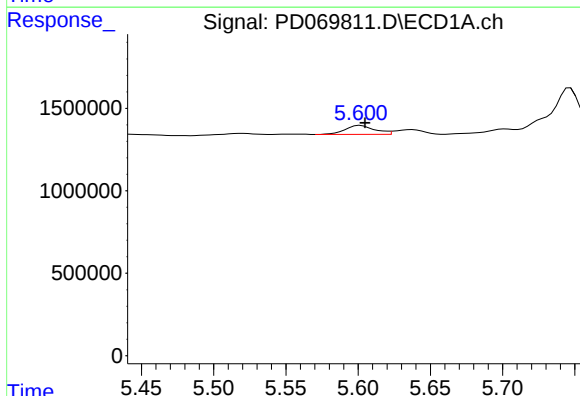


#12 4,4'-DDE

R.T.: 5.601 min
Delta R.T.: -0.003 min
Response: 782211
Conc: 0.68 ng/ml

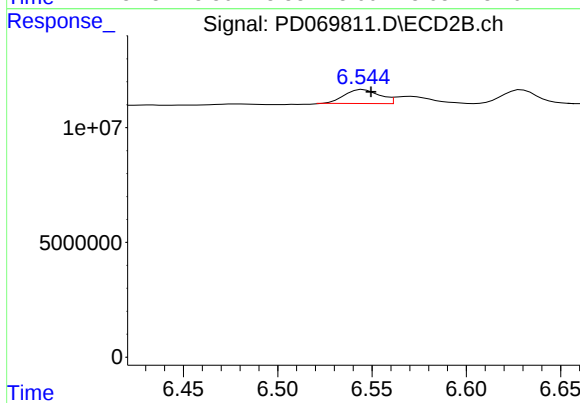

#12 4,4'-DDE

R.T.: 6.544 min
Delta R.T.: -0.006 min
Response: 8376690
Conc: 0.84 ng/ml m

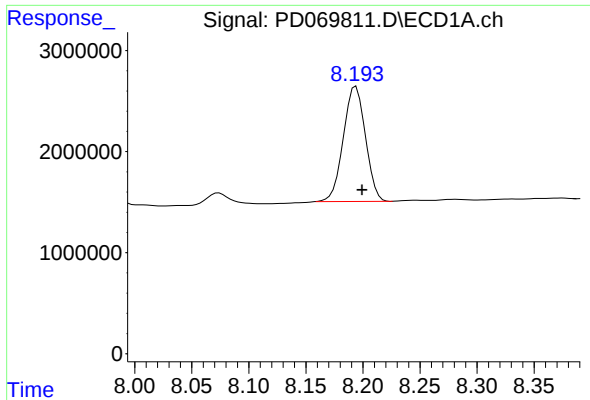


#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: -0.005 min
Response: 15382115
Conc: 14.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
P030-SS001-1218-01

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/24/2022
Supervised By :Ankita Jodhani 05/24/2022

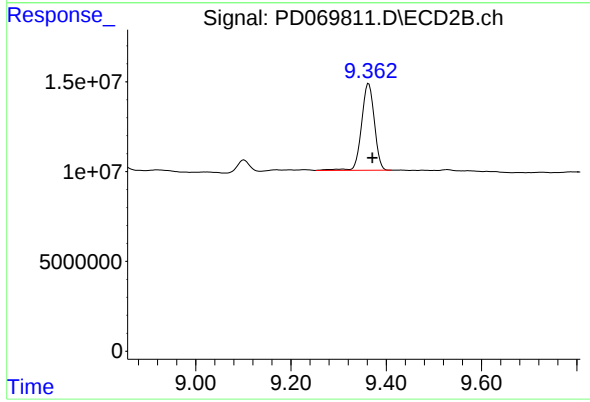

#28 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: -0.008 min
Response: 89966168
Conc: 15.01 ng/ml