

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052422\
 Data File : PD069816.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2022 00:31
 Operator : AR\AJ
 Sample : N2896-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P038-SS001-0006-02

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/13/2022
 Supervised By :Ankita Jodhani 06/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 02:49:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
 Quant Title : GC Extractables
 QLast Update : Mon May 23 02:08:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.442	4.169	11473419	115.4E6	11.450	12.077m
2) SA Decachlor...	8.194	9.361	15446800	88427740	14.321	14.755m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052422\
Data File : PD069816.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2022 00:31
Operator : AR\AJ
Sample : N2896-07
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
P038-SS001-0006-02


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/13/2022
Supervised By :Ankita Jodhani 06/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 02:49:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052022.M
Quant Title : GC Extractables
QLast Update : Mon May 23 02:08:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

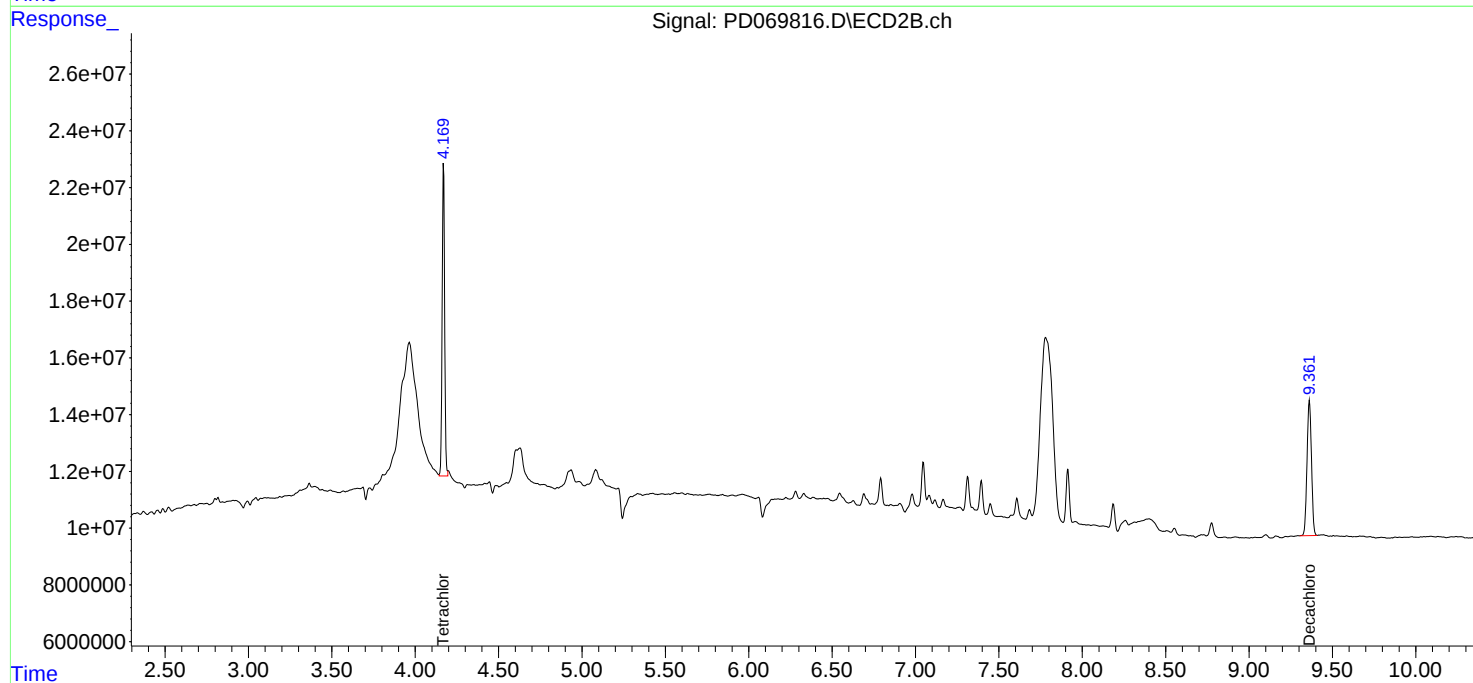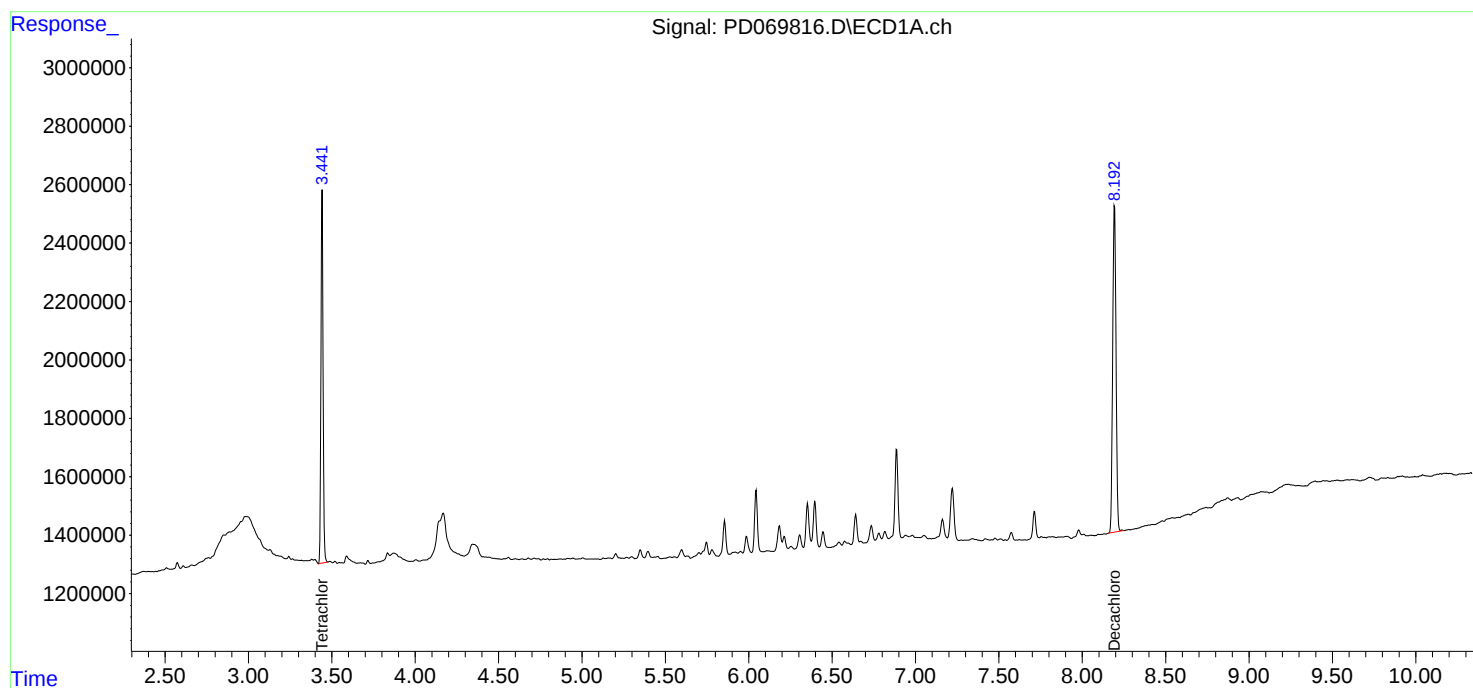

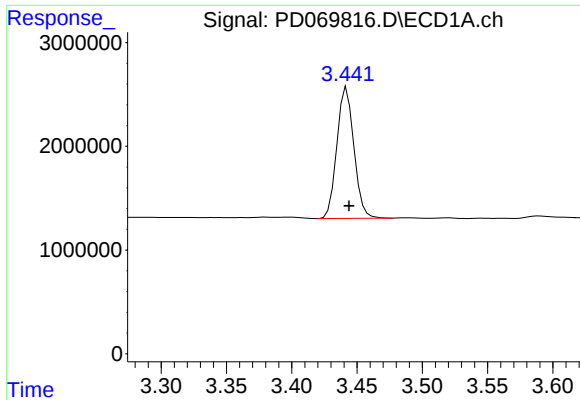


#1 Tetrachloro-m-xylene

R.T.: 3.442 min
Delta R.T.: -0.002 min
Response: 11473419
Conc: 11.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
P038-SS001-0006-02


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/13/2022
Supervised By :Ankita Jodhani 06/13/2022

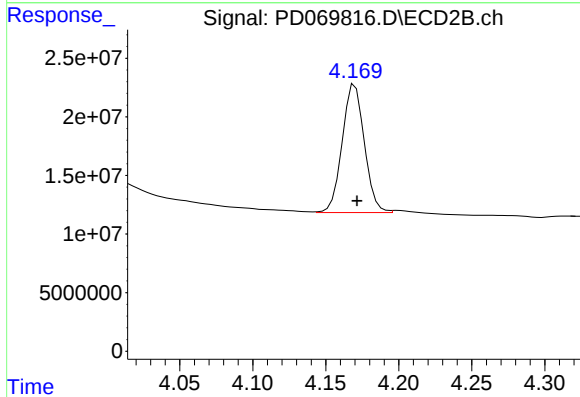


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: -0.003 min
Response: 115380349
Conc: 12.08 ng/ml m

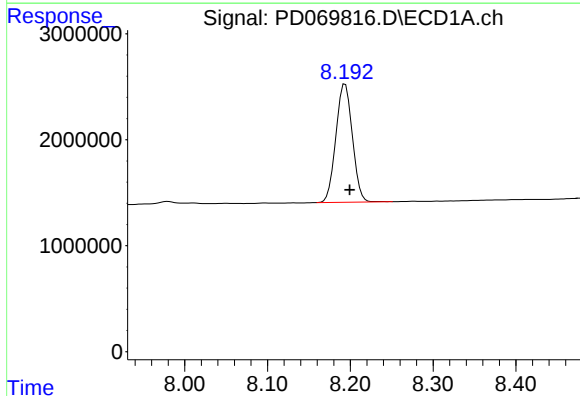

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: -0.006 min
Response: 15446800
Conc: 14.32 ng/ml

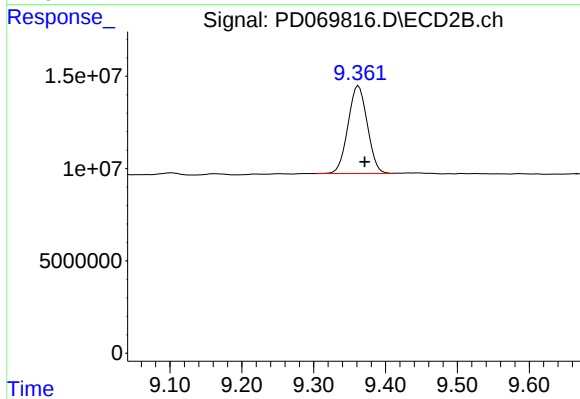

#28 Decachlorobiphenyl

R.T.: 9.361 min
Delta R.T.: -0.010 min
Response: 88427740
Conc: 14.76 ng/ml m