

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052424\
 Data File : PD082964.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2024 16:48
 Operator : AR\AJ
 Sample : P2547-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH5P2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/23/2024
 Supervised By :Ankita Jodhani 05/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 22:10:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.564	2.775	13106732	37265724	8.763	9.583
2) SA Decachlor...	9.130	7.904	28178905	32143278	14.058	8.124 #
Target Compounds						
9) A Endosulfan I	6.136	5.118	3620486	7226587	1.740m	1.602m
12) B 4,4'-DDE	6.226	5.224	9081512	28817014	4.164	6.043 #
17) MA 4,4'-DDT	7.060	6.028	8207751	19822963	5.103m	5.163

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052424\
Data File : PD082964.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2024 16:48
Operator : AR\AJ
Sample : P2547-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 22:10:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

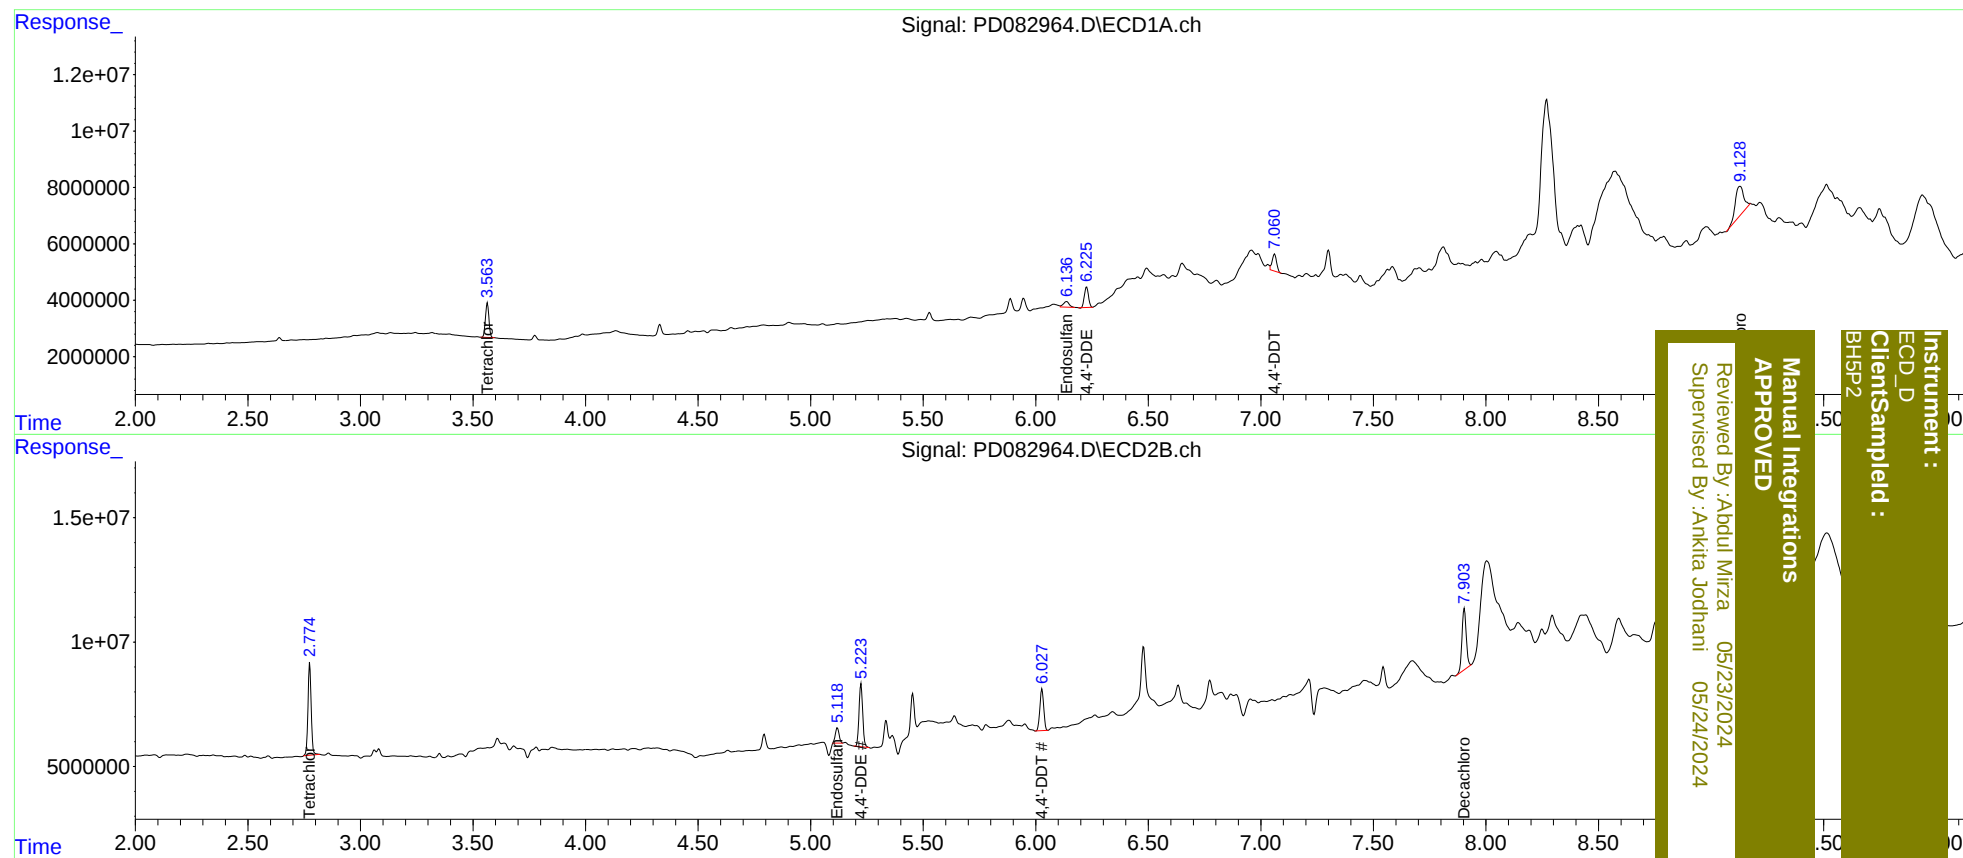

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/23/2024
Supervised By: Ankita Jodhani 05/24/2024

Instrument :
ECD_D
ClientSampled :
BHSP2