

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD052424\  
 Data File : PD082967.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 22 May 2024 17:28  
 Operator : AR\AJ  
 Sample : P2547-07  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 BH5Q0

Manual Integrations  
 APPROVED

Reviewed By :Abdul Mirza 05/23/2024  
 Supervised By :Ankita Jodhani 05/24/2024

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 22 22:13:49 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD051924CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Fri May 17 05:17:58 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


| Compound                    | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml    |
|-----------------------------|-------|-------|----------|----------|---------|----------|
| -----                       |       |       |          |          |         |          |
| System Monitoring Compounds |       |       |          |          |         |          |
| 1) SA Tetrachlo...          | 3.563 | 2.774 | 13241283 | 39658954 | 8.853m  | 10.199m  |
| 27) SA Decachlor...         | 9.114 | 7.903 | 39909065 | 93924861 | 19.911m | 23.740   |
| Target Compounds            |       |       |          |          |         |          |
| 4) MA Heptachlor            | 4.973 | 3.923 | 3690073  | 5759455  | 1.465m  | 1.034m#  |
| 8) B Heptachlo...           | 5.716 | 4.720 | 1553834  | 7080354  | 0.696m  | 1.386m#  |
| 9) A Endosulfan I           | 6.139 | 5.118 | 32233940 | 65854250 | 15.491m | 14.602m  |
| 10) B trans-Chl...          | 5.974 | 4.972 | 6428070  | 14196314 | 2.969m  | 2.851m   |
| 11) B cis-Chlor...          | 6.059 | 5.035 | 23897608 | 15256278 | 10.700  | 3.004m#  |
| 12) B 4,4'-DDE              | 6.227 | 5.224 | 42819715 | 138.9E6  | 19.635  | 29.129 # |
| 13) MA Dieldrin             | 6.403 | 5.362 | 17981358 | 89663244 | 8.181   | 17.943m# |
| 14) MA Endrin               | 6.643 | 5.638 | 10034306 | 23204094 | 5.627m  | 5.305m   |
| 16) A 4,4'-DDD              | 6.731 | 5.777 | 23315891 | 29748391 | 15.034m | 7.906m#  |
| 17) MA 4,4'-DDT             | 7.060 | 6.028 | 54424116 | 141.8E6  | 33.838m | 36.934   |
| -----                       |       |       |          |          |         |          |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD052424\  
Data File : PD082967.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 22 May 2024 17:28  
Operator : AR\AJ  
Sample : P2547-07  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 22 22:13:49 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD051924CLP.M  
Quant Title : GC Extractables  
QLast Update : Fri May 17 05:17:58 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

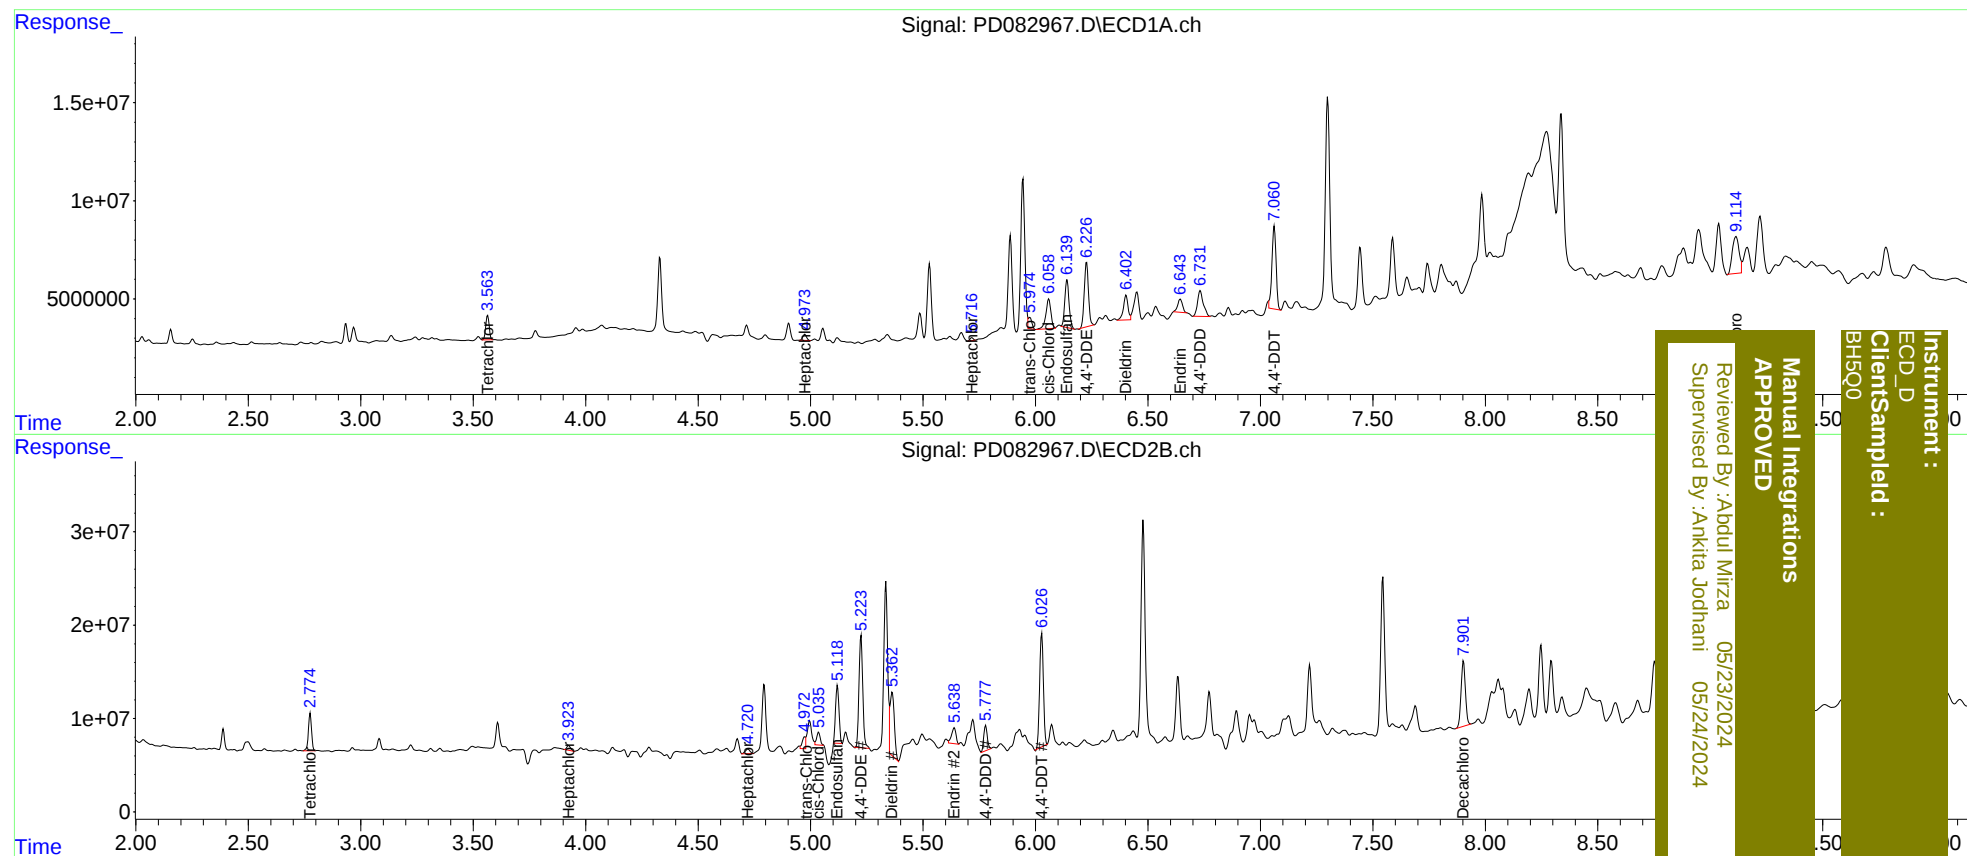

Manual Integrations  
APPROVED  
Reviewed By: Abdul Mirza 05/23/2024  
Supervised By: Ankita Jodhani 05/24/2024

Instrument :  
ECD\_D  
ClientSampled :  
BH500