

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052424\
 Data File : PD082977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2024 20:08
 Operator : AR\AJ
 Sample : P2547-14
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH5X1

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/23/2024
 Supervised By :Ankita Jodhani 05/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 22:27:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.565	2.775	14788814	42321310	9.887	10.883
27) SA Decachlor...	9.118	7.904	18602862	43818605	9.281	11.075
Target Compounds						
9) A Endosulfan I	6.138	5.119	3212450	9395463	1.544m	2.083m#
12) B 4,4'-DDE	6.227	5.224	33305764	100.5E6	15.272	21.085 #
14) MA Endrin	6.647	5.639	10448725	20632544	5.860m	4.718m
17) MA 4,4'-DDT	7.062	6.029	40402441	99799450	25.120	25.992

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052424\
Data File : PD082977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2024 20:08
Operator : AR\AJ
Sample : P2547-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 22:27:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

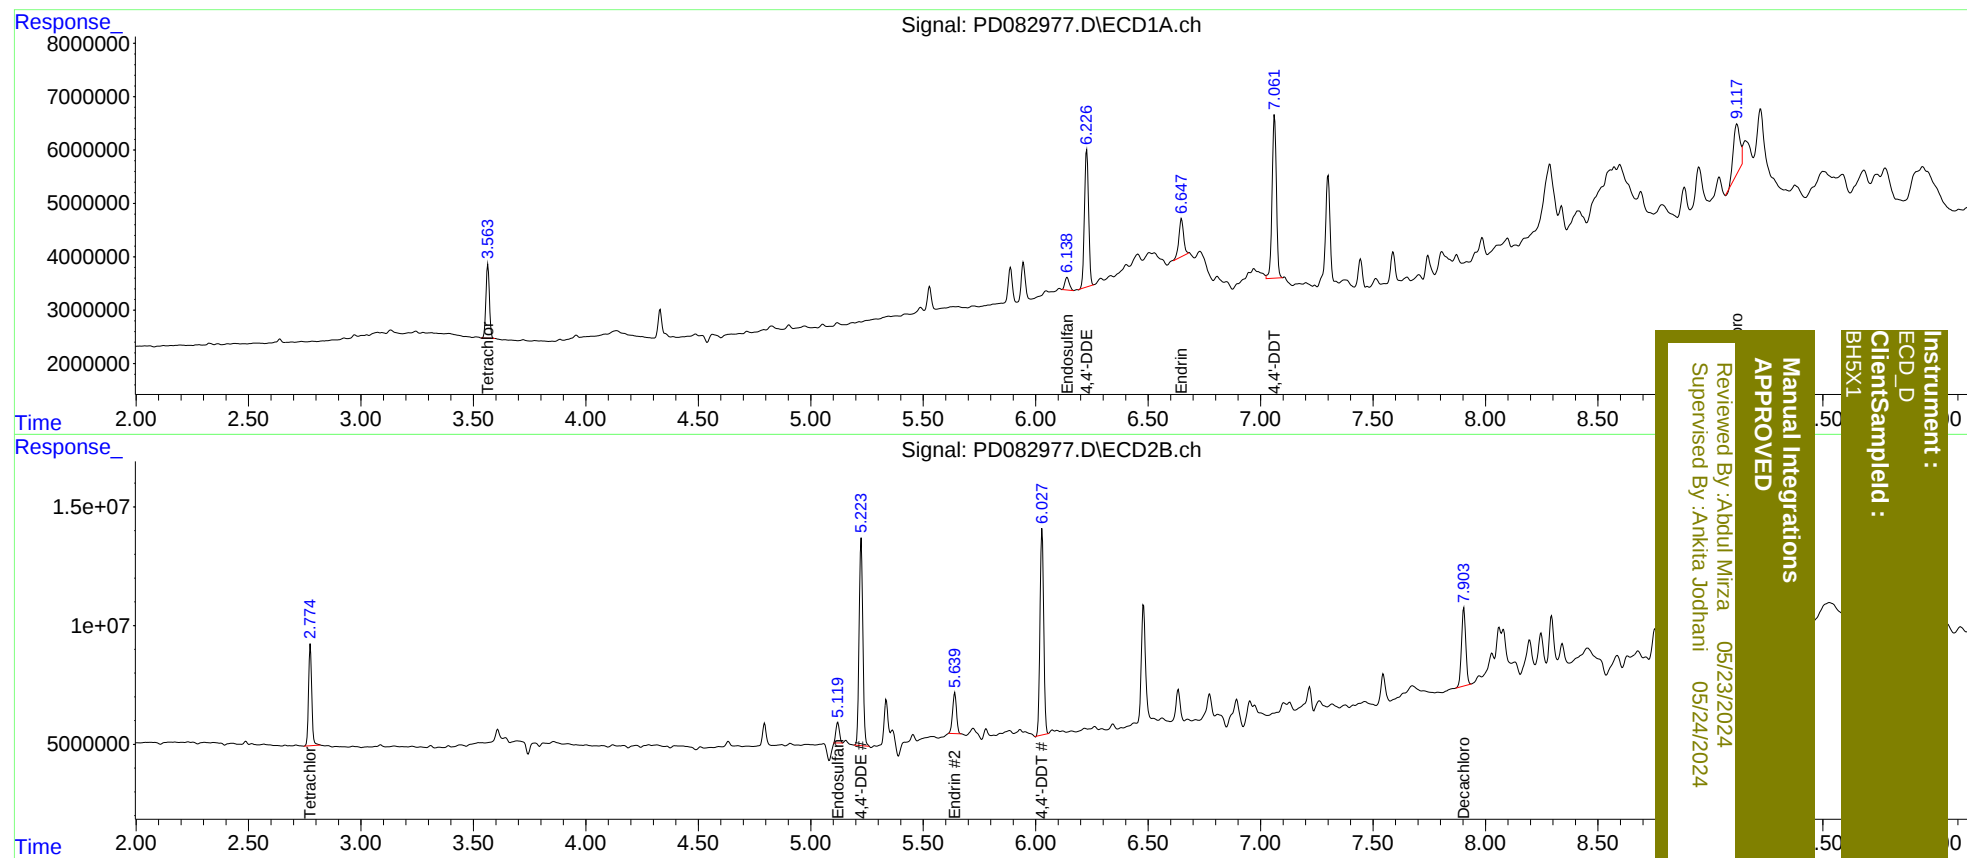

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/23/2024
Supervised By: Ankita Jodhani 05/24/2024

Instrument :
ECD_D
Client Sampled :
BH5X1