

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052521\
 Data File : PD063266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2021 10:39
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 23:36:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX051721.M
 Quant Title : GC Extractables
 QLast Update : Tue May 25 08:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.445	3.971	63458980	605.7E6	50.918	50.728
7) SA Decachlor...	8.200	9.027	65929984	557.8E6	50.953	51.669
Target Compounds						
2) Toxaphene-1	6.000	6.544	5178993	71948626	502.062	477.347
3) Toxaphene-2	6.183	7.051	6068032	55988048	562.861	502.620
4) Toxaphene-3	6.302	7.127	12393365	166.1E6	503.298	535.988
5) Toxaphene-4	6.548	7.213	12729663	101.3E6	521.587	541.046
6) Toxaphene-5	7.035	7.627	13447936	72150898	488.430	568.392

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052521\
Data File : PD063266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2021 10:39
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 23:36:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX051721.M
Quant Title : GC Extractables
QLast Update : Tue May 25 08:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

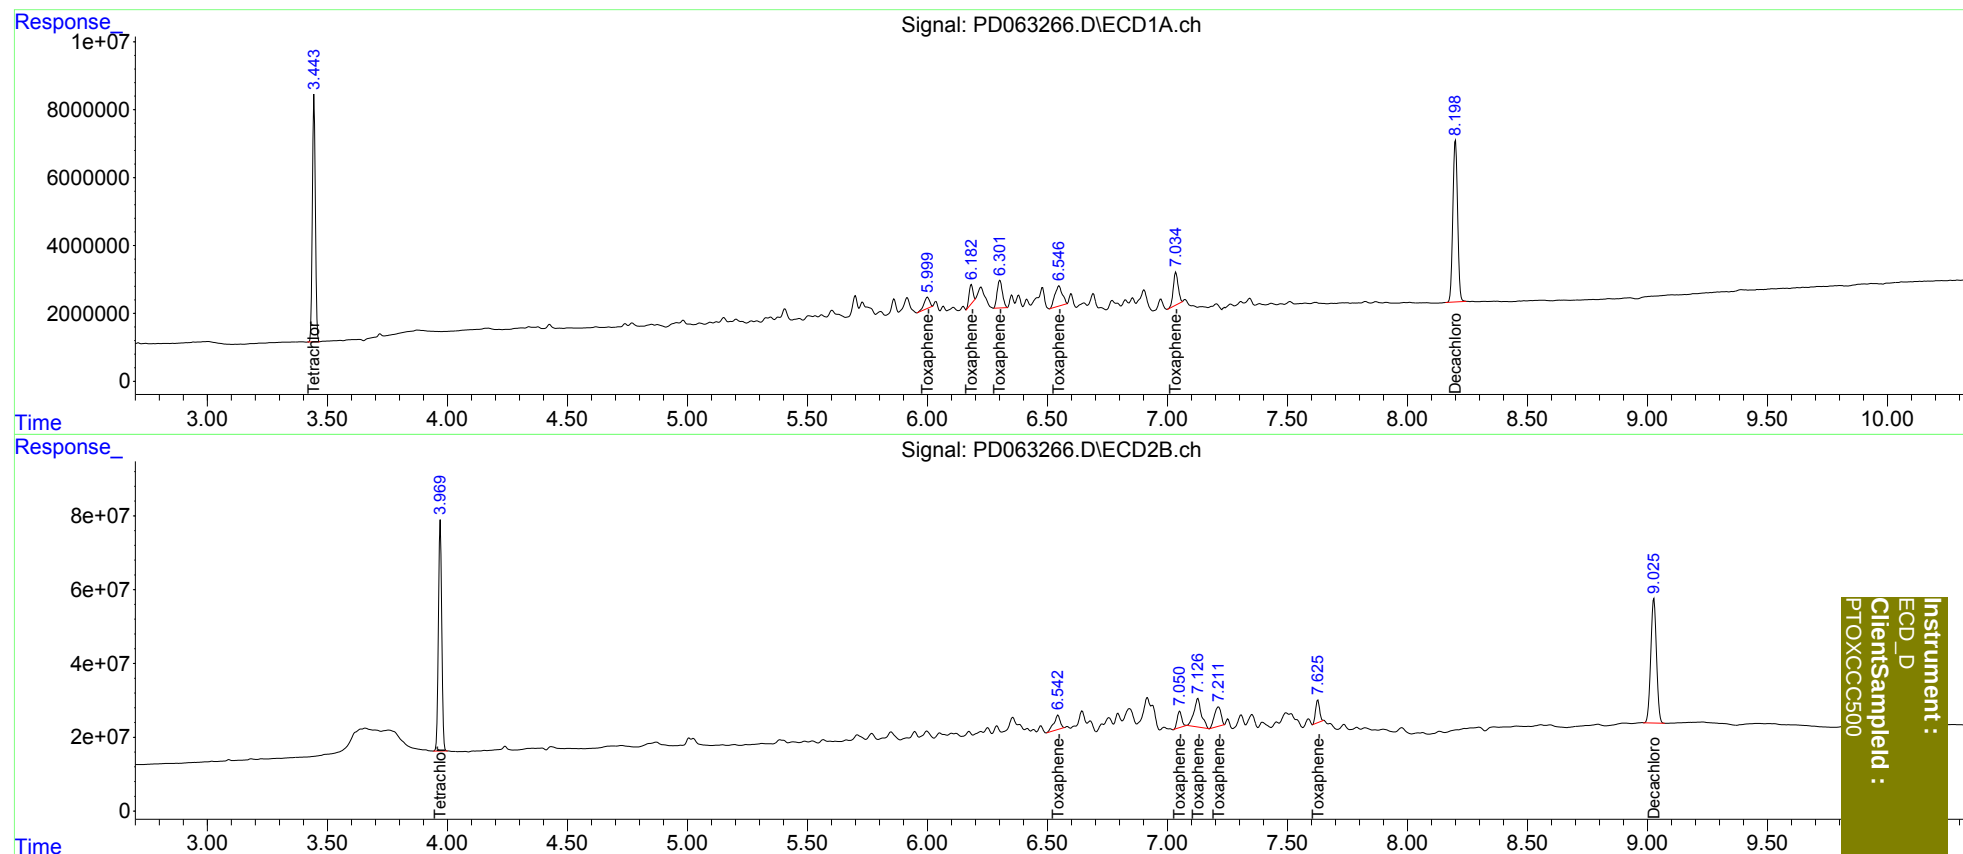

Instrument :
ECD_D
ClientSampled :
PTOXCCC500