

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052524\
 Data File : PD083009.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2024 14:53
 Operator : AR\AJ
 Sample : P2548-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH5X8

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/28/2024
 Supervised By : Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 22:29:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.570	2.772	10116564	45216279	6.764m	11.628m#
2) SA Decachlor...	9.115	7.902	57107161	110.9E6	28.491m	28.040
Target Compounds						
12) B 4,4'-DDE	6.237	5.224	529.0E6	1443.1E6	242.569	302.620
13) MA Dieldrin	6.410	5.361	42054501	202.3E6	19.134m	40.480m#
16) A 4,4'-DDD	6.742	5.777	53228036	65803066	34.321	17.488m#
17) MA 4,4'-DDT	7.071	6.028	511.4E6	1036.3E6	317.935	269.903

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052524\
Data File : PD083009.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2024 14:53
Operator : AR\AJ
Sample : P2548-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 22:29:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

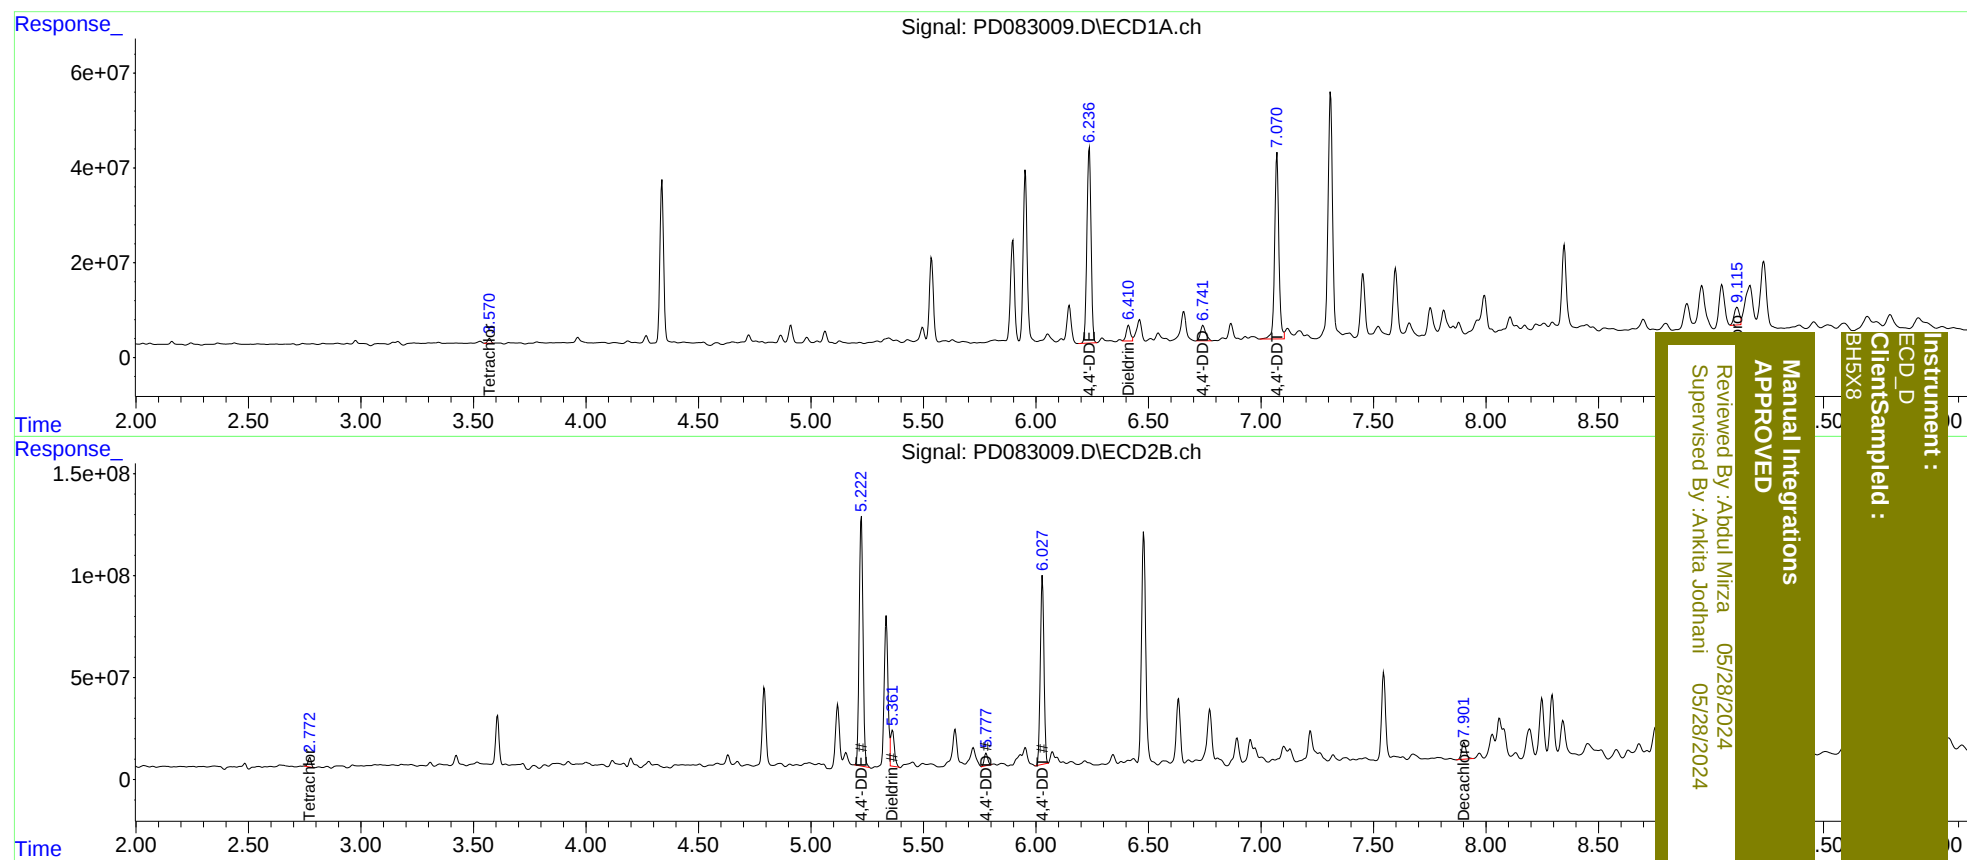

Instrument :
ECD_D
ClientSampled :
BH5X8

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/28/2024
Supervised By :Ankita Jodhani 05/28/2024