

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052524\
 Data File : PD083024.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2024 22:01
 Operator : AR\AJ
 Sample : P2548-14MS
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH610MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/28/2024
 Supervised By :Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 08:58:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.776	17248215	50526661	11.531m	12.993
27)	SA Decachlor...	9.112	7.903	37742708	80325382	18.830m	20.302
Target Compounds							
2)	A alpha-BHC	4.022	3.275	105.8E6	251.7E6	41.471	40.494
3)	MA gamma-BHC...	4.354	3.604	95623101	243.4E6	38.750m	42.060
4)	MA Heptachlor	4.947	3.942	103.7E6	219.4E6	41.177m	39.394
5)	MB Aldrin	5.292	4.222	95581123	223.7E6	39.476	40.481
6)	B beta-BHC	4.551	3.899	34882638	91029661	32.153m	36.296
7)	B delta-BHC	4.801	4.129	97231088	238.0E6	39.708	40.235
8)	B Heptachlo...	5.718	4.722	80867310	196.7E6	36.212m	38.499
9)	A Endosulfan I	6.106	5.094	76194586	120.7E6	36.617	26.771 #
10)	B trans-Chl...	5.974	4.970	83914509	207.1E6	38.765m	41.582m
11)	B cis-Chlor...	6.056	5.036	102.4E6	234.1E6	45.848	46.095
12)	B 4,4'-DDE	6.228	5.224	179.1E6	519.4E6	82.134	108.916 #
13)	MA Dieldrin	6.383	5.355	177.9E6	502.2E6	80.940	100.492m
14)	MA Endrin	6.614	5.631	129.9E6	379.1E6	72.867	86.671
15)	B Endosulfa...	6.833	5.925	140.6E6	381.3E6	72.975	90.487
16)	A 4,4'-DDD	6.746	5.778	132.3E6	293.0E6	85.291	77.871
17)	MA 4,4'-DDT	7.062	6.028	193.3E6	412.3E6	120.169	107.381
18)	B Endrin al...	6.963	6.102	100.6E6	218.4E6	72.431	69.247m
19)	B Endosulfa...	7.198	6.326	130.4E6	310.2E6	73.895	77.163
20)	A Methoxychlor	7.539	6.603	321.6E6	714.5E6	371.695	364.114
21)	B Endrin ke...	7.687	6.831	125.8E6	289.1E6	66.706	64.278

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052524\
Data File : PD083024.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2024 22:01
Operator : AR\AJ
Sample : P2548-14MS
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 08:58:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

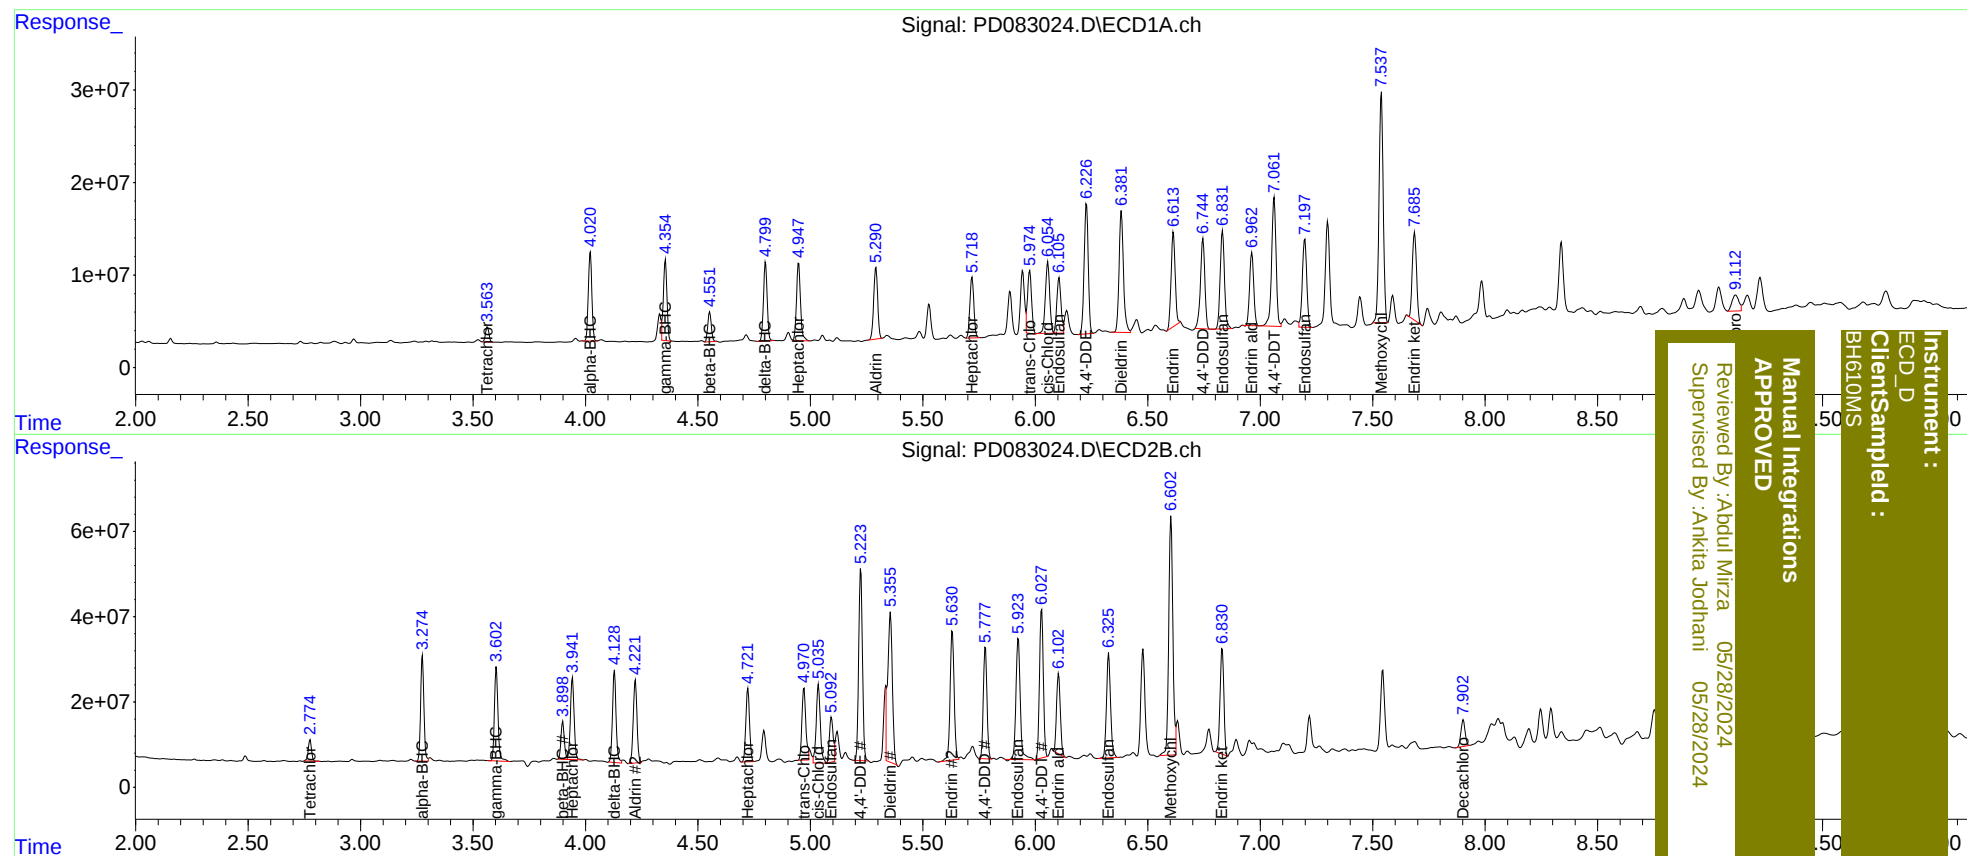

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/28/2024
Supervised By: Ankita Jodhani 05/28/2024

Instrument :
ECD_D
ClientSampled :
BH610MS