

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052524\
 Data File : PD083025.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2024 22:28
 Operator : AR\AJ
 Sample : P2548-15MSD
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH610MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/28/2024
 Supervised By :Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 09:07:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.776	17143252	51367479	11.461m	13.209
27)	SA Decachlor...	9.114	7.903	37399310	82863414	18.659m	20.944
Target Compounds							
2)	A alpha-BHC	4.022	3.275	106.4E6	253.5E6	41.695	40.785
3)	MA gamma-BHC...	4.355	3.604	99182835	245.5E6	40.192m	42.435
4)	MA Heptachlor	4.947	3.942	103.2E6	223.3E6	41.002m	40.103
5)	MB Aldrin	5.292	4.221	96429823	226.0E6	39.827	40.884
6)	B beta-BHC	4.551	3.899	34997403	92582992	32.259m	36.915
7)	B delta-BHC	4.801	4.127	97299002	233.4E6	39.736	39.458m
8)	B Heptachlo...	5.720	4.722	80002892	198.8E6	35.825	38.912
9)	A Endosulfan I	6.107	5.094	77657516	124.2E6	37.320	27.546 #
10)	B trans-Chl...	5.975	4.971	84339257	207.2E6	38.961m	41.613m
11)	B cis-Chlor...	6.057	5.036	104.2E6	237.6E6	46.661	46.777
12)	B 4,4'-DDE	6.228	5.224	182.0E6	528.3E6	83.440	110.792 #
13)	MA Dieldrin	6.383	5.355	180.6E6	497.8E6	82.149	99.613m
14)	MA Endrin	6.614	5.631	131.1E6	383.8E6	73.541	87.760
15)	B Endosulfa...	6.834	5.923	142.5E6	365.5E6	73.959	86.733m
16)	A 4,4'-DDD	6.746	5.778	134.6E6	293.9E6	86.801	78.099
17)	MA 4,4'-DDT	7.063	6.028	193.9E6	419.7E6	120.558	109.293
18)	B Endrin al...	6.964	6.104	101.0E6	213.8E6	72.712	67.798
19)	B Endosulfa...	7.199	6.326	125.8E6	312.2E6	71.263	77.644
20)	A Methoxychlor	7.539	6.604	311.2E6	721.8E6	359.701	367.869
21)	B Endrin ke...	7.687	6.831	124.7E6	290.8E6	66.170	64.657

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052524\
Data File : PD083025.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2024 22:28
Operator : AR\AJ
Sample : P2548-15MSD
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 09:07:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

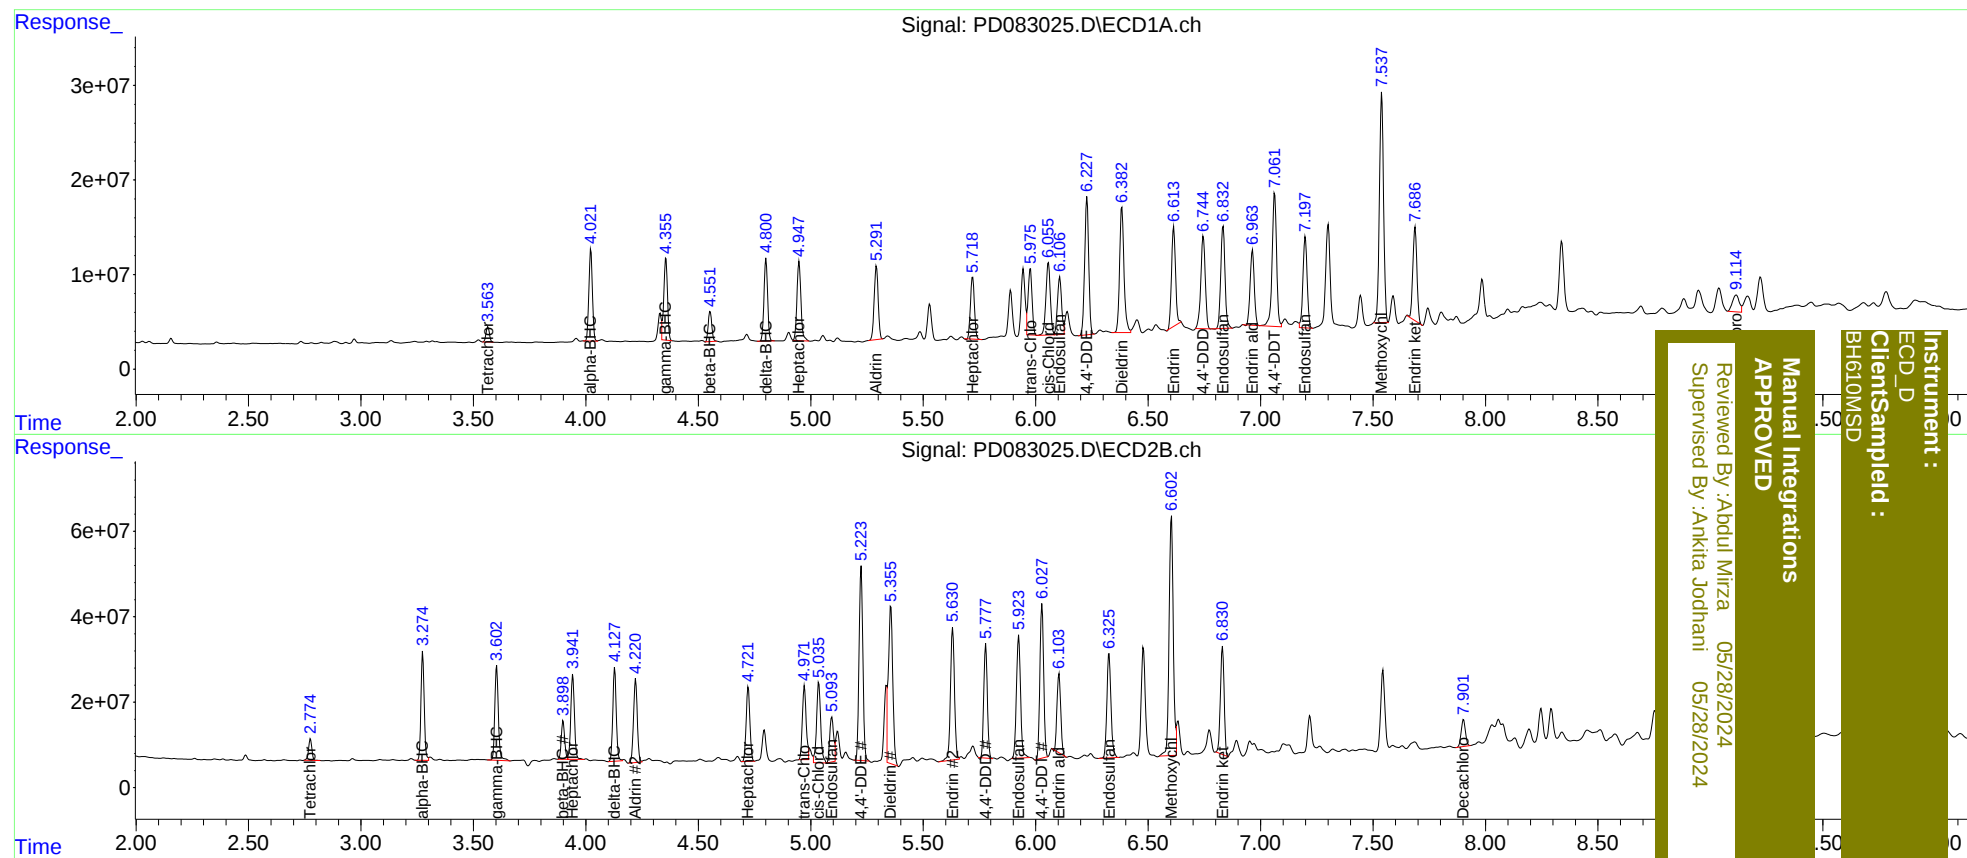

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/28/2024
Supervised By: Ankita Jodhani 05/28/2024

Instrument :
ECD_D
Client Sampled :
BH610MSD