

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052524\
 Data File : PD083011.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2024 15:46
 Operator : AR\AJ
 Sample : P2548-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH5Y0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/28/2024
 Supervised By : Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 22:31:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.563	2.776	11482551	44611670	7.677m	11.472 #
2) SA Decachlor...	9.102	7.902	41904618	80066732	20.906m	20.237
Target Compounds						
12) B 4,4'-DDE	6.228	5.225	1190.9E6	2838.6E6	546.102	595.242
13) MA Dieldrin	6.402	5.362	30335115	144.5E6	13.802	28.925m#
16) A 4,4'-DDD	6.735	5.777	38787699	55398358	25.010	14.723m#
17) MA 4,4'-DDT	7.062	6.028	1427.7E6	2708.8E6	887.672	705.460

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052524\
Data File : PD083011.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2024 15:46
Operator : AR\AJ
Sample : P2548-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 22:31:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

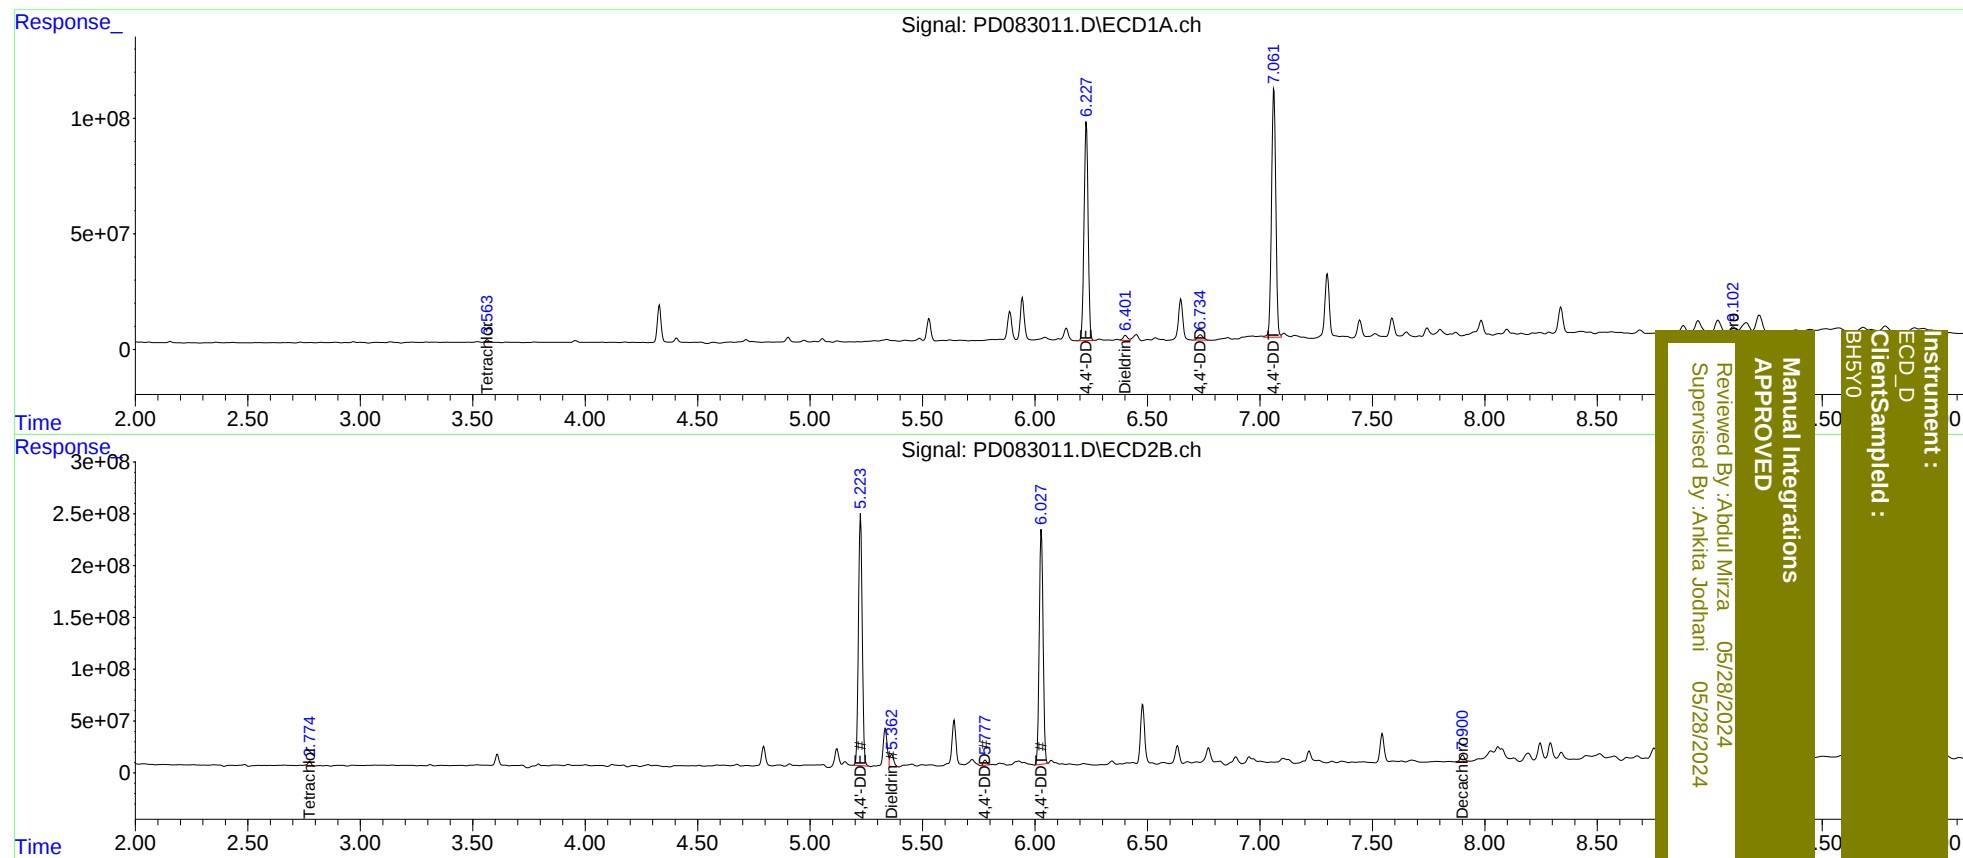

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/28/2024
Supervised By: Ankita Jodhani 05/28/2024

Instrument :
ECD_D
Client Sampled :
BHSYO