

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052524\
 Data File : PD083014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2024 18:02
 Operator : AR\AJ
 Sample : P2548-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH5Y3

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/28/2024
 Supervised By : Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 22:33:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.573	2.774	15505267	58271081	10.366m	14.985 #
2)	SA Decachlor...	9.119	7.904	36649409	87801225	18.284m	22.192
Target Compounds							
12)	B 4,4'-DDE	6.240	5.225	244.2E6	729.3E6	111.995	152.939 #
13)	MA Dieldrin	6.412	5.362	19431191	111.4E6	8.841m	22.300m#
16)	A 4,4'-DDD	6.745	5.778	30933570	44039911	19.946	11.704m#
17)	MA 4,4'-DDT	7.072	6.029	269.0E6	590.8E6	167.260m	153.869

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052524\
Data File : PD083014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2024 18:02
Operator : AR\AJ
Sample : P2548-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 22:33:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

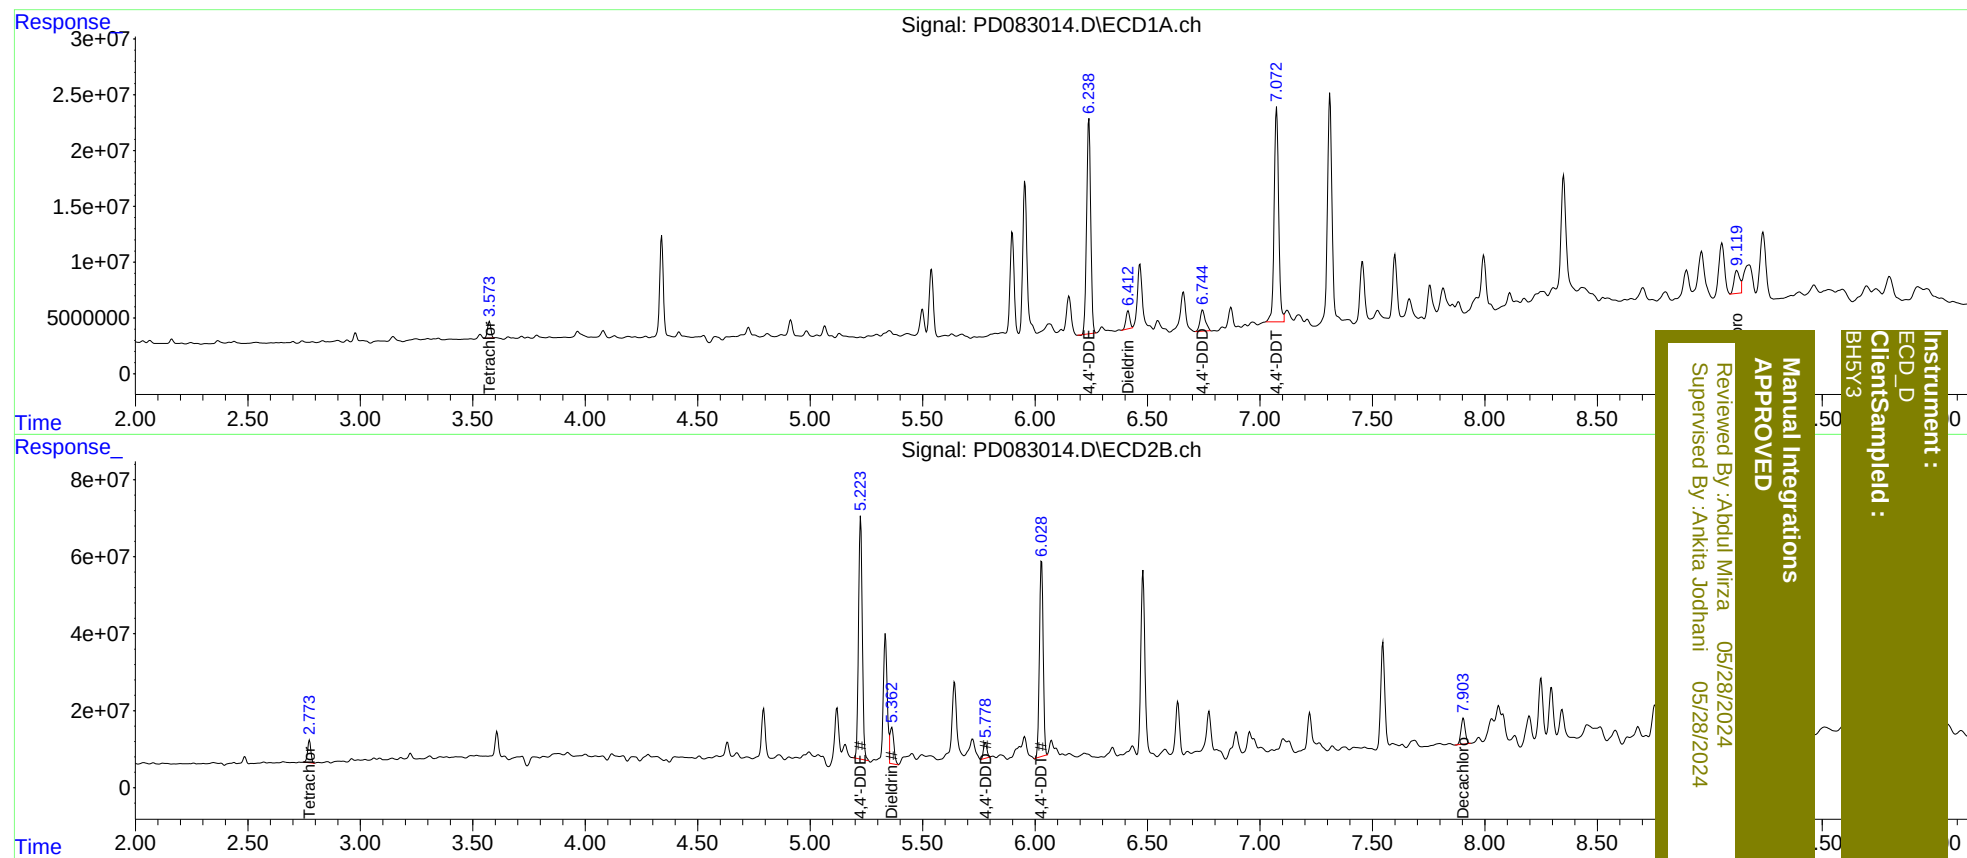

Reviewed By: Aboul Mirza 05/28/2024
Supervised By: Ankita Jodhani 05/28/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BHSY3