

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052620\
 Data File : PD058096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2020 15:30
 Operator : AJ\MA
 Sample : PB129082BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB129082BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 05:00:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.866	15476774	22387978	19.803	19.657
28)	SA Decachlor...	7.850	8.850	16194111	20710939	20.253	19.977
Target Compounds							
3)	MA gamma-BHC...	3.910	0.000	566871	0	0.483	N.D. #
5)	MB Aldrin	4.416	0.000	532679	0	0.508	N.D. #
8)	B Heptachlo...	4.851	0.000	153906	0	0.158	N.D. #
9)	A Endosulfan I	5.171	0.000	42129	0	0.046	N.D. #
10)	B gamma-Chl...	5.079	0.000	83666	0	0.084	N.D. #
11)	B alpha-Chl...	5.128	0.000	122462	0	0.124	N.D. #
14)	MA Endrin	5.689f	0.000	38636	0	0.048	N.D. #
24)	Chlordane-2	4.505f	0.000	266433	0	8.334	N.D. #
25)	Chlordane-3	5.079	0.000	83666	0	0.933	N.D. #
26)	Chlordane-4	5.128	0.000	122462	0	1.433	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052620\
Data File : PD058096.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2020 15:30
Operator : AJ\MA
Sample : PB129082BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB129082BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 05:00:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

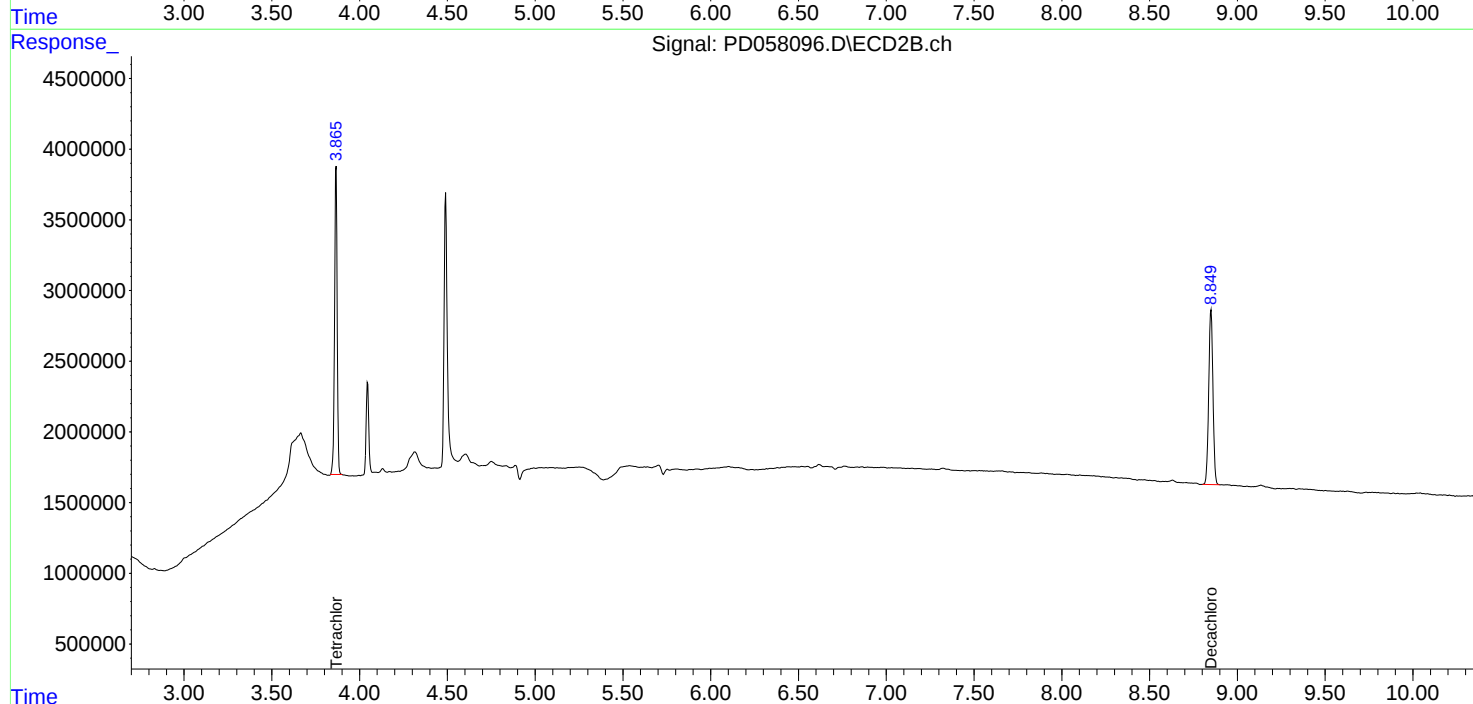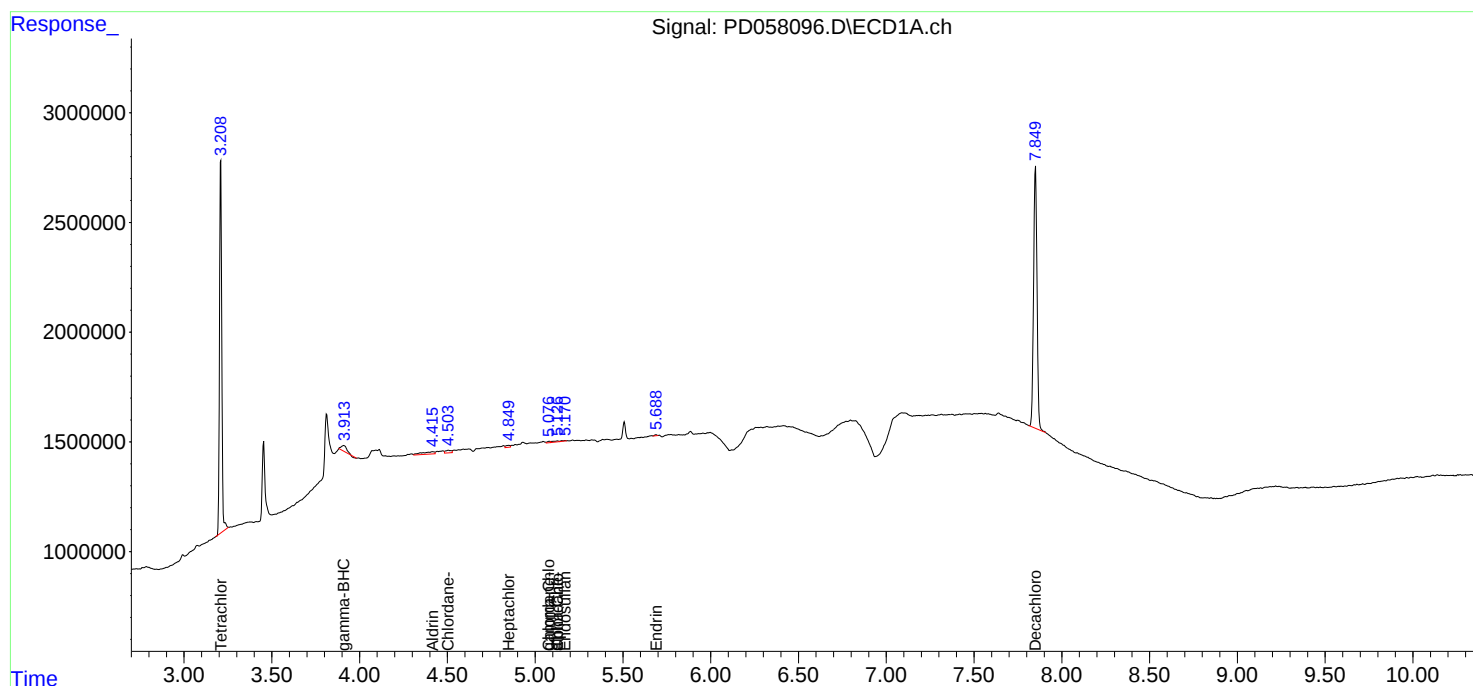


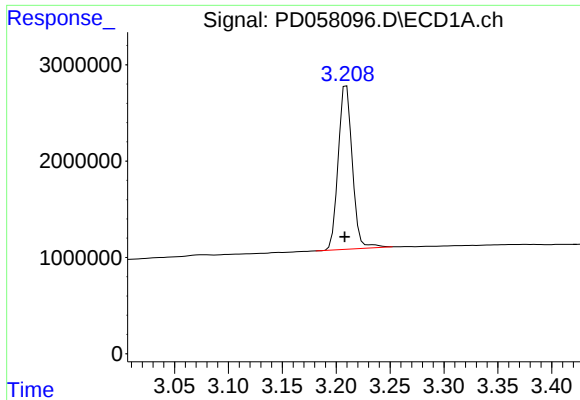

#1 Tetrachloro-m-xylene


R.T.: 3.210 min
Delta R.T.: 0.002 min
Response: 15476774
Conc: 19.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB129082BL

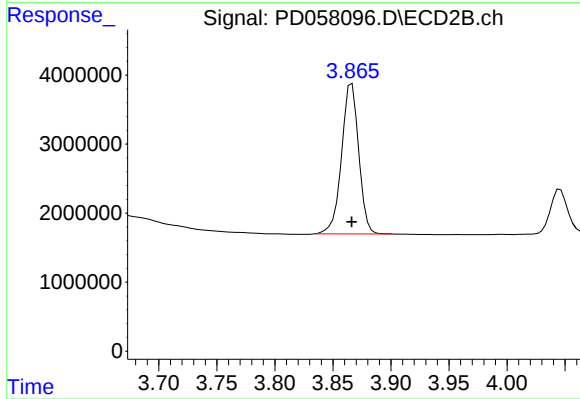


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 22387978
Conc: 19.66 ng/ml

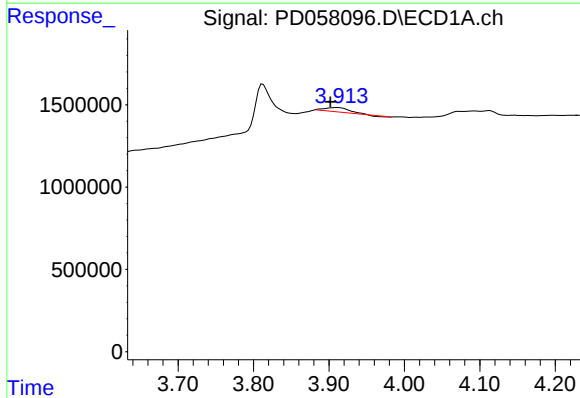


#3 gamma-BHC (Lindane)

R.T.: 3.910 min
Delta R.T.: 0.008 min
Response: 566871
Conc: 0.48 ng/ml

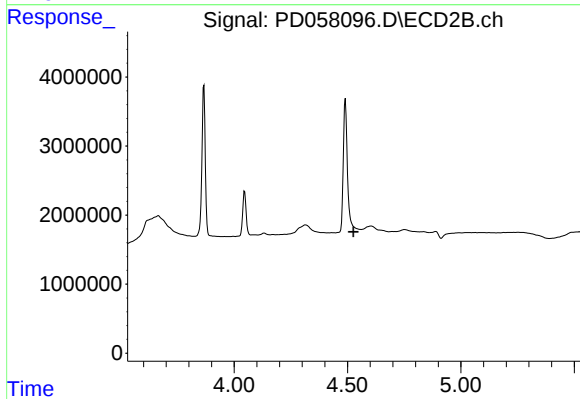

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.527 min
Response: 0
Conc: N.D.

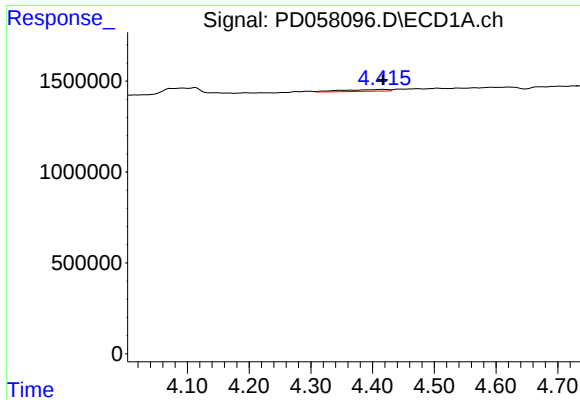

#5 Aldrin


R.T.: 4.416 min
Delta R.T.: 0.000 min
Response: 532679
Conc: 0.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB129082BL

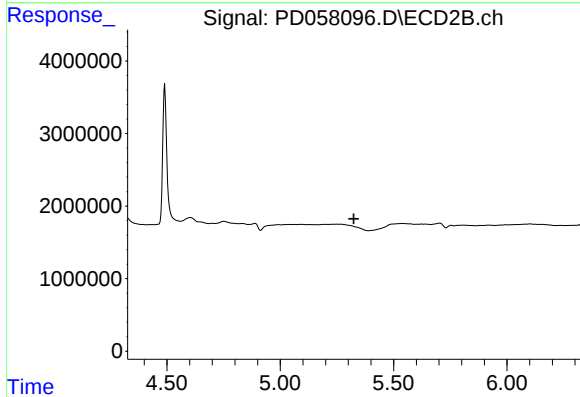


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.325 min
Response: 0
Conc: N.D.

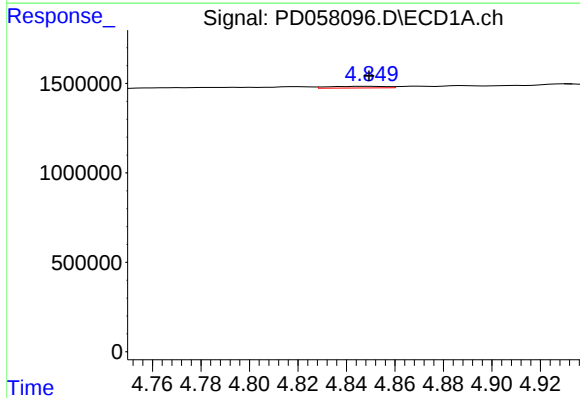


#8 Heptachlor epoxide

R.T.: 4.851 min
Delta R.T.: 0.001 min
Response: 153906
Conc: 0.16 ng/ml

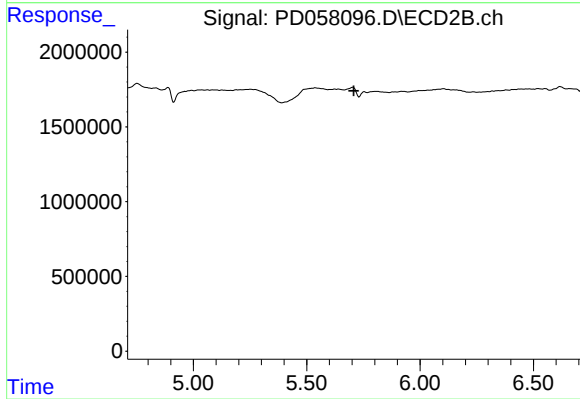

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.708 min
Response: 0
Conc: N.D.

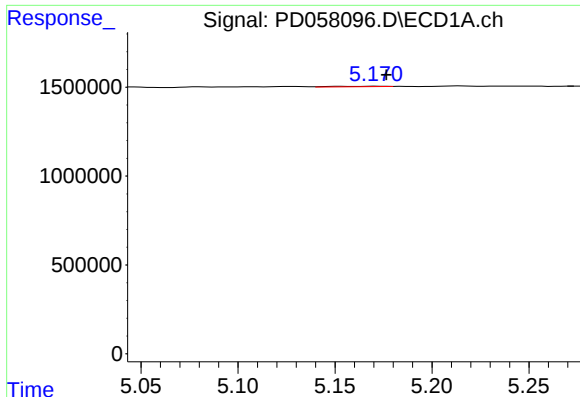

#9 Endosulfan I


R.T.: 5.171 min
Delta R.T.: -0.005 min
Response: 42129
Conc: 0.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB129082BL

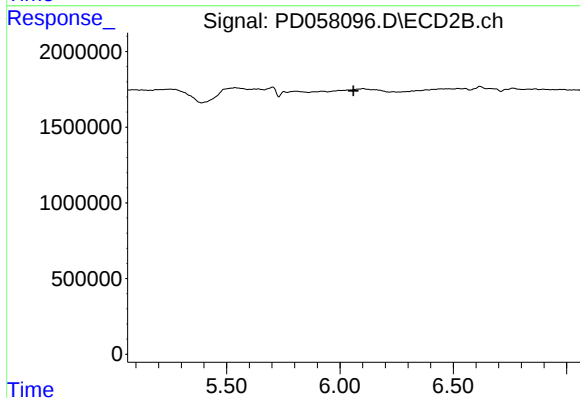


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.060 min
Response: 0
Conc: N.D.

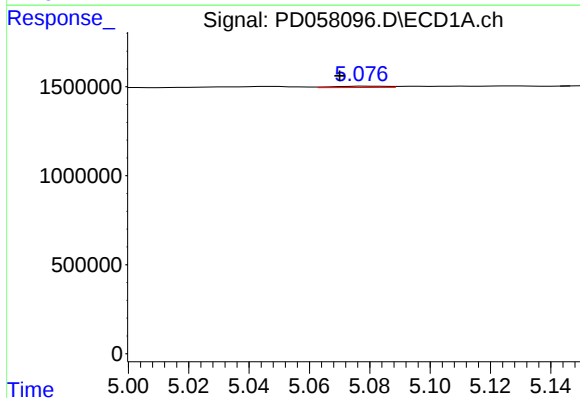


#10 gamma-Chlordane

R.T.: 5.079 min
Delta R.T.: 0.009 min
Response: 83666
Conc: 0.08 ng/ml

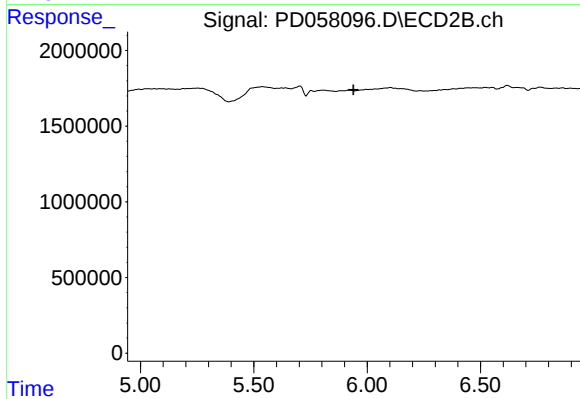

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.940 min
Response: 0
Conc: N.D.

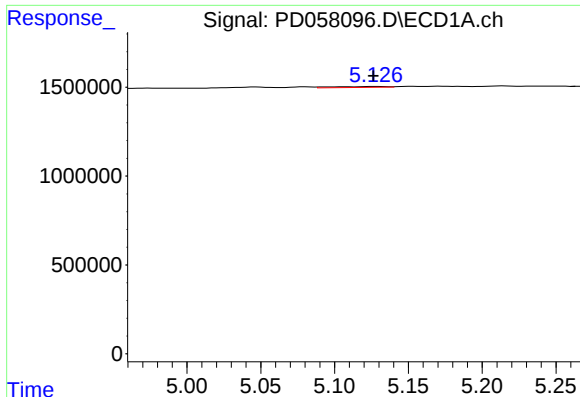

#11 alpha-Chlordane


R.T.: 5.128 min
Delta R.T.: 0.001 min
Response: 122462
Conc: 0.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB129082BL

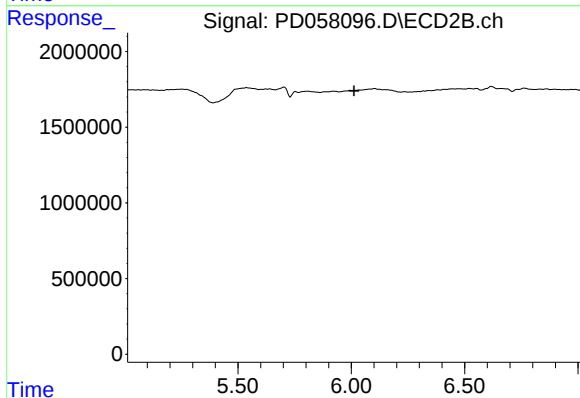


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.012 min
Response: 0
Conc: N.D.

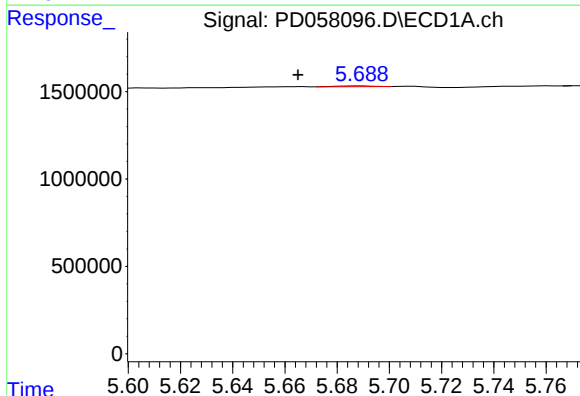


#14 Endrin

R.T.: 5.689 min
Delta R.T.: 0.024 min
Response: 38636
Conc: 0.05 ng/ml

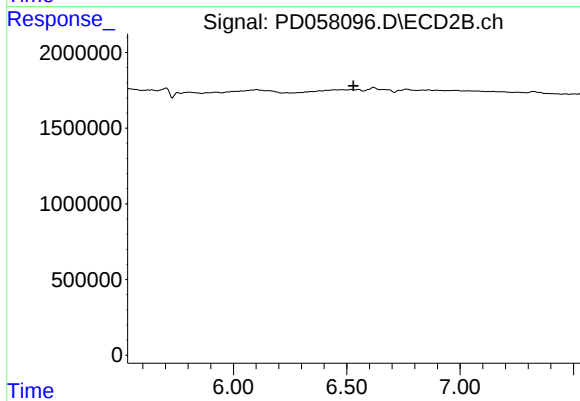

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.530 min
Response: 0
Conc: N.D.

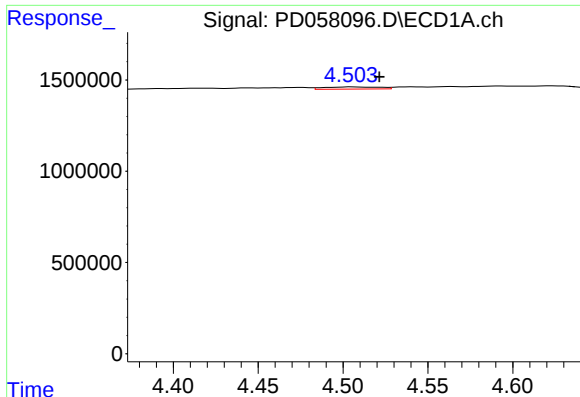

#24 Chlordane-2


R.T.: 4.505 min
Delta R.T.: -0.016 min
Response: 266433
Conc: 8.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB129082BL

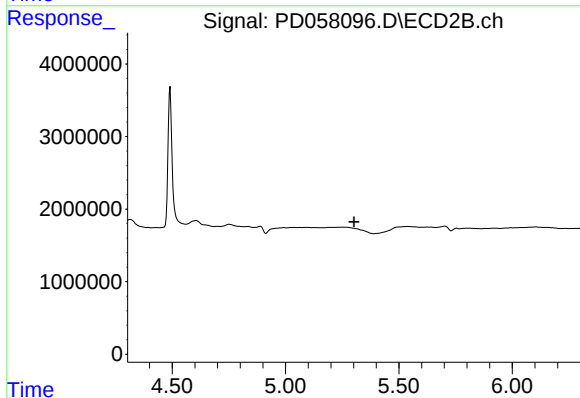


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.302 min
Response: 0
Conc: N.D.

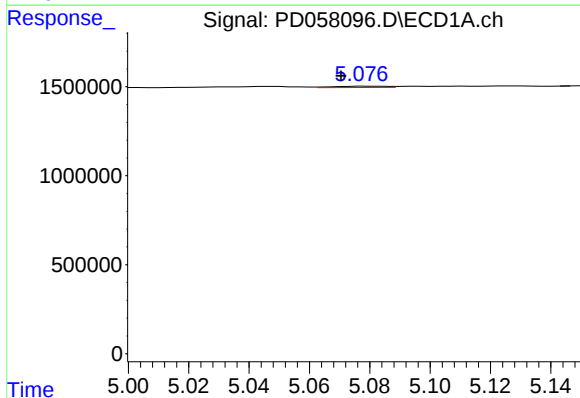


#25 Chlordane-3

R.T.: 5.079 min
Delta R.T.: 0.009 min
Response: 83666
Conc: 0.93 ng/ml

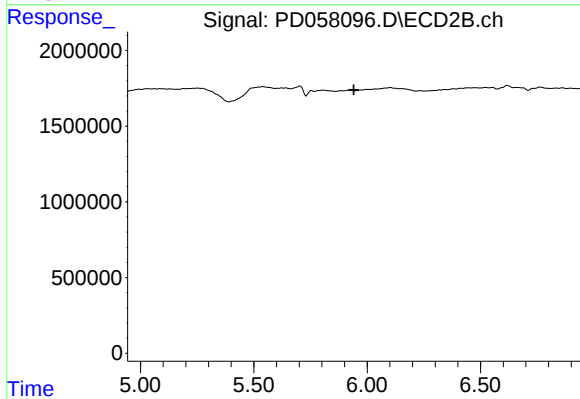

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.941 min
Response: 0
Conc: N.D.

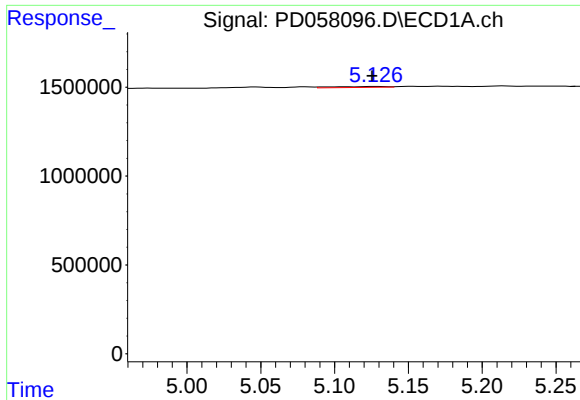

#26 Chlordane-4


R.T.: 5.128 min
Delta R.T.: 0.002 min
Response: 122462
Conc: 1.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB129082BL

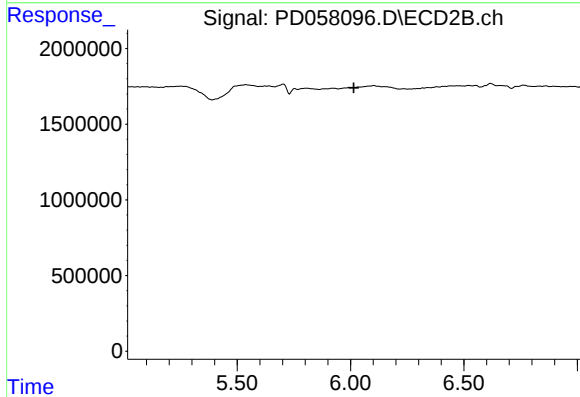


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.015 min
Response: 0
Conc: N.D.

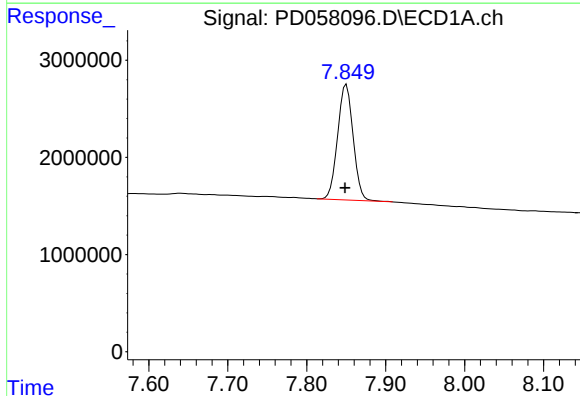

#28 Decachlorobiphenyl

R.T.: 7.850 min
Delta R.T.: 0.002 min
Response: 16194111
Conc: 20.25 ng/ml

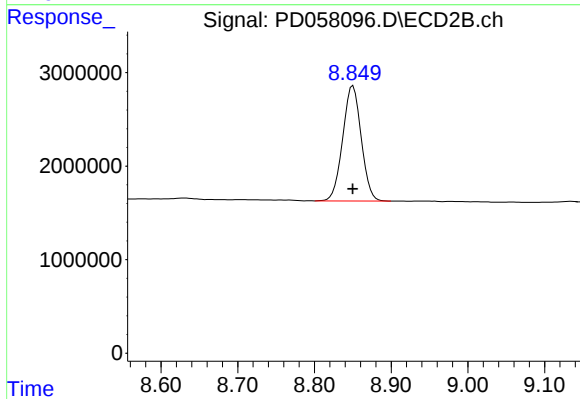

#28 Decachlorobiphenyl

R.T.: 8.850 min
Delta R.T.: 0.000 min
Response: 20710939
Conc: 19.98 ng/ml