

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052620\
 Data File : PD058095.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2020 15:16
 Operator : AJ\MA
 Sample : L2744-15
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 NM40-COMP-2020-0-6

Manual Integrations
 APPROVED

mohammad
 5/28/2020 10:37:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 04:59:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.866	9827383	14018718	12.574	12.309
28)	SA Decachlor...	7.851	8.850	10733373	14001245	13.424	13.505
Target Compounds							
12)	B 4,4'-DDE	5.299	6.170	1432948	1415654	1.539	1.108 #
17)	MA 4,4'-DDT	6.036	6.953	1501525	629558	2.177	0.632m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052620\
Data File : PD058095.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2020 15:16
Operator : AJ\MA
Sample : L2744-15
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
NM40-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/28/2020 10:37:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 04:59:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

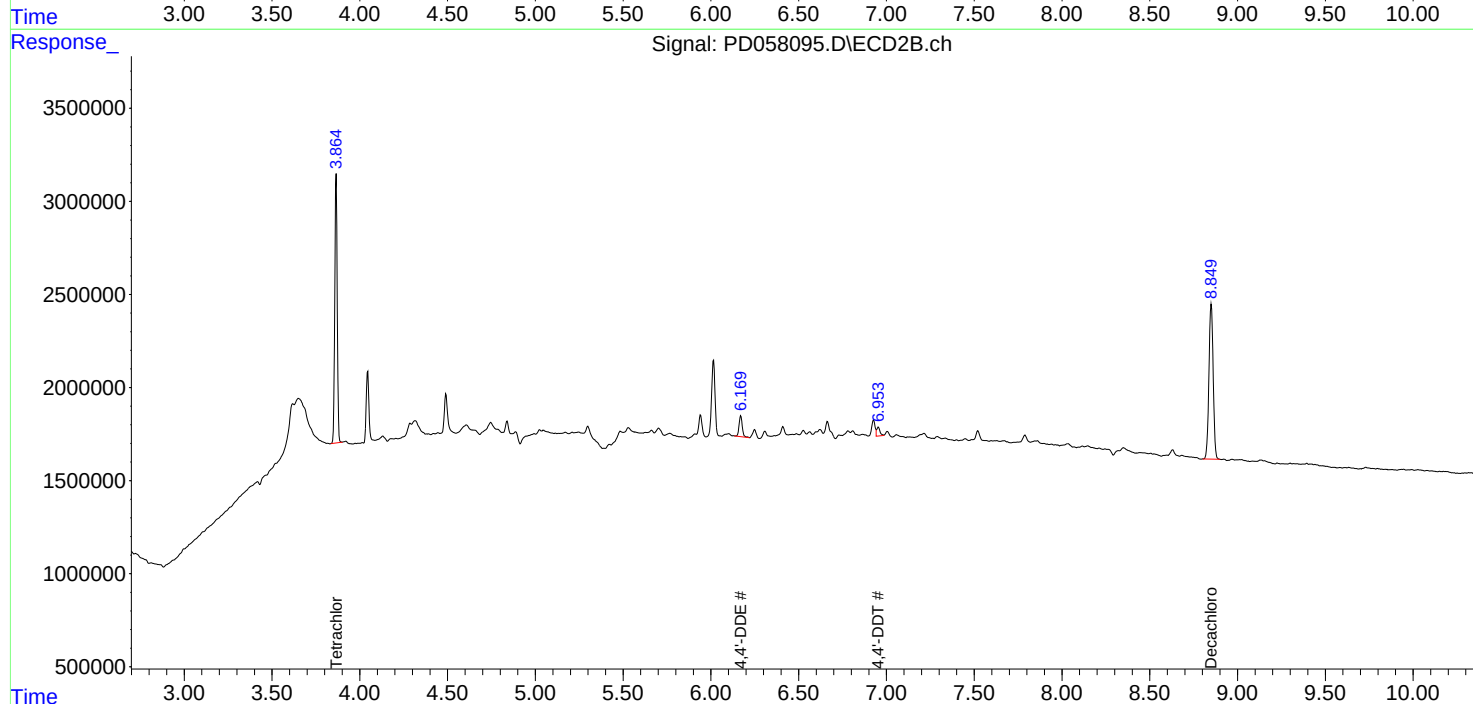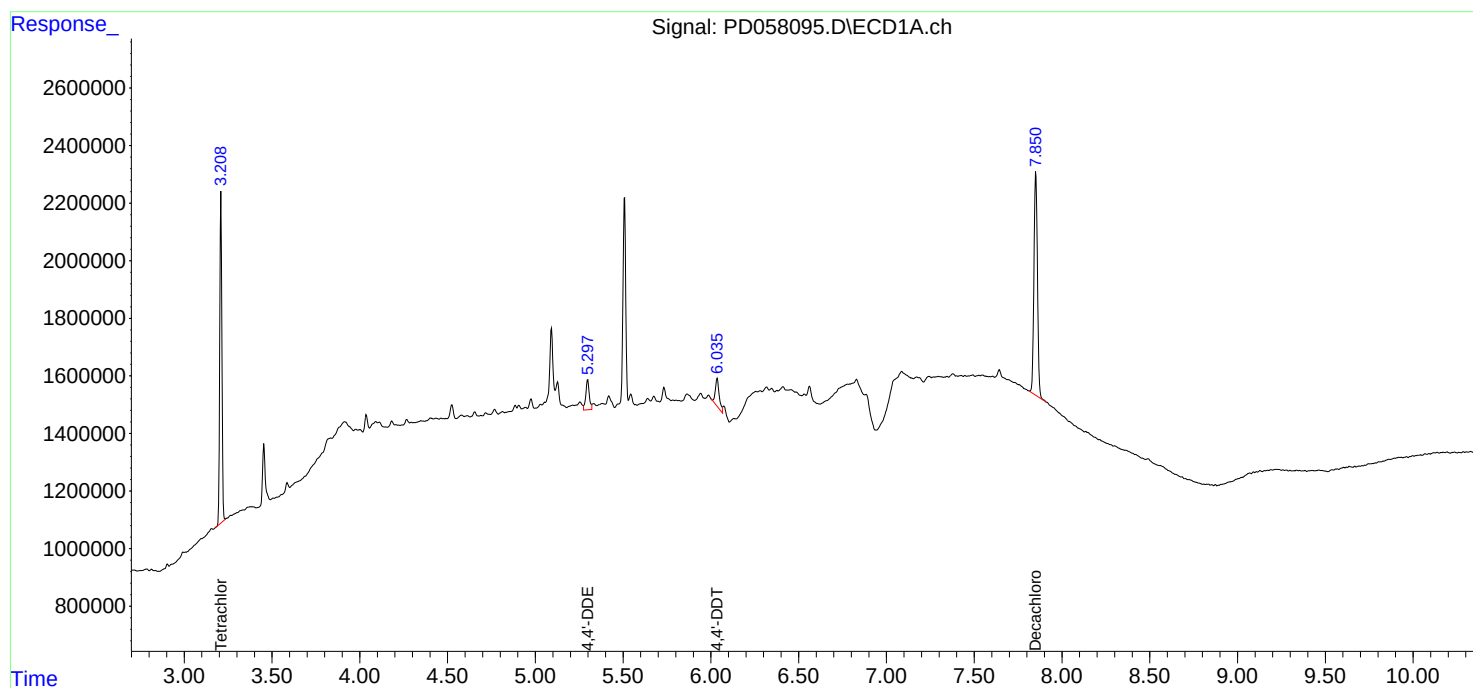

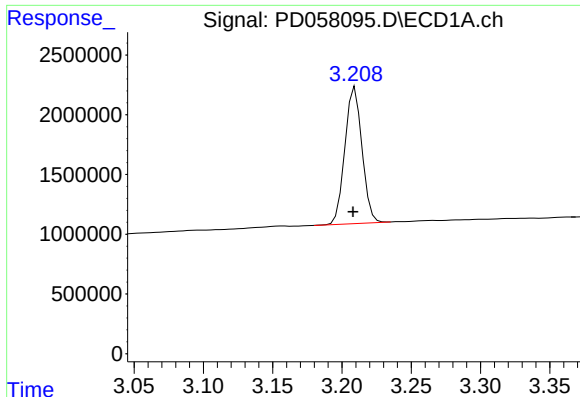


#1 Tetrachloro-m-xylene

R.T.: 3.210 min
Delta R.T.: 0.002 min
Response: 9827383
Conc: 12.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM40-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/28/2020 10:37:13 AM

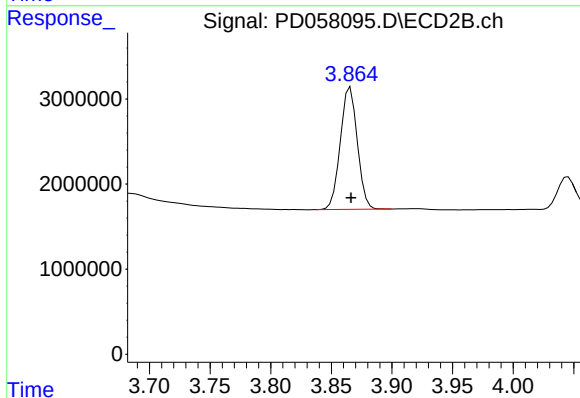


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 14018718
Conc: 12.31 ng/ml

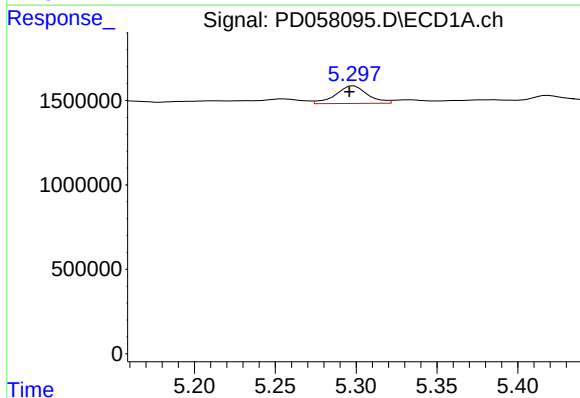


#12 4,4'-DDE

R.T.: 5.299 min
Delta R.T.: 0.003 min
Response: 1432948
Conc: 1.54 ng/ml

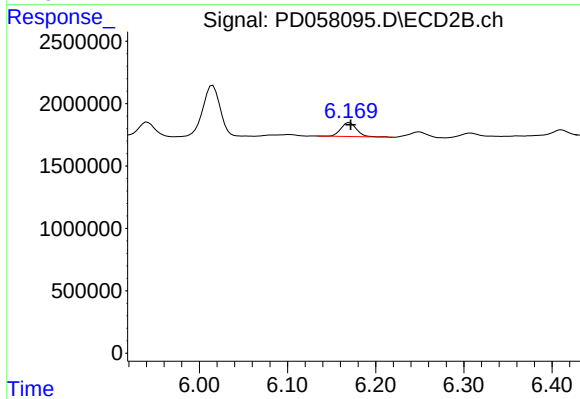

#12 4,4'-DDE

R.T.: 6.170 min
Delta R.T.: -0.001 min
Response: 1415654
Conc: 1.11 ng/ml

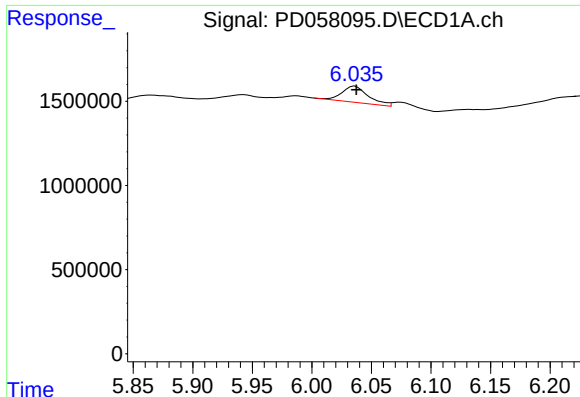


#17 4,4'-DDT

R.T.: 6.036 min
Delta R.T.: -0.001 min
Response: 1501525
Conc: 2.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM40-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/28/2020 10:37:13 AM

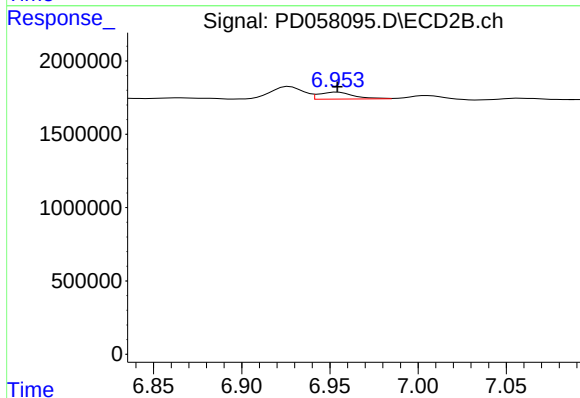


#17 4,4'-DDT

R.T.: 6.953 min
Delta R.T.: -0.001 min
Response: 629558
Conc: 0.63 ng/ml m

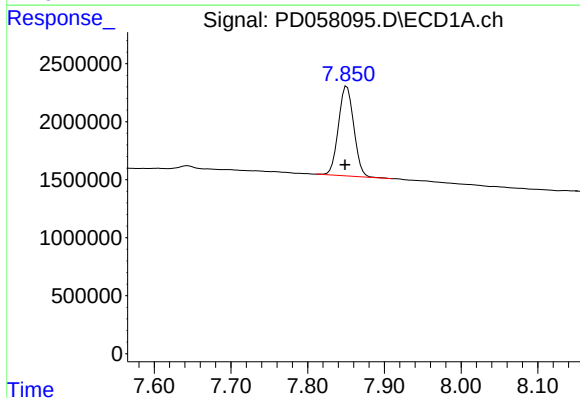

#28 Decachlorobiphenyl

R.T.: 7.851 min
Delta R.T.: 0.003 min
Response: 10733373
Conc: 13.42 ng/ml

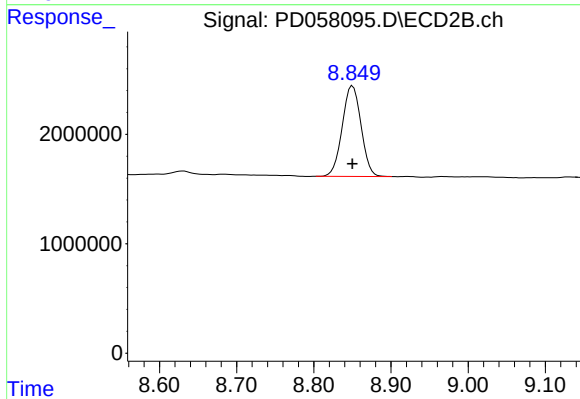

#28 Decachlorobiphenyl

R.T.: 8.850 min
Delta R.T.: 0.000 min
Response: 14001245
Conc: 13.51 ng/ml