

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052620\
 Data File : PD058110.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2020 18:49
 Operator : AJ\MA
 Sample : L2745-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 NM80-COMP-2020-0-6

Manual Integrations
 APPROVED

mohammad
 5/28/2020 10:37:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 05:04:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.209	3.867	7537728	10634072	9.645	9.337
28) SA Decachlor...	7.850	8.851	7070847	9134543	8.843	8.811
Target Compounds						
12) B 4,4'-DDE	5.295	6.172	1074553	1424258	1.154m	1.115
17) MA 4,4'-DDT	6.033	6.954	1166407	580671	1.691	0.583m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052620\
Data File : PD058110.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2020 18:49
Operator : AJ\MA
Sample : L2745-03
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
NM80-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/28/2020 10:37:44 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 05:04:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

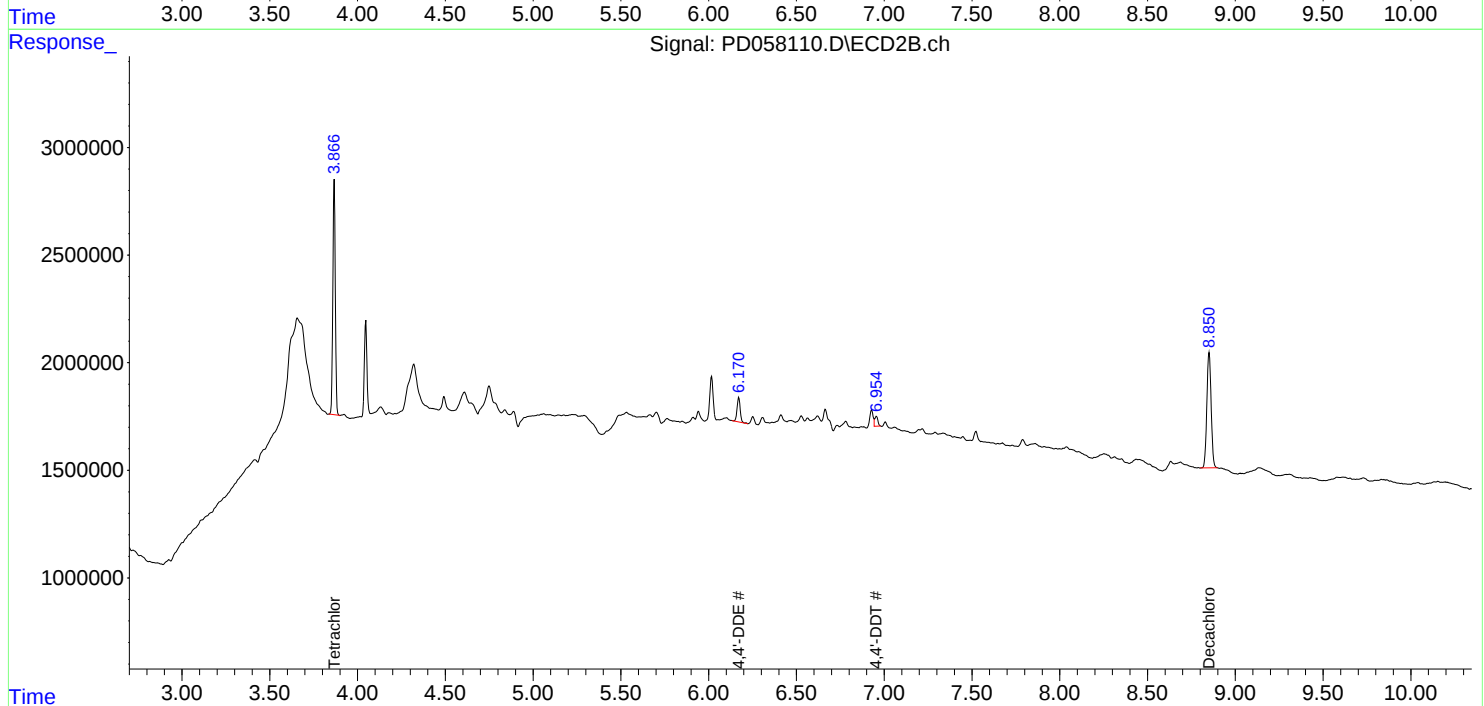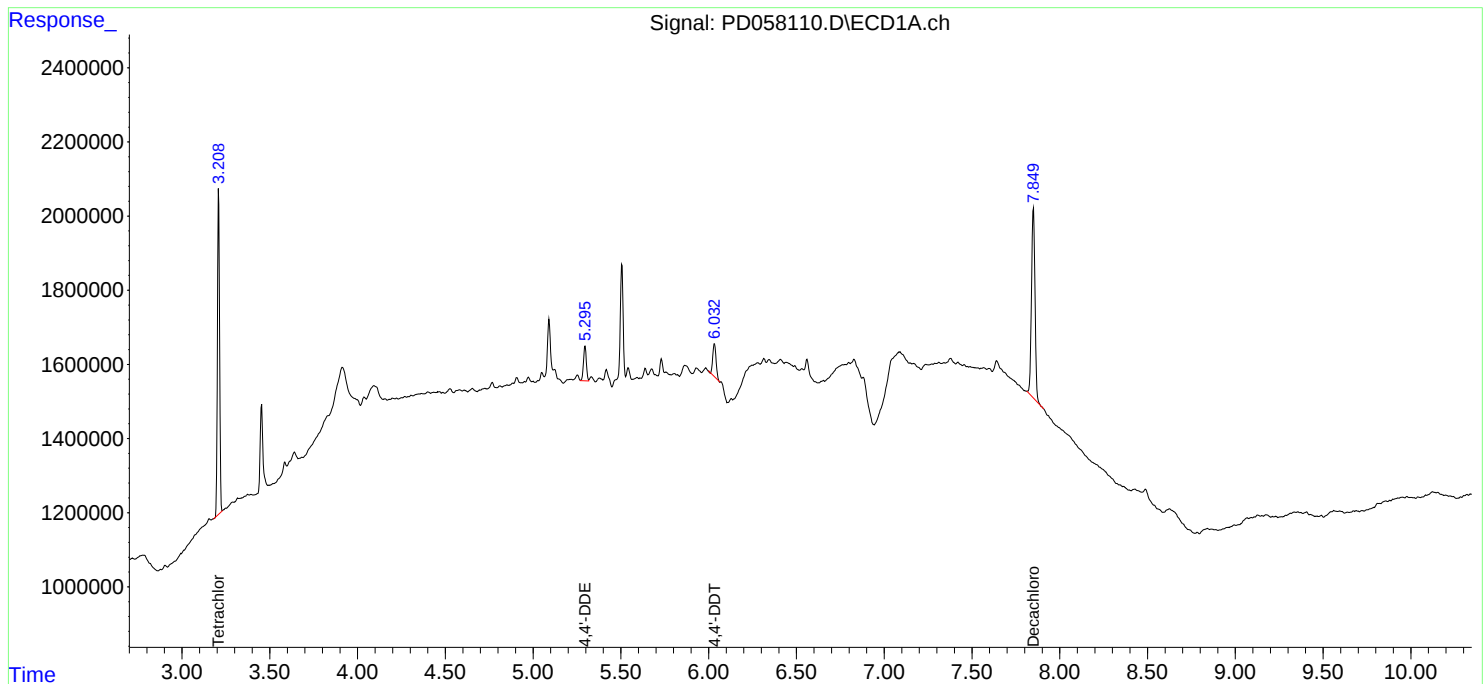

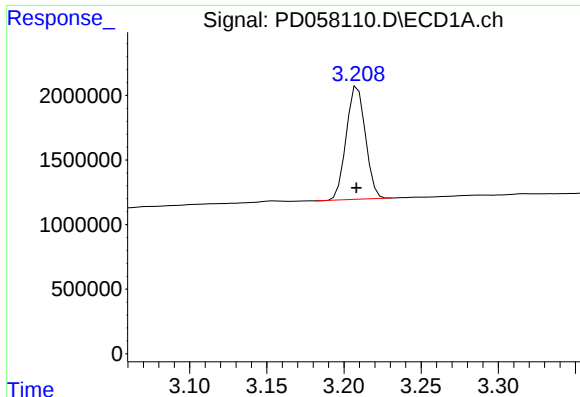


#1 Tetrachloro-m-xylene

R.T.: 3.209 min
Delta R.T.: 0.001 min
Response: 7537728
Conc: 9.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM80-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/28/2020 10:37:44 AM

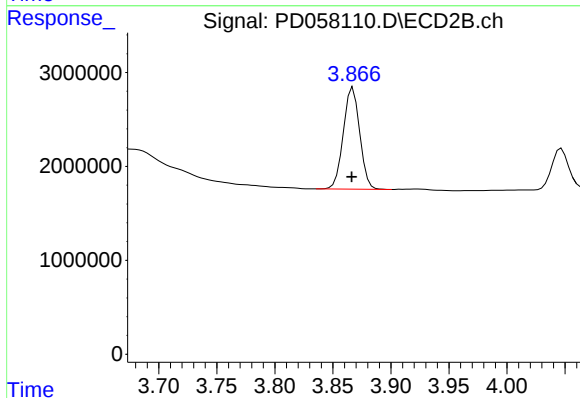


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.001 min
Response: 10634072
Conc: 9.34 ng/ml

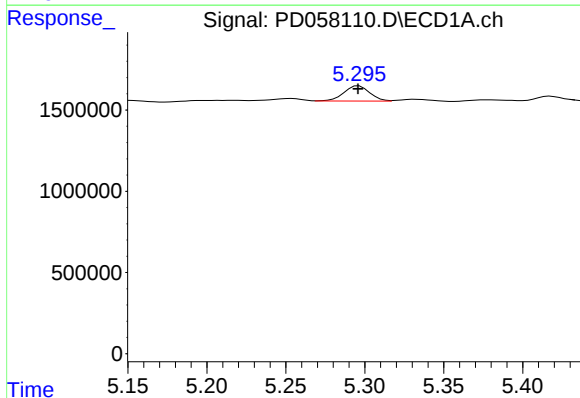


#12 4,4'-DDE

R.T.: 5.295 min
Delta R.T.: 0.000 min
Response: 1074553
Conc: 1.15 ng/ml m

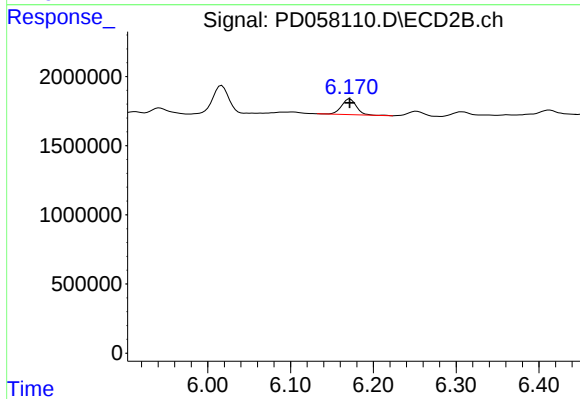

#12 4,4'-DDE

R.T.: 6.172 min
Delta R.T.: 0.000 min
Response: 1424258
Conc: 1.12 ng/ml

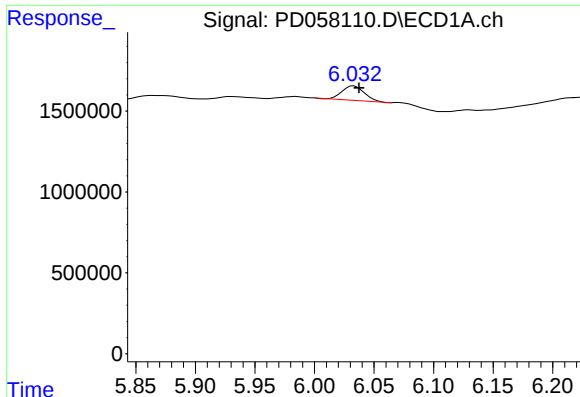


#17 4,4'-DDT

R.T.: 6.033 min
Delta R.T.: -0.004 min
Response: 1166407
Conc: 1.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM80-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/28/2020 10:37:44 AM

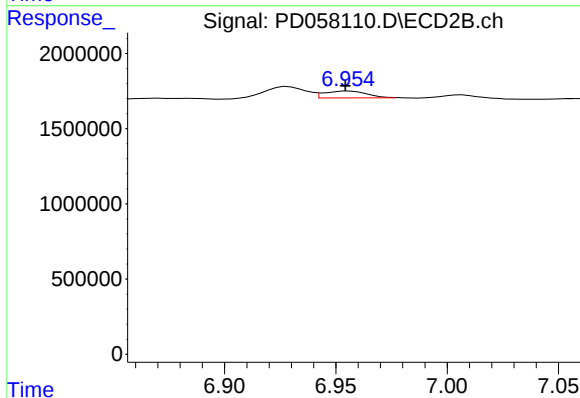


#17 4,4'-DDT

R.T.: 6.954 min
Delta R.T.: 0.000 min
Response: 580671
Conc: 0.58 ng/ml m

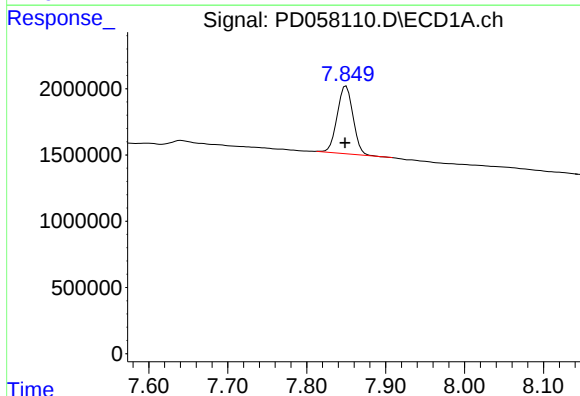

#28 Decachlorobiphenyl

R.T.: 7.850 min
Delta R.T.: 0.001 min
Response: 7070847
Conc: 8.84 ng/ml

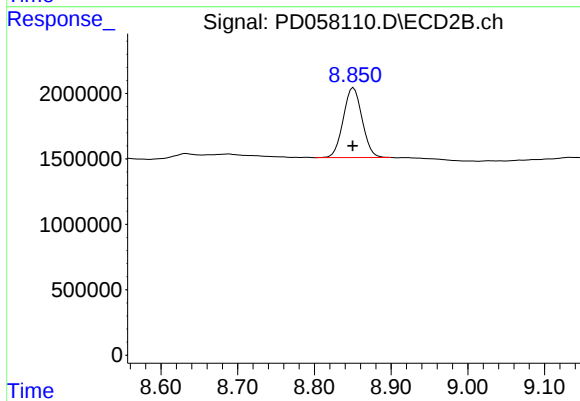

#28 Decachlorobiphenyl

R.T.: 8.851 min
Delta R.T.: 0.001 min
Response: 9134543
Conc: 8.81 ng/ml