

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052620\
 Data File : PD058115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2020 19:59
 Operator : AJ\MA
 Sample : L2745-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 NM63-COMP-2020-0-6

Manual Integrations
 APPROVED

mohammad
 5/28/2020 10:37:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 05:05:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.867	6592614	9161475	8.435	8.044
28)	SA Decachlor...	7.850	8.851	5274321	5931470	6.596	5.721m
Target Compounds							
12)	B 4,4'-DDE	5.295	6.171	477382	623165	0.513m	0.488m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052620\
Data File : PD058115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2020 19:59
Operator : AJ\MA
Sample : L2745-09
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
NM63-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/28/2020 10:37:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 05:05:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

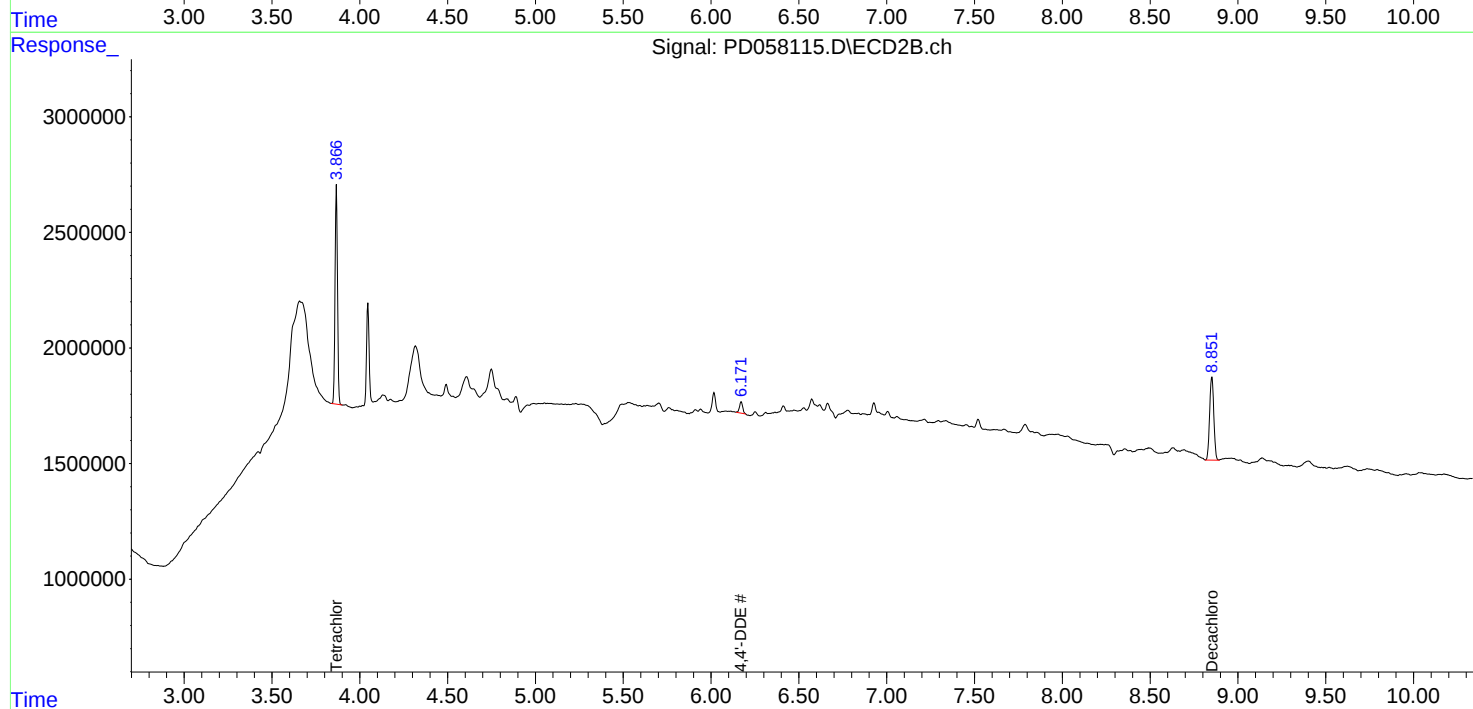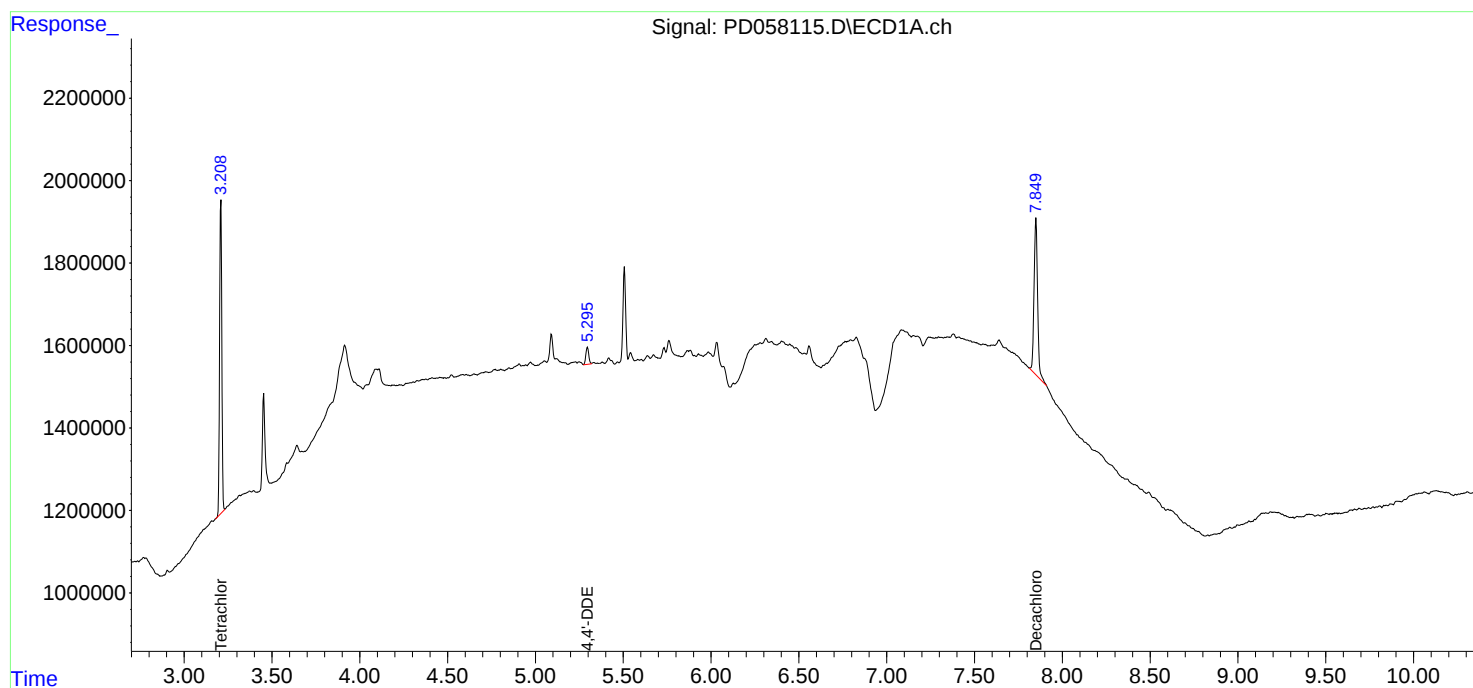

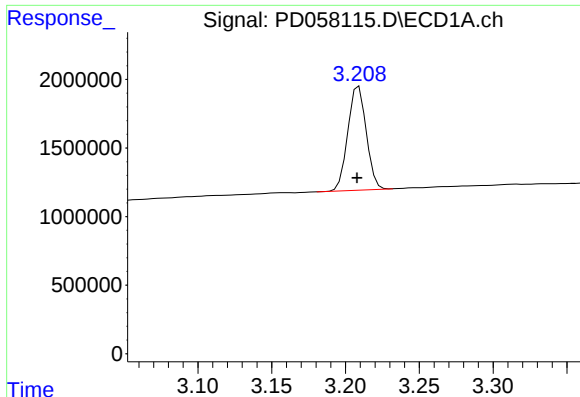


#1 Tetrachloro-m-xylene

R.T.: 3.209 min
Delta R.T.: 0.001 min
Response: 6592614
Conc: 8.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM63-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/28/2020 10:37:59 AM

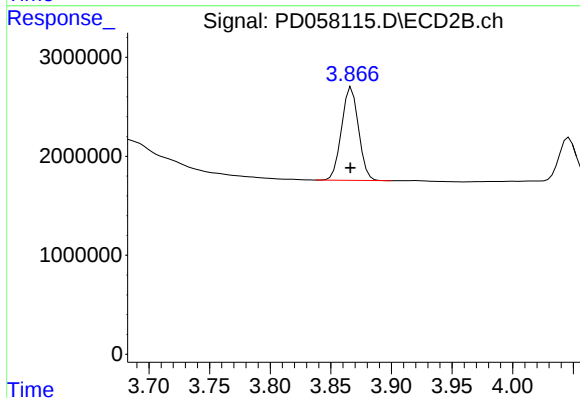


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 9161475
Conc: 8.04 ng/ml

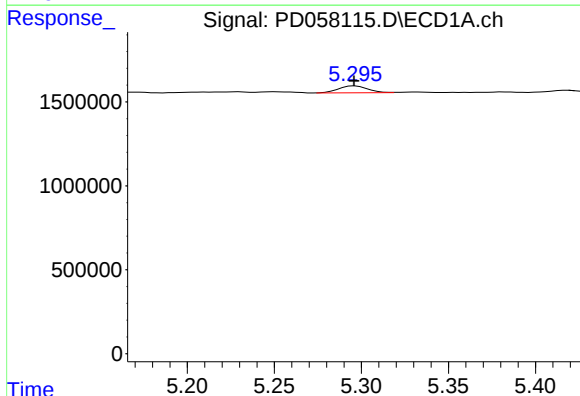


#12 4,4'-DDE

R.T.: 5.295 min
Delta R.T.: 0.000 min
Response: 477382
Conc: 0.51 ng/ml m

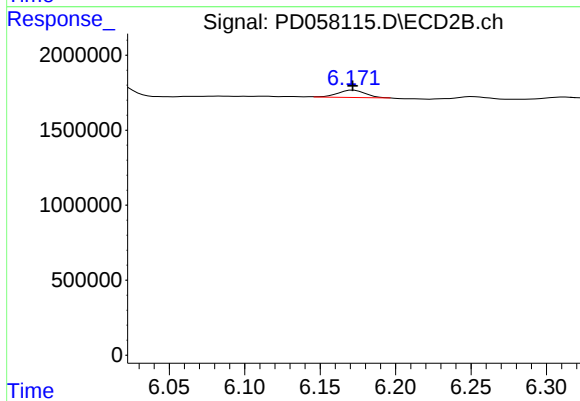

#12 4,4'-DDE

R.T.: 6.171 min
Delta R.T.: -0.001 min
Response: 623165
Conc: 0.49 ng/ml m

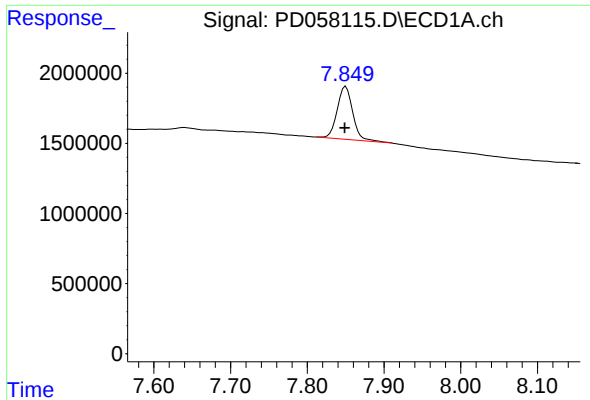


#28 Decachlorobiphenyl

R.T.: 7.850 min
Delta R.T.: 0.002 min
Response: 5274321
Conc: 6.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM63-COMP-2020-0-6

Manual Integrations
APPROVED

mohammad
5/28/2020 10:37:59 AM

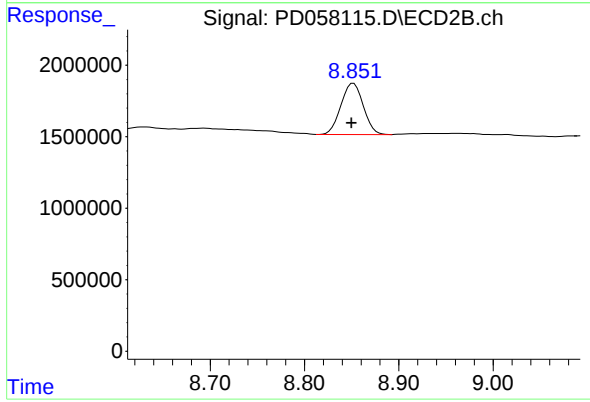

#28 Decachlorobiphenyl

R.T.: 8.851 min
Delta R.T.: 0.000 min
Response: 5931470
Conc: 5.72 ng/ml m