

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052620\
 Data File : PD058118.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2020 20:42
 Operator : AJ\MA
 Sample : L2745-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 NM23-COMP-2020-0-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 05:07:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.229f	3.867	7381843	10400293	9.445	9.132
28)	SA Decachlor...	7.869f	8.851	6819297	8133831	8.529	7.846

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052620\
Data File : PD058118.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2020 20:42
Operator : AJ\MA
Sample : L2745-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
NM23-COMP-2020-0-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 05:07:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

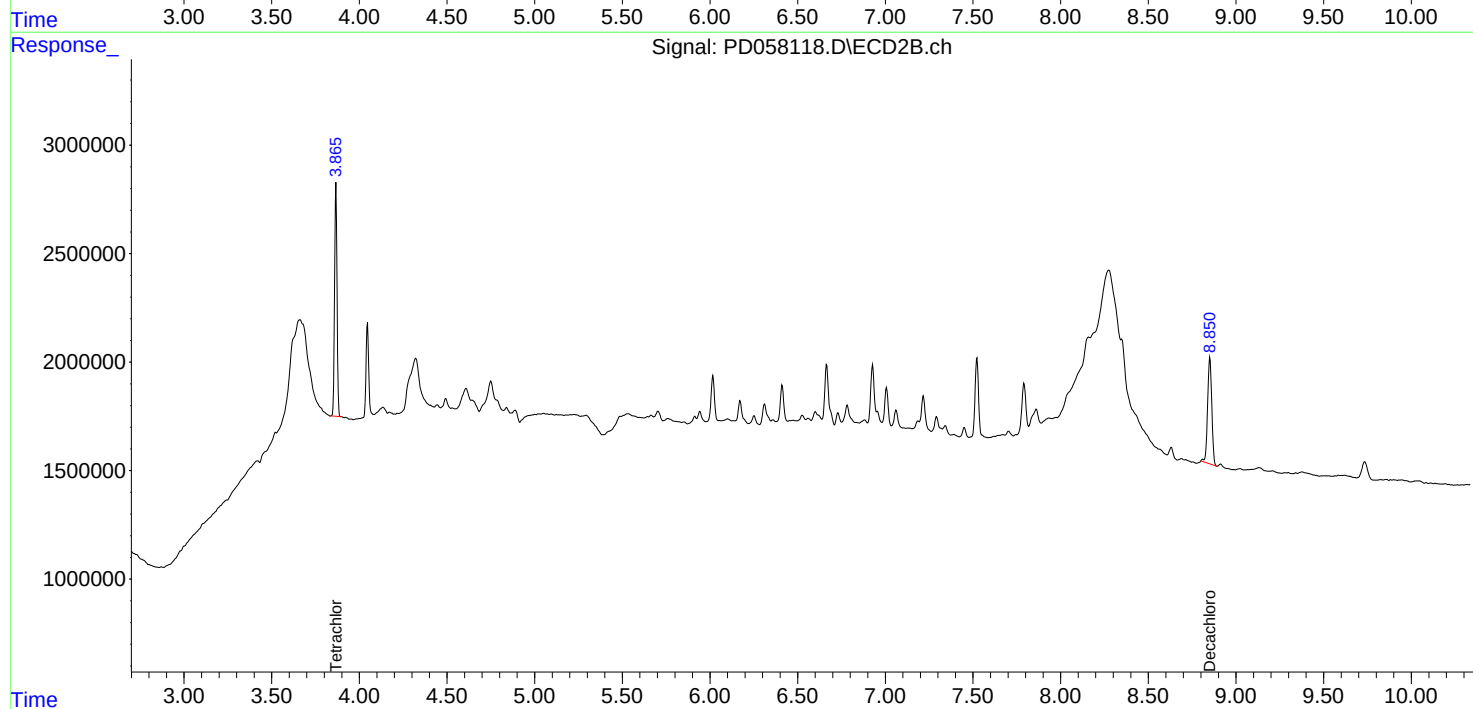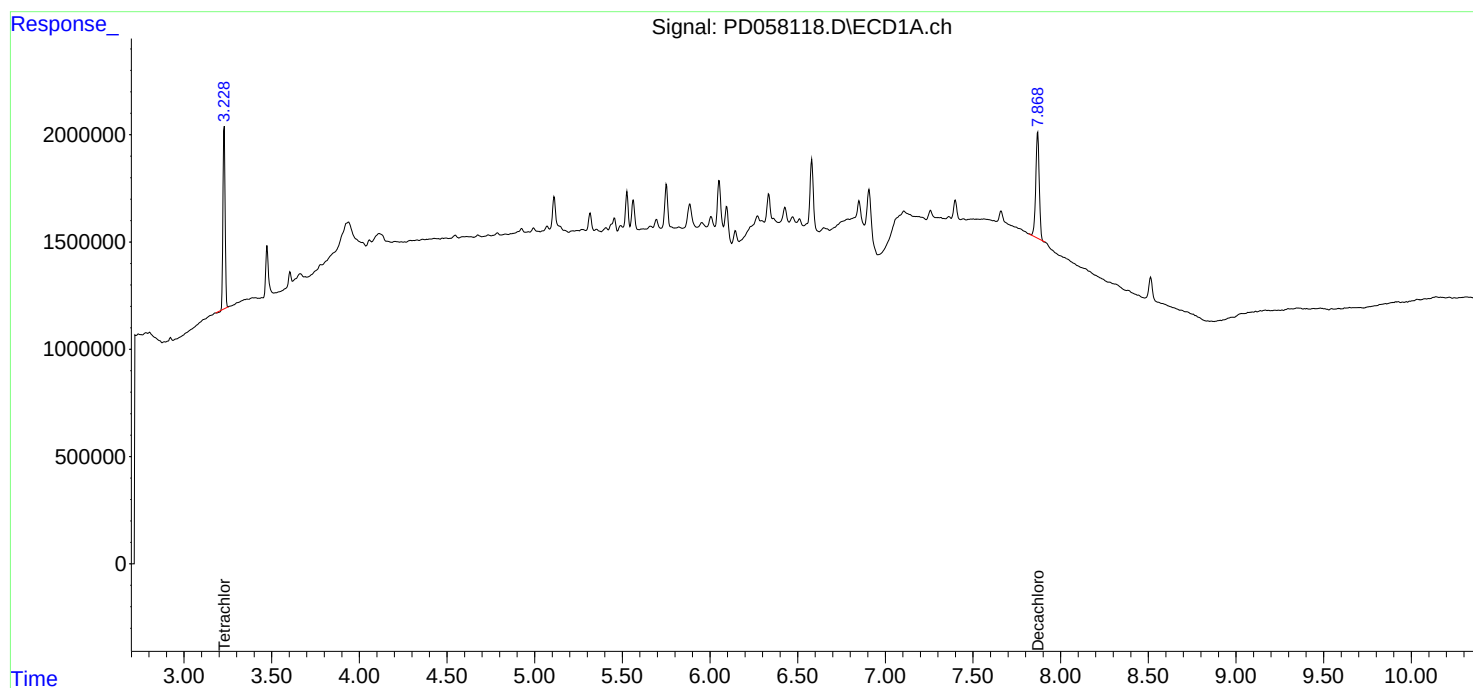


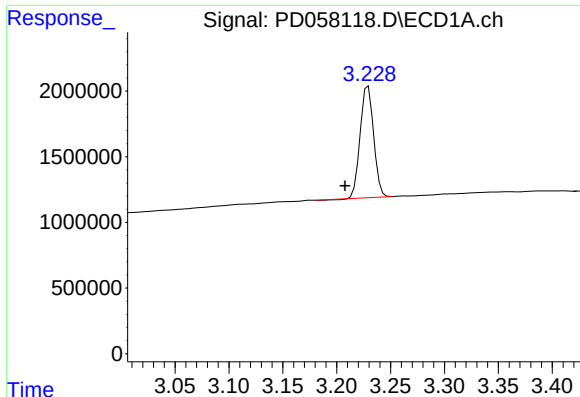

#1 Tetrachloro-m-xylene


R.T.: 3.229 min
Delta R.T.: 0.021 min
Response: 7381843
Conc: 9.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM23-COMP-2020-0-6

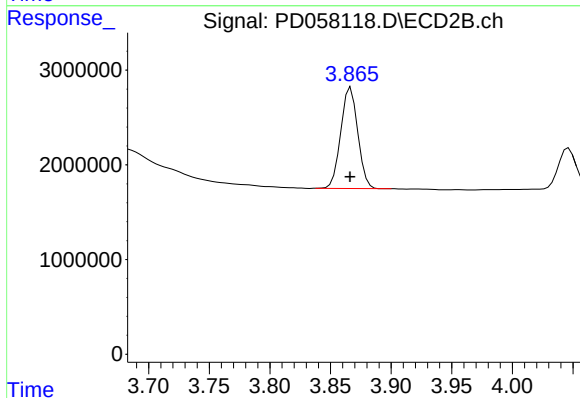


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 10400293
Conc: 9.13 ng/ml

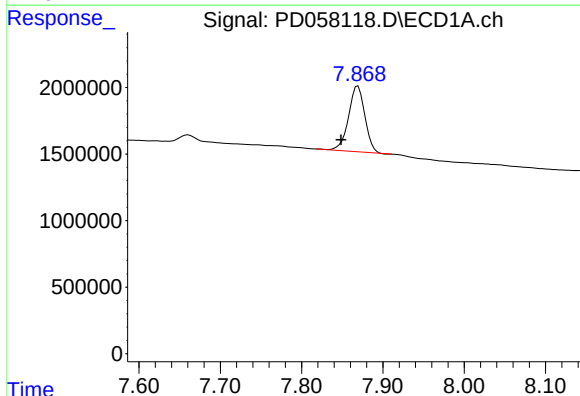

#28 Decachlorobiphenyl

R.T.: 7.869 min
Delta R.T.: 0.021 min
Response: 6819297
Conc: 8.53 ng/ml

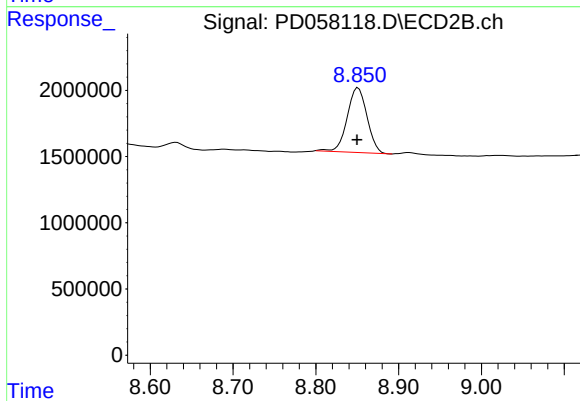

#28 Decachlorobiphenyl

R.T.: 8.851 min
Delta R.T.: 0.001 min
Response: 8133831
Conc: 7.85 ng/ml