

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052620\
 Data File : PD058119.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2020 20:56
 Operator : AJ\MA
 Sample : L2745-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 NM36-COMP-2020-0-6

Manual Integrations
 APPROVED

mohammad
 5/28/2020 10:38:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 05:08:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.867	4730263	6598486	6.053	5.794
28)	SA Decachlor...	7.850	8.850	3421117	4045472	4.279	3.902
Target Compounds							
12)	B 4,4'-DDE	5.296	6.170	416665	681094	0.447	0.533m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052620\
Data File : PD058119.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2020 20:56
Operator : AJ\MA
Sample : L2745-16
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
NM36-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/28/2020 10:38:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 05:08:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

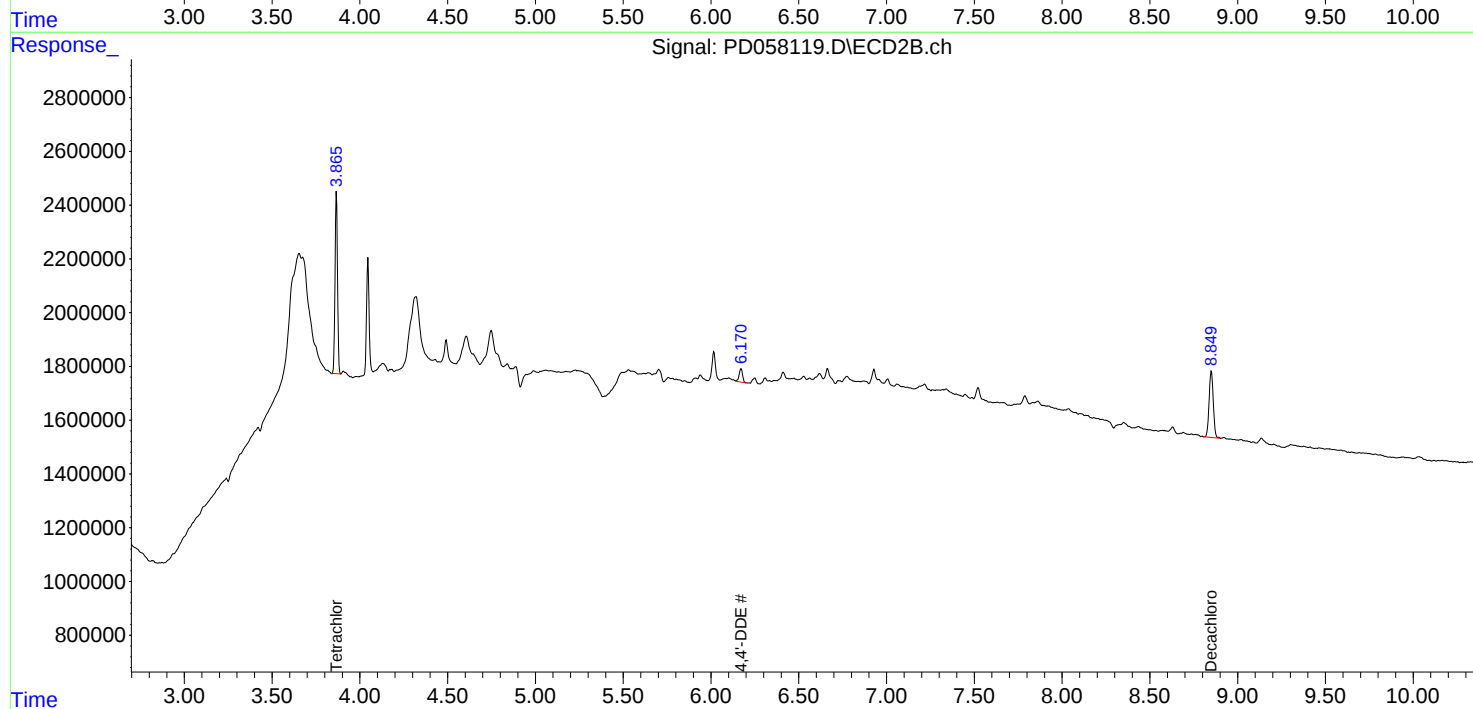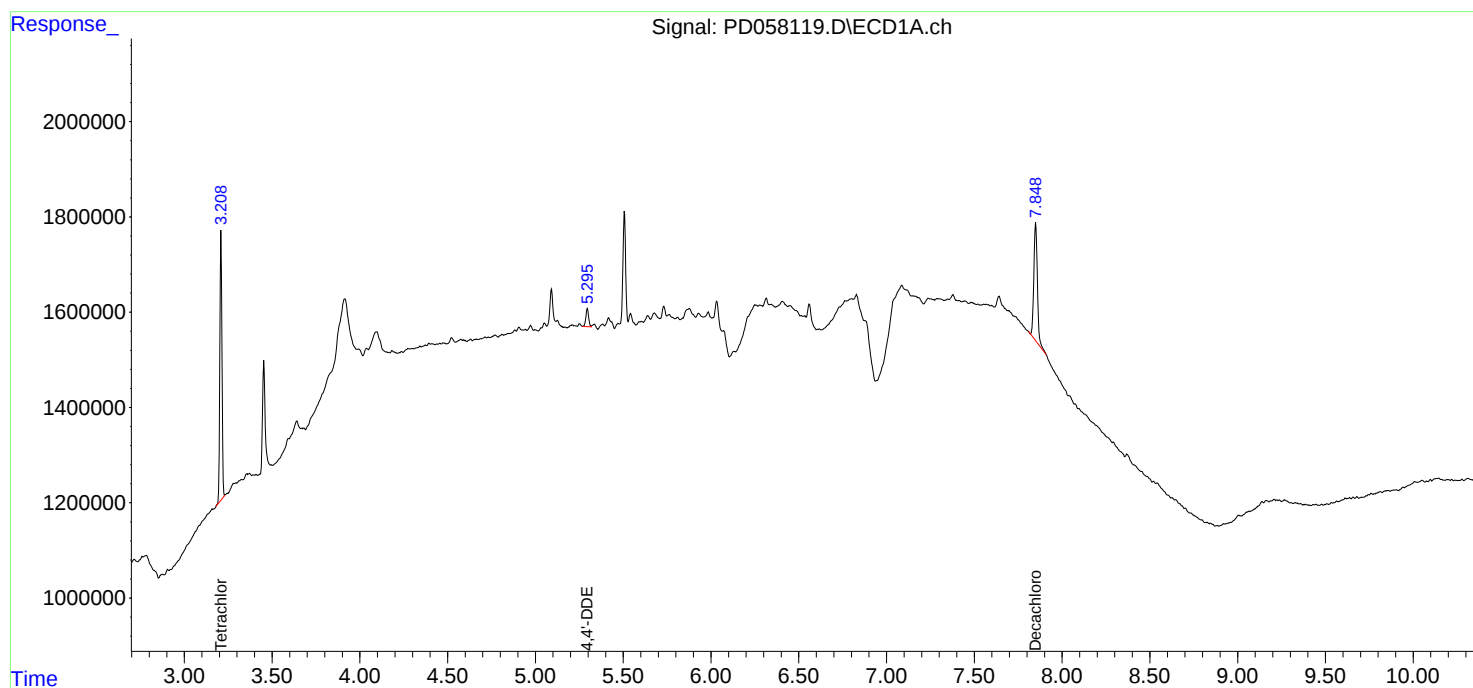

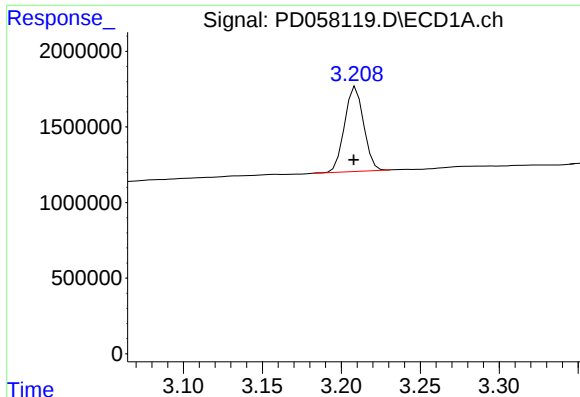


#1 Tetrachloro-m-xylene

R.T.: 3.209 min
Delta R.T.: 0.001 min
Response: 4730263
Conc: 6.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM36-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/28/2020 10:38:08 AM

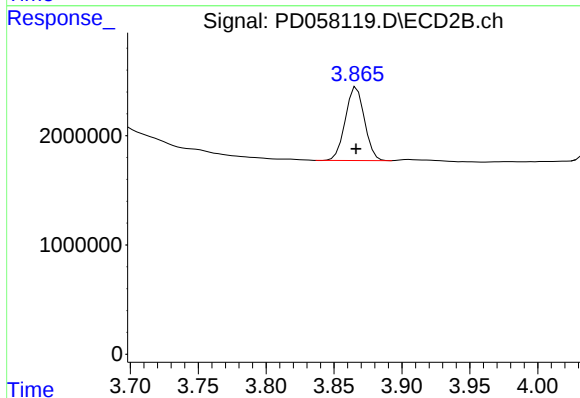


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 6598486
Conc: 5.79 ng/ml

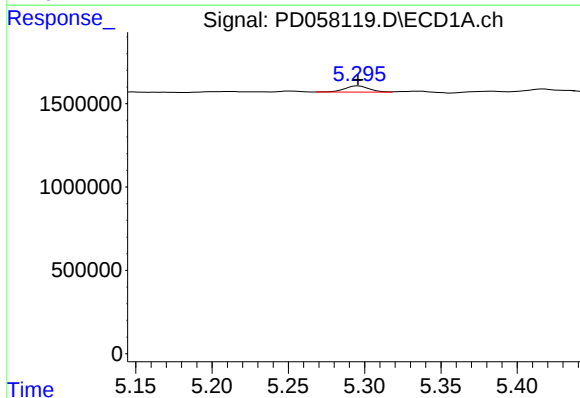


#12 4,4'-DDE

R.T.: 5.296 min
Delta R.T.: 0.000 min
Response: 416665
Conc: 0.45 ng/ml

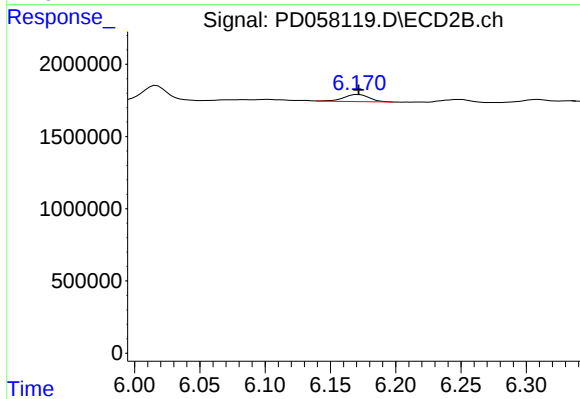

#12 4,4'-DDE

R.T.: 6.170 min
Delta R.T.: -0.002 min
Response: 681094
Conc: 0.53 ng/ml m

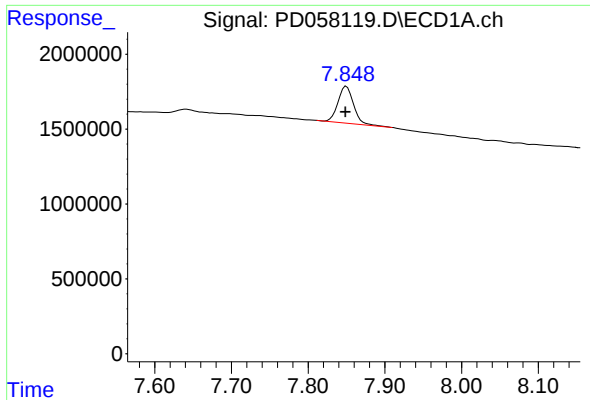


#28 Decachlorobiphenyl

R.T.: 7.850 min
Delta R.T.: 0.001 min
Response: 3421117
Conc: 4.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM36-COMP-2020-0-6

Manual Integrations
APPROVED

mohammad
5/28/2020 10:38:08 AM

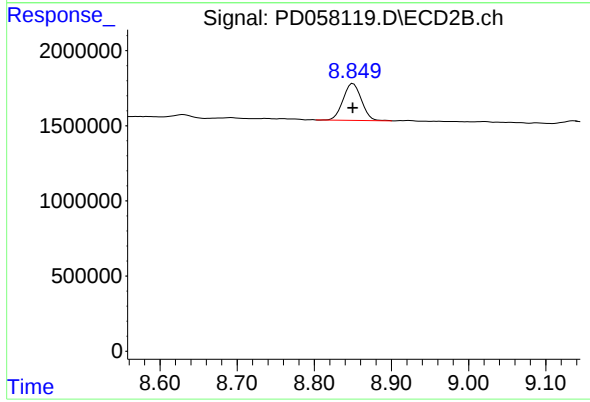

#28 Decachlorobiphenyl

R.T.: 8.850 min
Delta R.T.: 0.000 min
Response: 4045472
Conc: 3.90 ng/ml