

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052621\
 Data File : PD063295.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2021 13:43
 Operator : AR\AJ
 Sample : M2521-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HR-03-052521

Manual Integrations
 APPROVED

Ankita
 5/27/2021 2:14:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 05:52:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Mon May 24 14:48:18 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.969	13004890	107.7E6	11.806	9.297m
28)	SA Decachlor...	8.197	9.026	25169959	119.4E6	19.999	11.707 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052621\
Data File : PD063295.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2021 13:43
Operator : AR\AJ
Sample : M2521-03
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
HR-03-052521


Manual Integrations
APPROVED

Ankita
5/27/2021 2:14:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 05:52:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Mon May 24 14:48:18 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

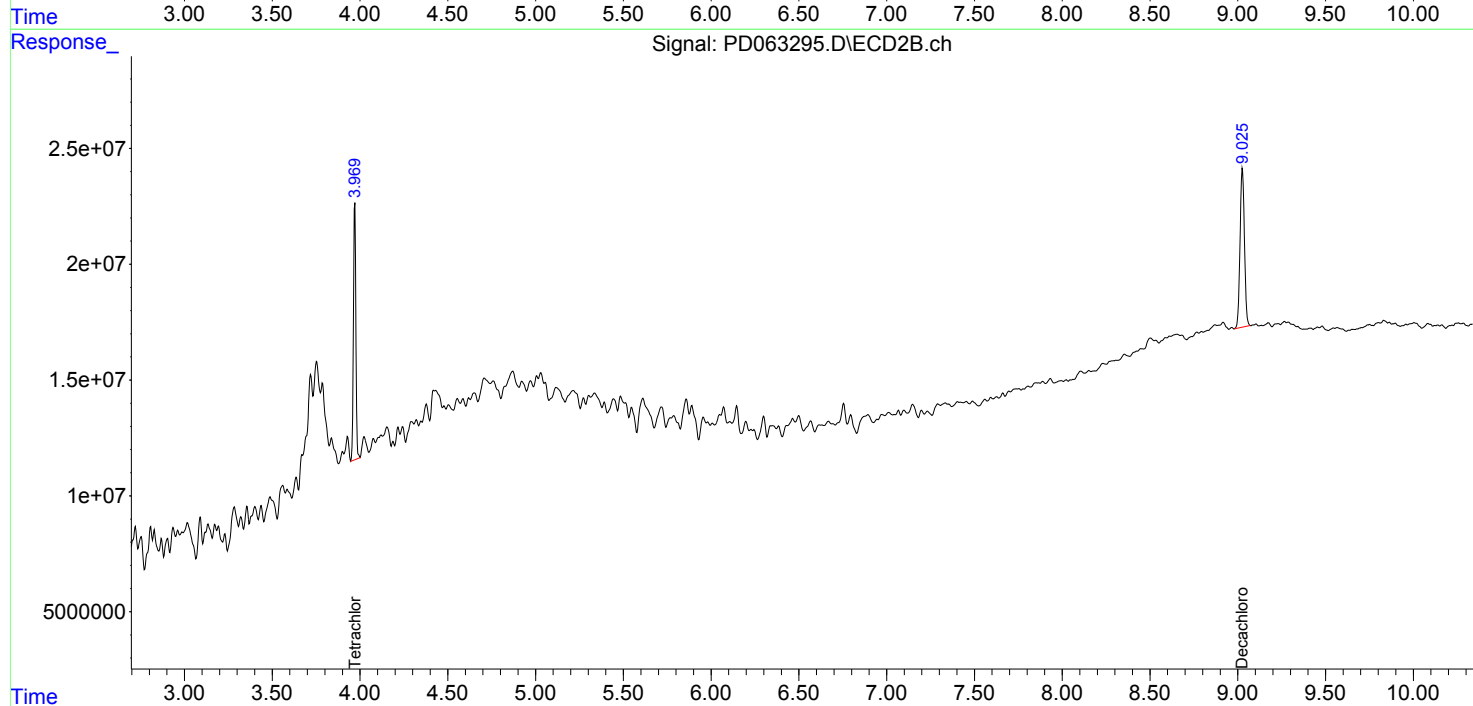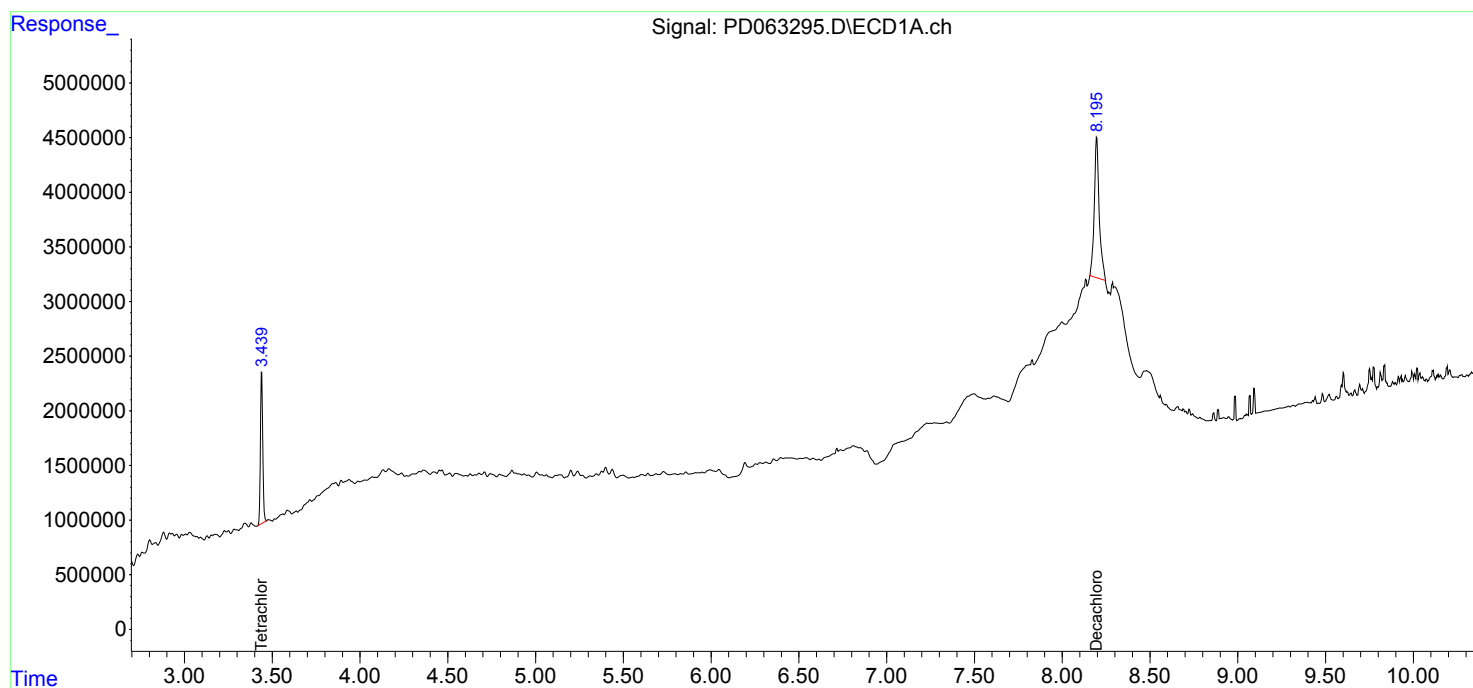

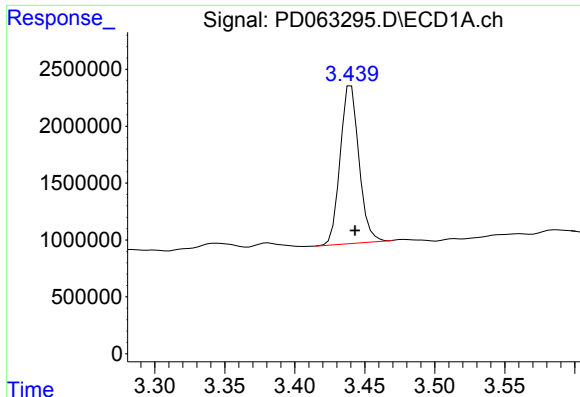


#1 Tetrachloro-m-xylene

R.T.: 3.440 min
Delta R.T.: -0.003 min
Response: 13004890
Conc: 11.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
HR-03-052521


Manual Integrations
APPROVED

Ankita
5/27/2021 2:14:29 PM

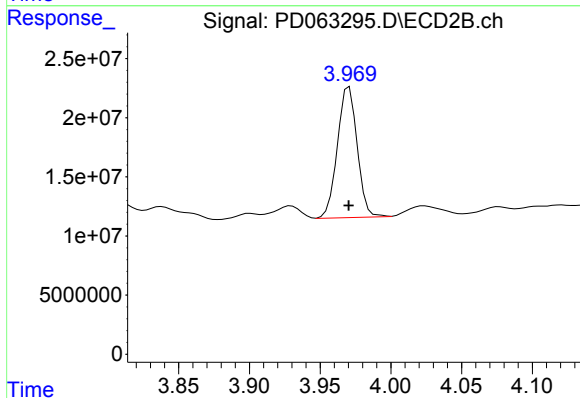


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 107735242
Conc: 9.30 ng/ml m

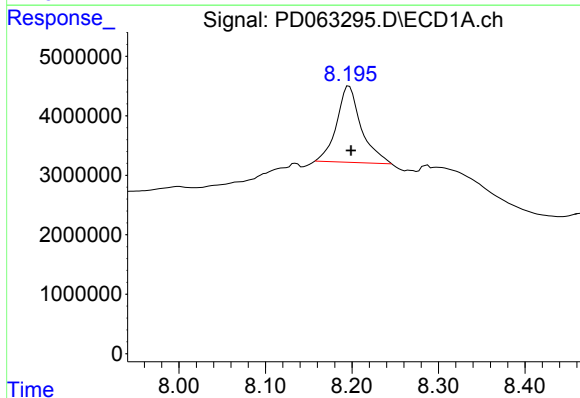

#28 Decachlorobiphenyl

R.T.: 8.197 min
Delta R.T.: -0.002 min
Response: 25169959
Conc: 20.00 ng/ml

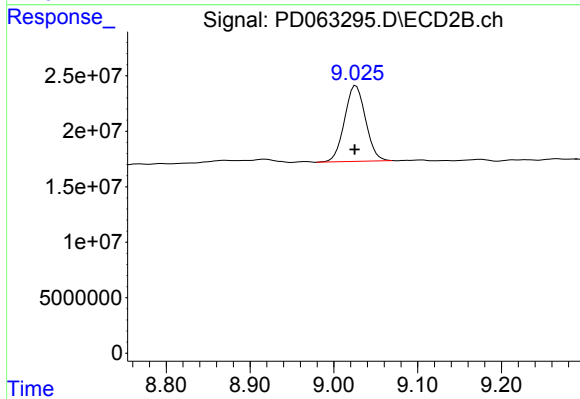

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: 0.001 min
Response: 119431558
Conc: 11.71 ng/ml