

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052621\
 Data File : PD063299.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2021 16:12
 Operator : AR\AJ
 Sample : M2521-01 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HR-01-052521

Manual Integrations
 APPROVED

Ankita
 5/27/2021 2:14:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 05:53:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Mon May 24 14:48:18 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.445	3.971	1881582	17685477	1.708	1.526
28) SA Decachlor...	8.204	9.029	2107190	16767549	1.674	1.644
Target Compounds						
12) B 4,4'-DDE	5.606	6.306	697551	10986770	0.486m	0.728 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052621\
Data File : PD063299.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2021 16:12
Operator : AR\AJ
Sample : M2521-01 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
HR-01-052521


Manual Integrations
APPROVED

Ankita
5/27/2021 2:14:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 05:53:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Mon May 24 14:48:18 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

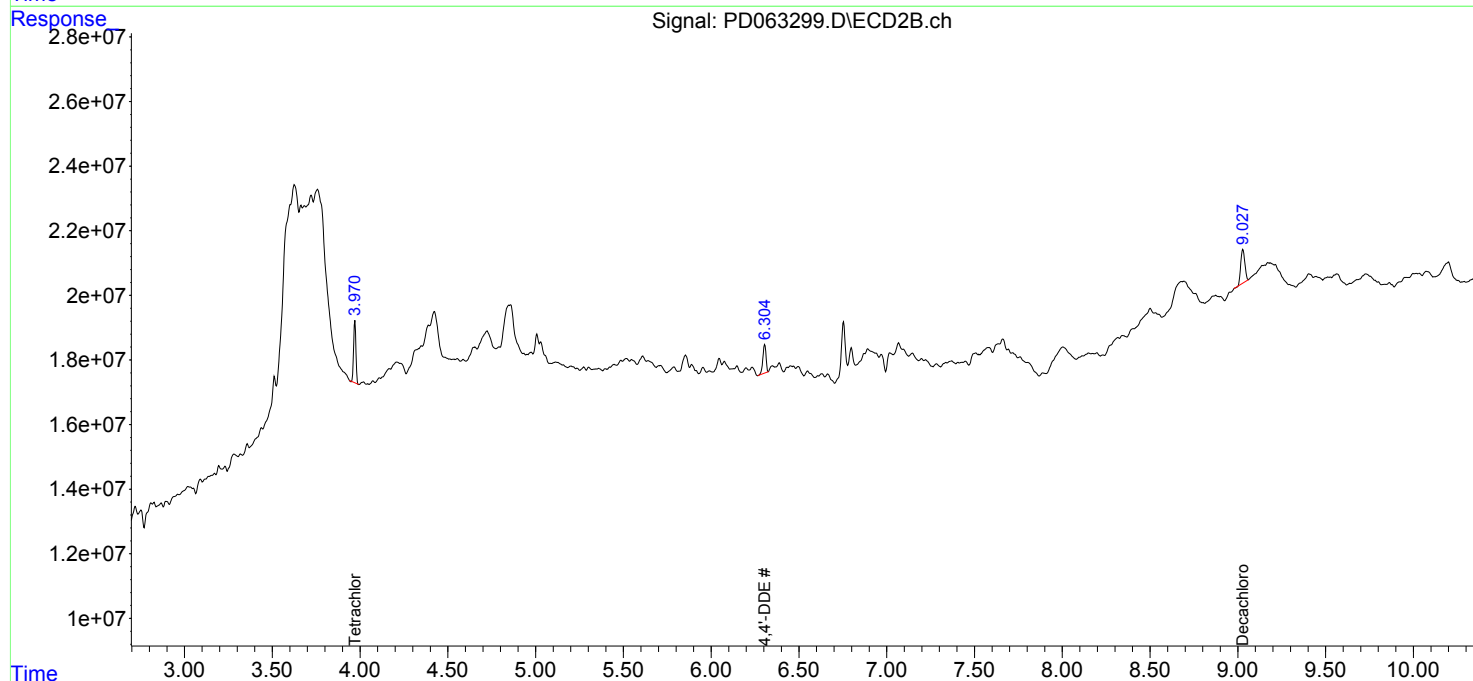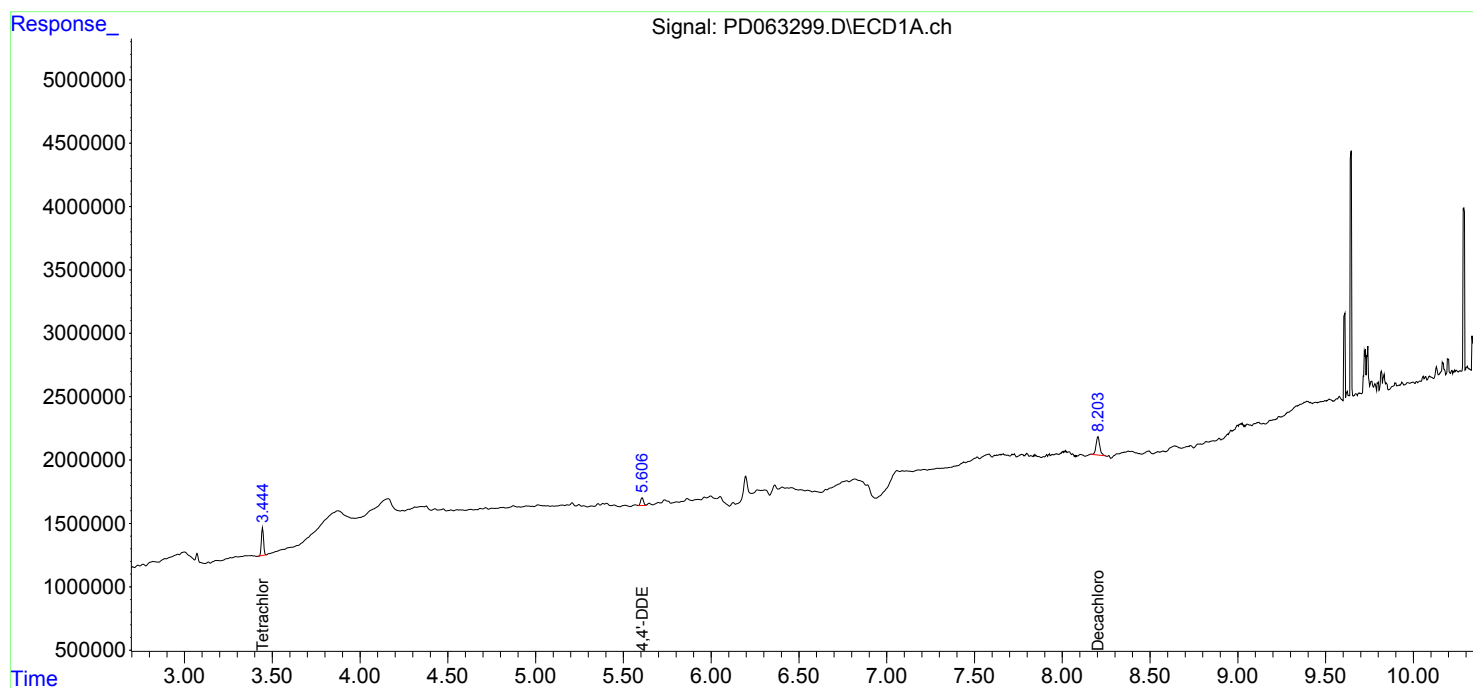

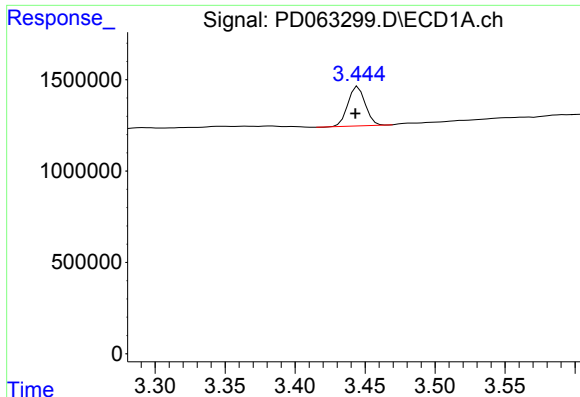


#1 Tetrachloro-m-xylene

R.T.: 3.445 min
Delta R.T.: 0.002 min
Response: 1881582
Conc: 1.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
HR-01-052521


Manual Integrations
APPROVED

Ankita
5/27/2021 2:14:34 PM

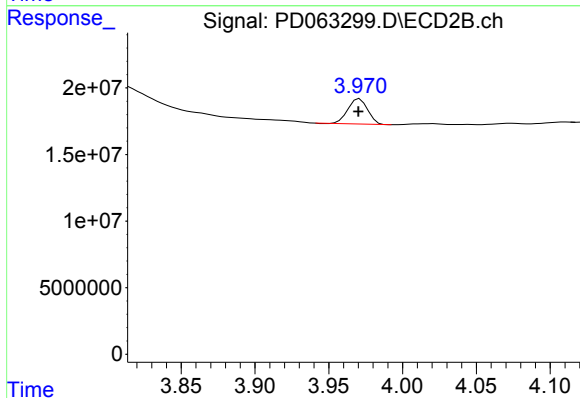


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 17685477
Conc: 1.53 ng/ml

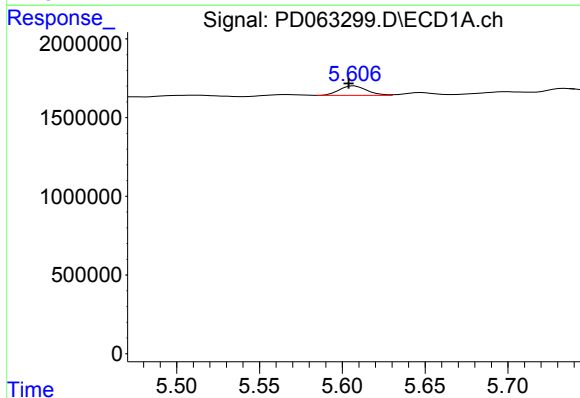


#12 4,4'-DDE

R.T.: 5.606 min
Delta R.T.: 0.002 min
Response: 697551
Conc: 0.49 ng/ml m

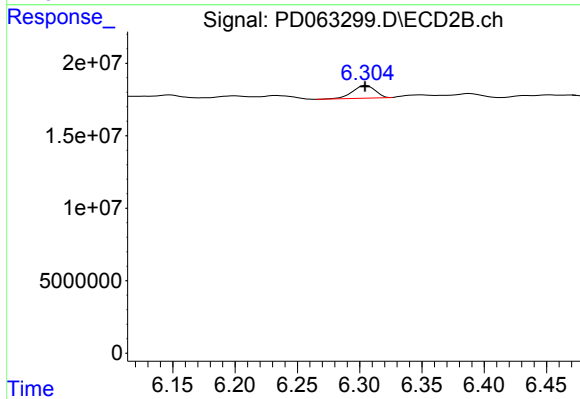

#12 4,4'-DDE

R.T.: 6.306 min
Delta R.T.: 0.001 min
Response: 10986770
Conc: 0.73 ng/ml

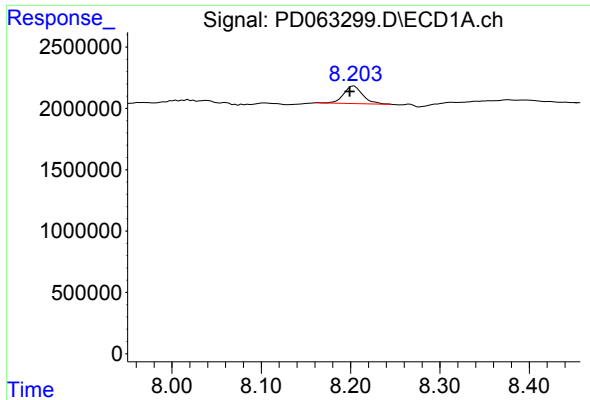


#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: 0.005 min
Response: 2107190
Conc: 1.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
HR-01-052521

Manual Integrations
APPROVED

Ankita
5/27/2021 2:14:34 PM

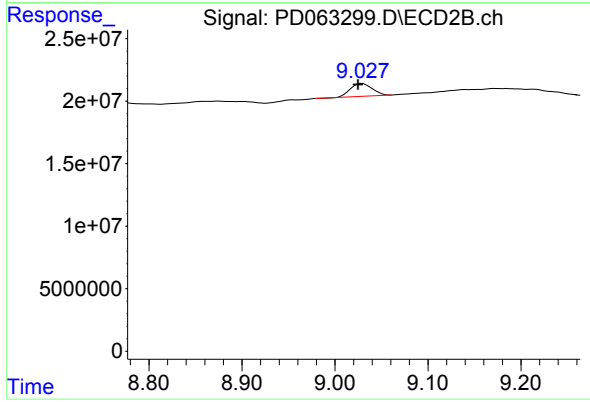

#28 Decachlorobiphenyl

R.T.: 9.029 min
Delta R.T.: 0.004 min
Response: 16767549
Conc: 1.64 ng/ml