

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052622\
 Data File : PD069854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2022 02:38
 Operator : AR\AJ
 Sample : PB144730BS
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 05:12:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.170	21010294	179.7E6	19.743	20.395
28)	SA Decachlor...	8.192	9.361	22986565	114.9E6	21.074	21.248
Target Compounds							
3)	MA gamma-BHC...	4.166	0.000	4070032	0	2.358	N.D. #
23)	Chlordane-1	4.338f	0.000	1264148	0	32.276	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052622\
Data File : PD069854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2022 02:38
Operator : AR\AJ
Sample : PB144730BS
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 05:12:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

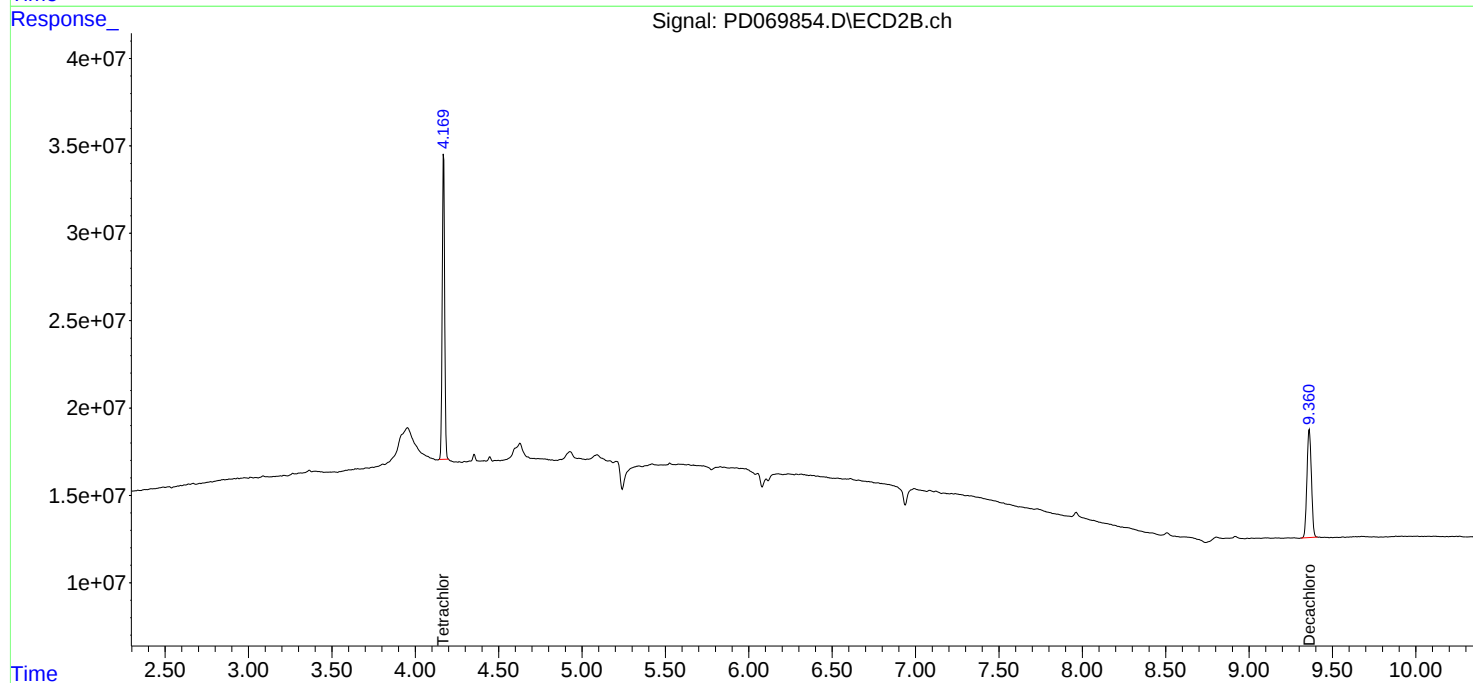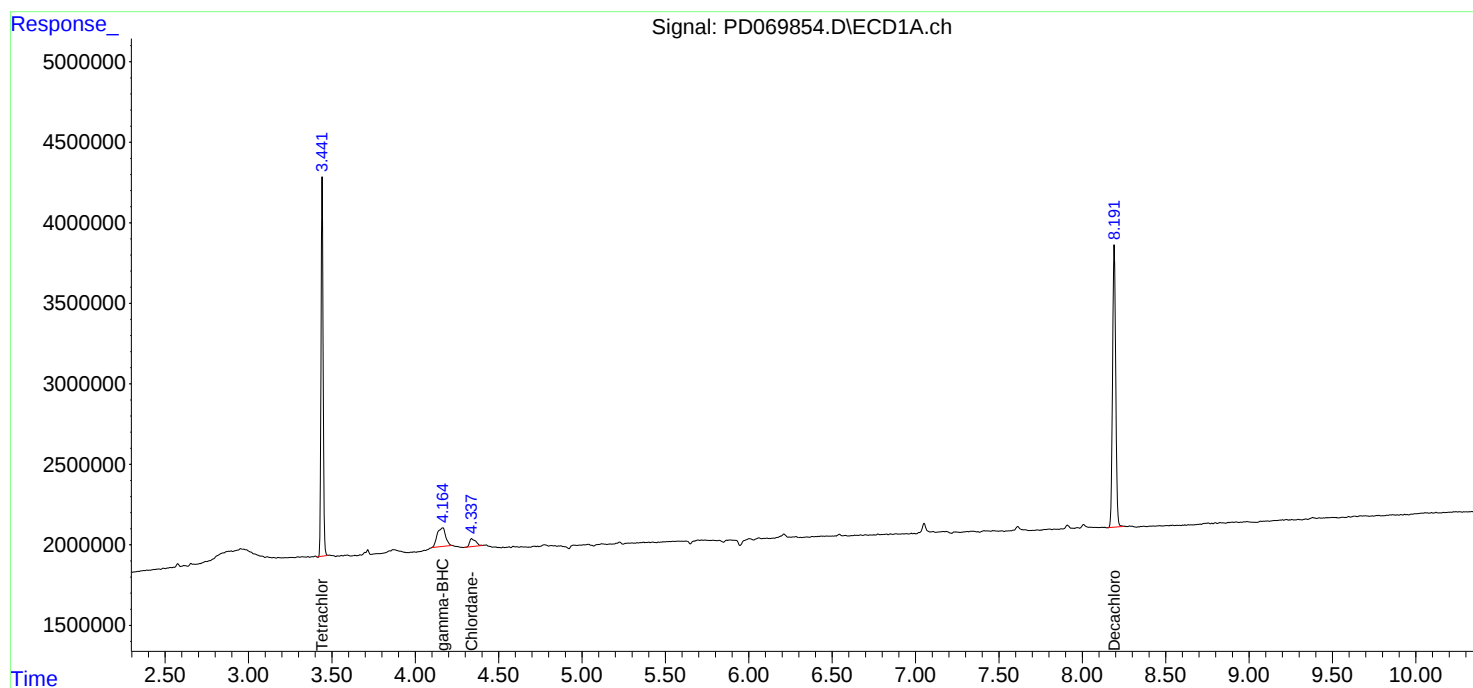


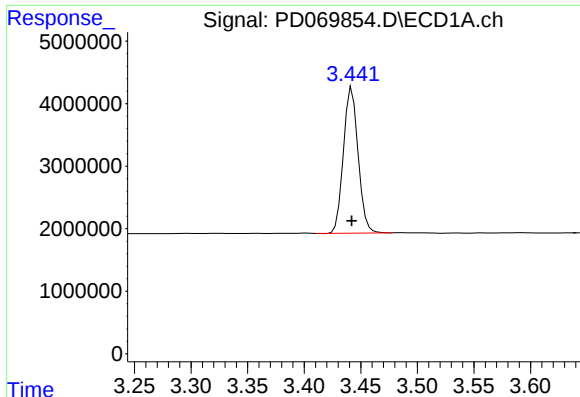

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 21010294
Conc: 19.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

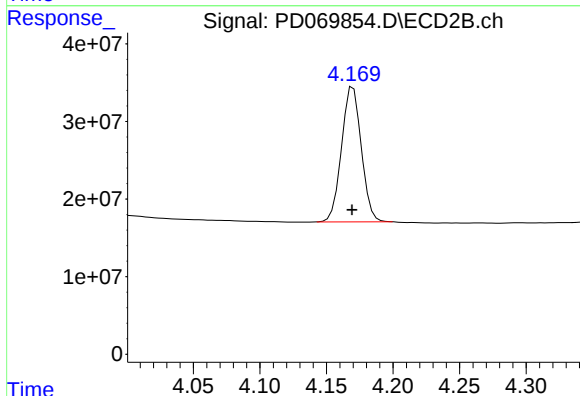


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: 0.000 min
Response: 179712338
Conc: 20.39 ng/ml

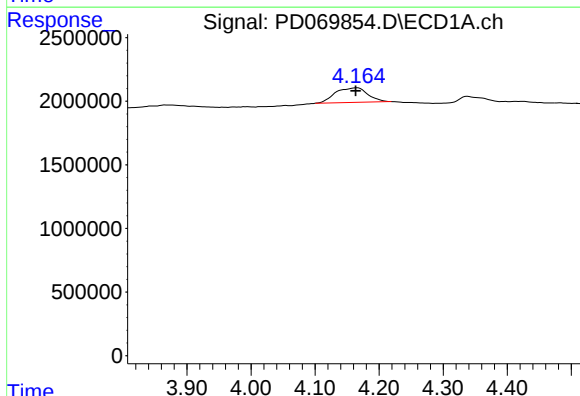


#3 gamma-BHC (Lindane)

R.T.: 4.166 min
Delta R.T.: 0.003 min
Response: 4070032
Conc: 2.36 ng/ml

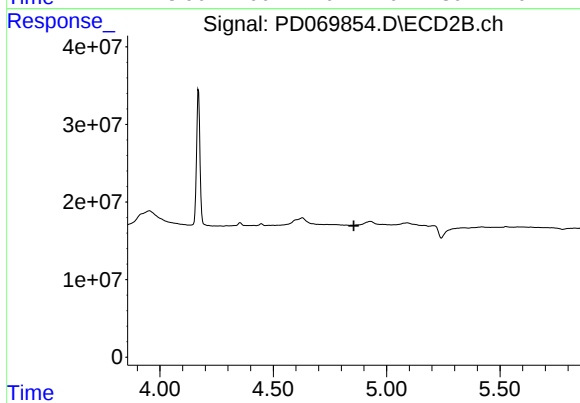

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

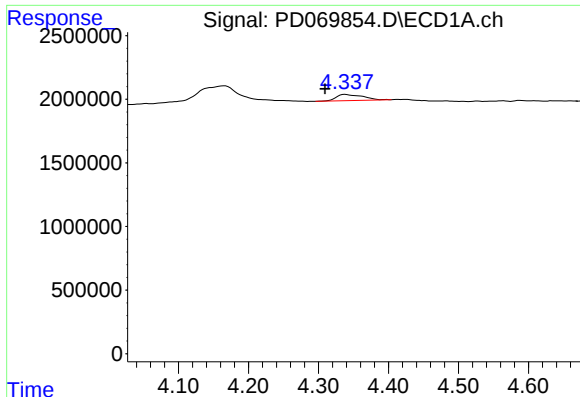

#23 Chlordane-1


R.T.: 4.338 min
Delta R.T.: 0.028 min
Response: 1264148
Conc: 32.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

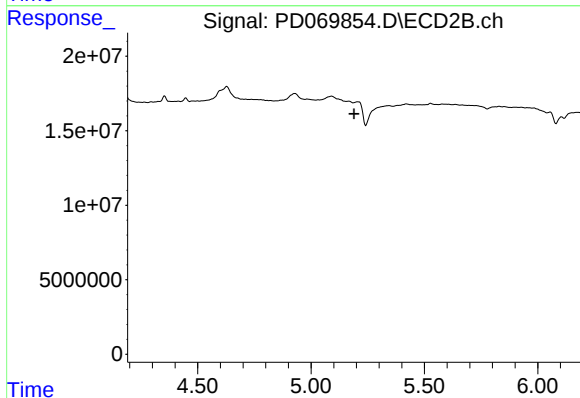


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.190 min
Response: 0
Conc: N.D.

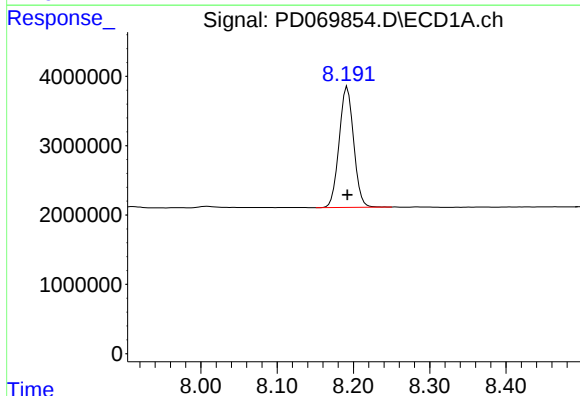

#28 Decachlorobiphenyl

R.T.: 8.192 min
Delta R.T.: 0.000 min
Response: 22986565
Conc: 21.07 ng/ml

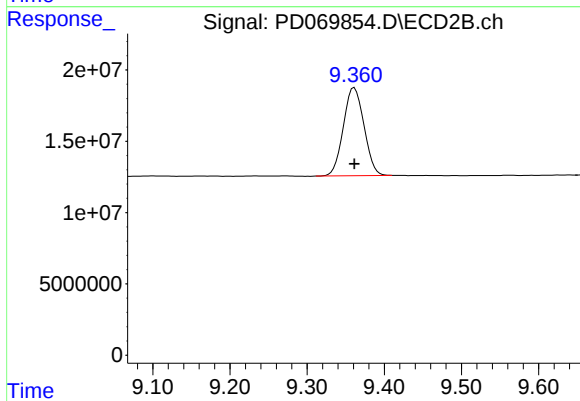

#28 Decachlorobiphenyl

R.T.: 9.361 min
Delta R.T.: 0.000 min
Response: 114912061
Conc: 21.25 ng/ml