

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052622\
 Data File : PD069839.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2022 23:07
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 02:15:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 02:15:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.170	95281886	658.2E6	74.719	74.484
28)	SA Decachlor...	8.193	9.361	81144712	392.4E6	74.374	74.025
Target Compounds							
23)	Chlordane-1	4.309	5.191	28697423	261.5E6	747.446	748.106
24)	Chlordane-2	4.810	5.664	32478266	269.5E6	743.950	743.032
25)	Chlordane-3	5.377	6.319	99122370	948.8E6	749.062	743.567
26)	Chlordane-4	5.435	6.396	81201753	1102.8E6	745.258	743.061
27)	Chlordane-5	6.272	7.207	32066809	232.6E6	744.996	800.895



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052622\
Data File : PD069839.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2022 23:07
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 02:15:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 02:15:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

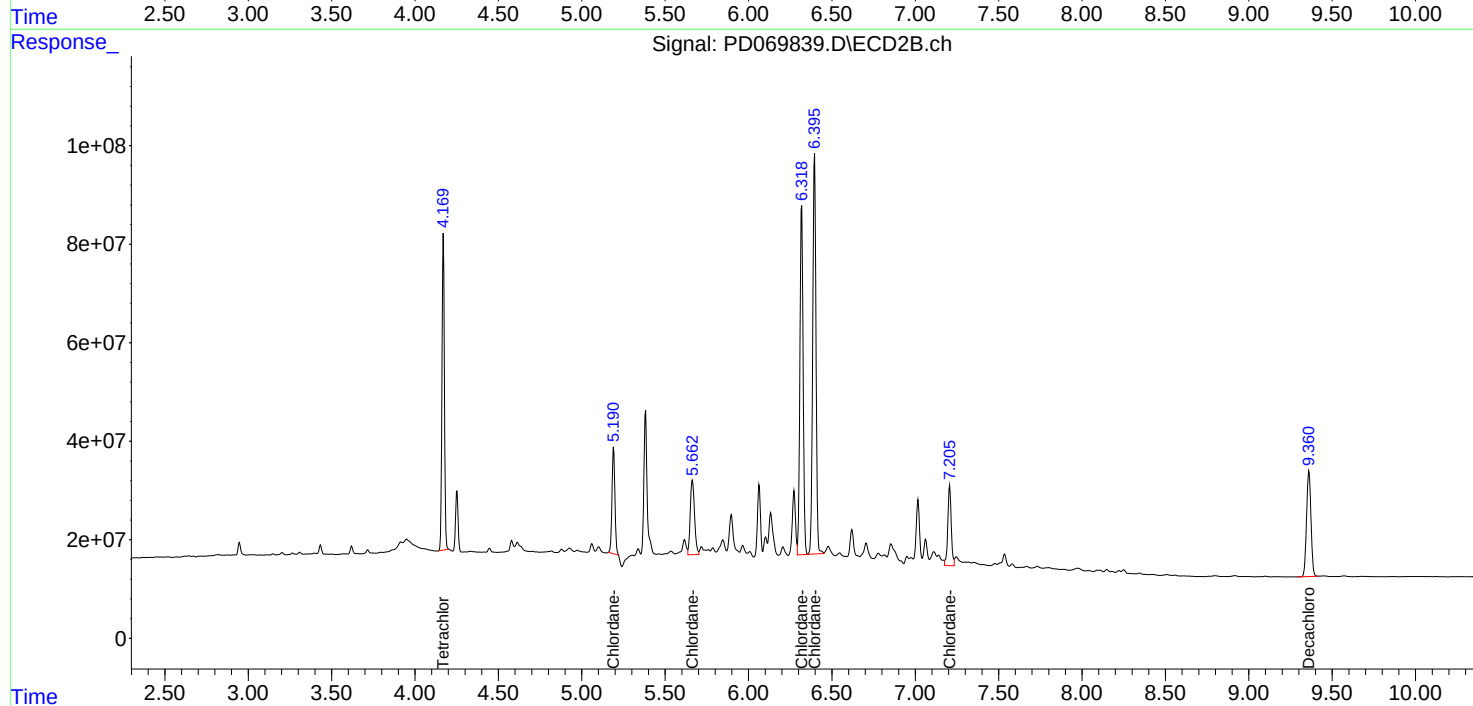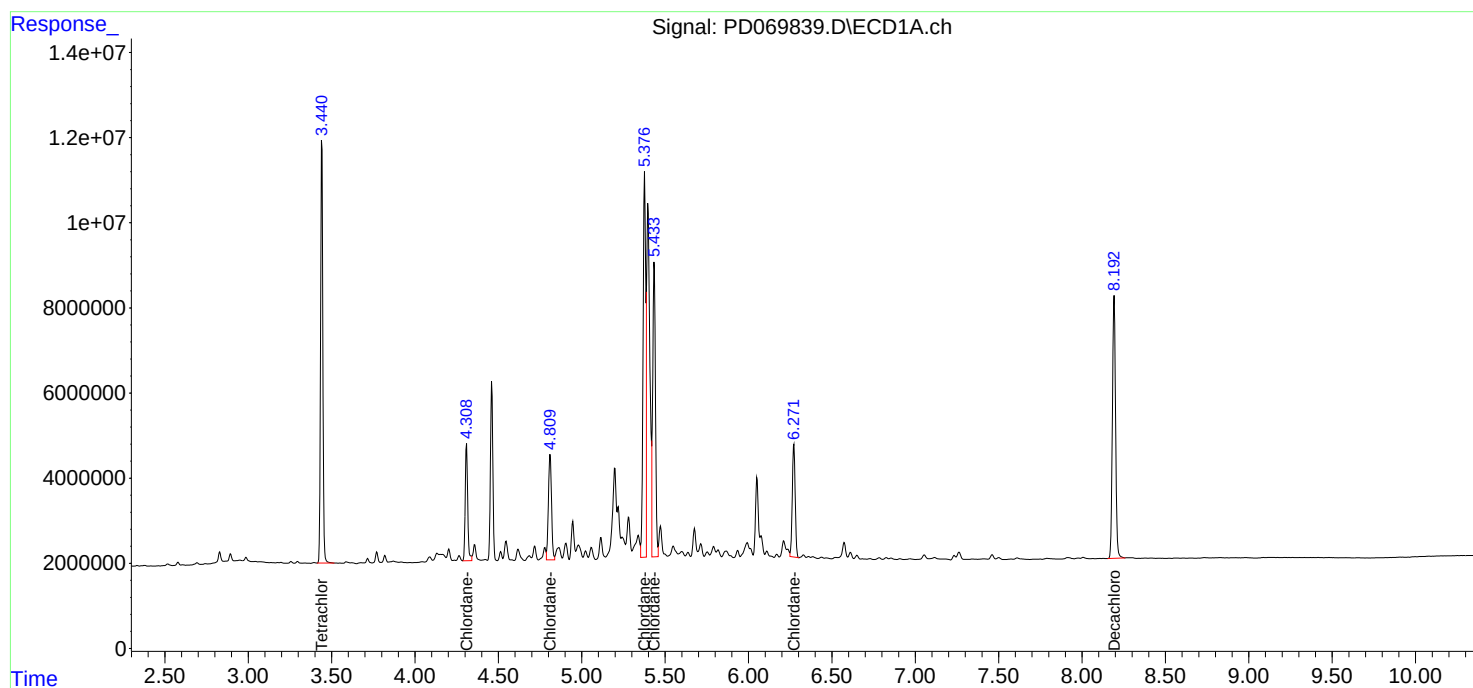


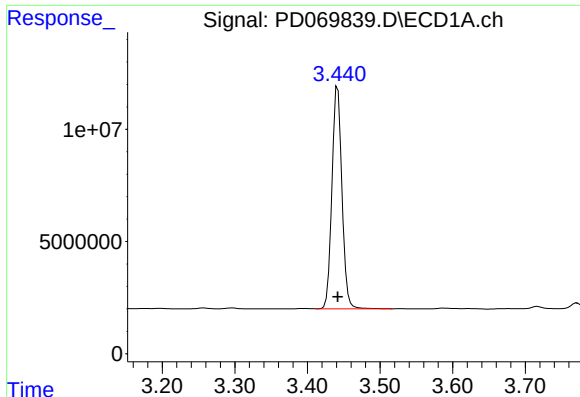

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 95281886
Conc: 74.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

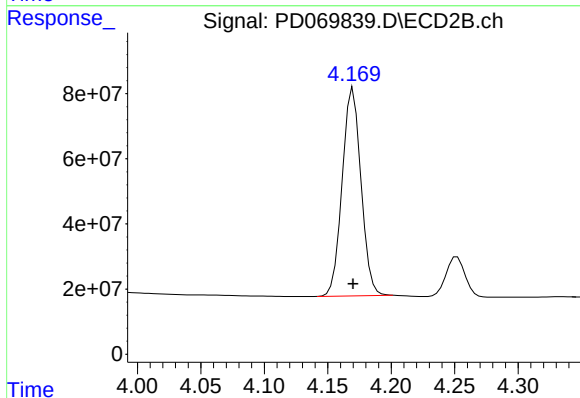


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: 0.000 min
Response: 658222570
Conc: 74.48 ng/ml

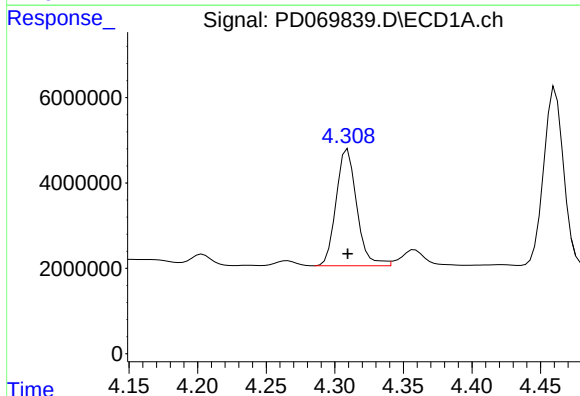


#23 Chlordane-1

R.T.: 4.309 min
Delta R.T.: 0.000 min
Response: 28697423
Conc: 747.45 ng/ml

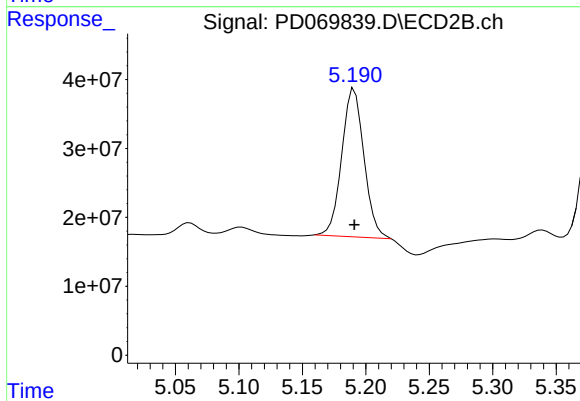

#23 Chlordane-1


R.T.: 5.191 min
Delta R.T.: 0.000 min
Response: 261509589
Conc: 748.11 ng/ml

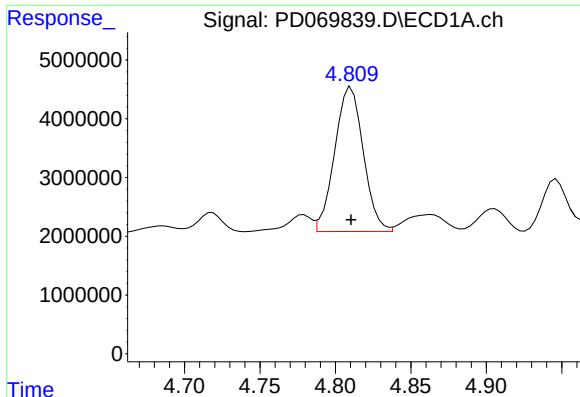

#24 Chlordane-2


R.T.: 4.810 min
Delta R.T.: 0.000 min
Response: 32478266
Conc: 743.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

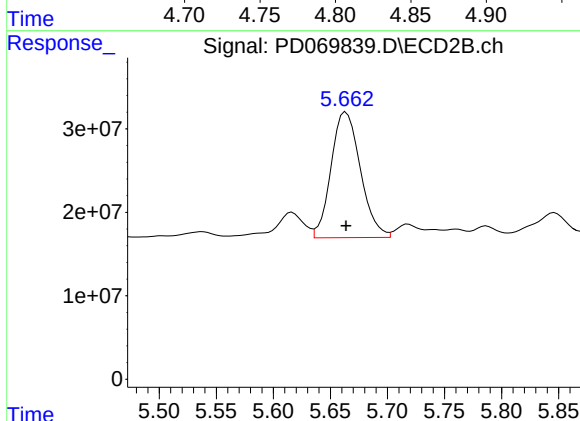


#24 Chlordane-2

R.T.: 5.664 min
Delta R.T.: 0.000 min
Response: 269544579
Conc: 743.03 ng/ml

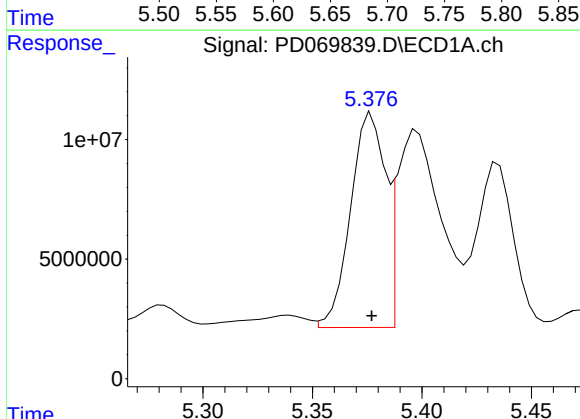


#25 Chlordane-3

R.T.: 5.377 min
Delta R.T.: 0.000 min
Response: 99122370
Conc: 749.06 ng/ml

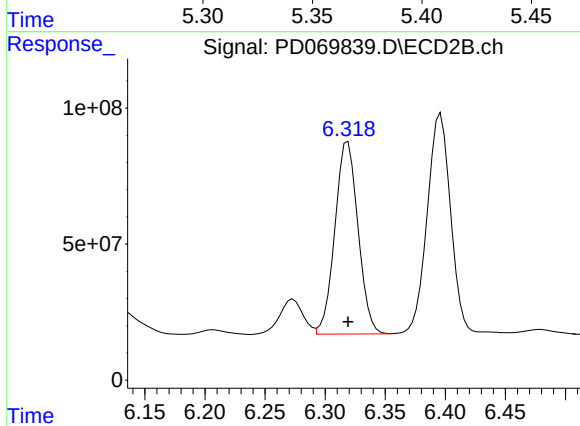

#25 Chlordane-3


R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 948823713
Conc: 743.57 ng/ml

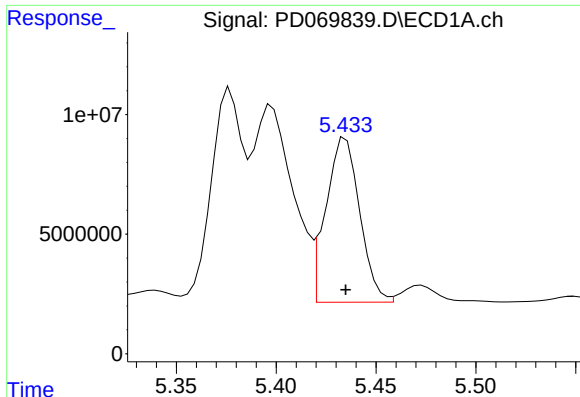

#26 Chlordane-4


R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 81201753
Conc: 745.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

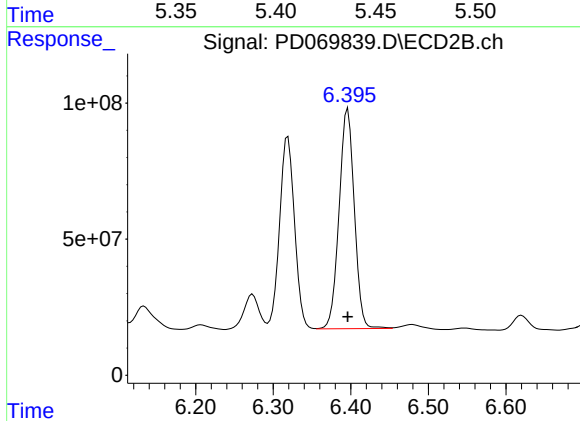


#26 Chlordane-4

R.T.: 6.396 min
Delta R.T.: 0.000 min
Response: 1102846548
Conc: 743.06 ng/ml

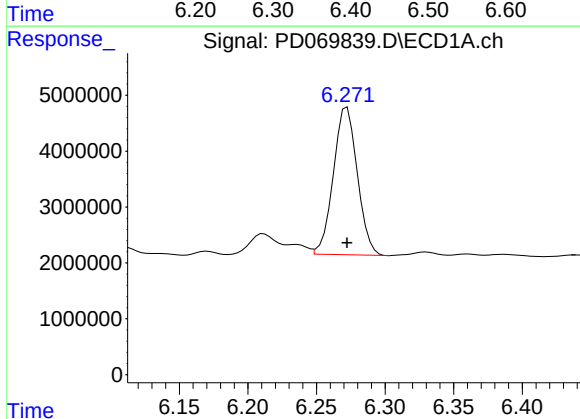


#27 Chlordane-5

R.T.: 6.272 min
Delta R.T.: 0.000 min
Response: 32066809
Conc: 745.00 ng/ml

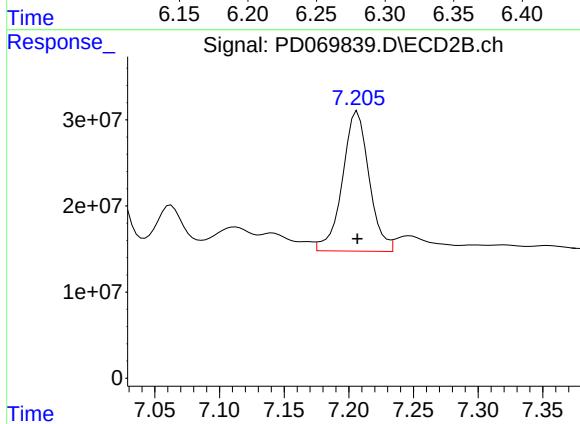

#27 Chlordane-5


R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 232553280
Conc: 800.89 ng/ml

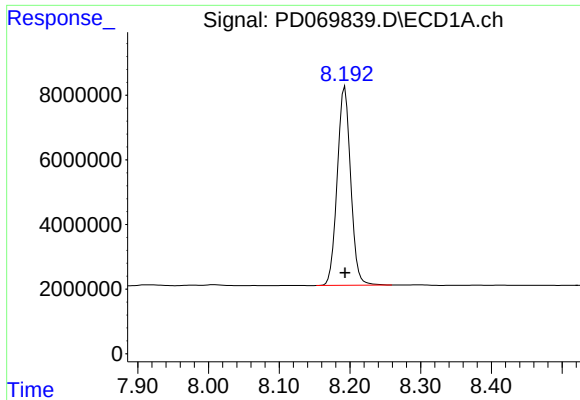

#28 Decachlorobiphenyl

R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 81144712
Conc: 74.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

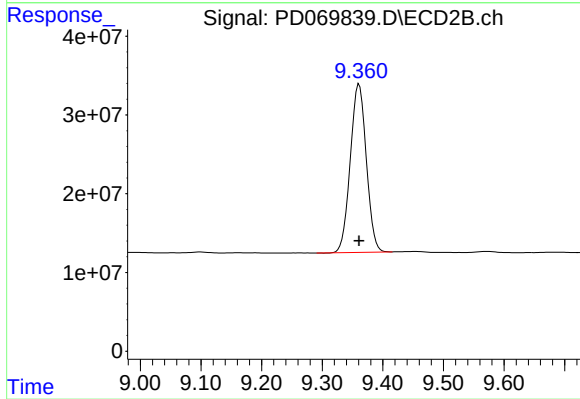

#28 Decachlorobiphenyl

R.T.: 9.361 min
Delta R.T.: 0.000 min
Response: 392370144
Conc: 74.02 ng/ml