

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052622\
 Data File : PD069840.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2022 23:22
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 02:08:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 02:06:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.170	63844866	457.3E6	50.000	50.000
28)	SA Decachlor...	8.193	9.360	56574375	278.2E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.310	5.192	19455927	179.7E6	500.000	500.000
24)	Chlordane-2	4.811	5.664	22616315	191.2E6	500.000	500.000
25)	Chlordane-3	5.377	6.320	66656480	659.0E6	500.000	500.000
26)	Chlordane-4	5.436	6.397	55277234	768.0E6	500.000	500.000
27)	Chlordane-5	6.272	7.207	21692992	133.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052622\
Data File : PD069840.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2022 23:22
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 02:08:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 02:06:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

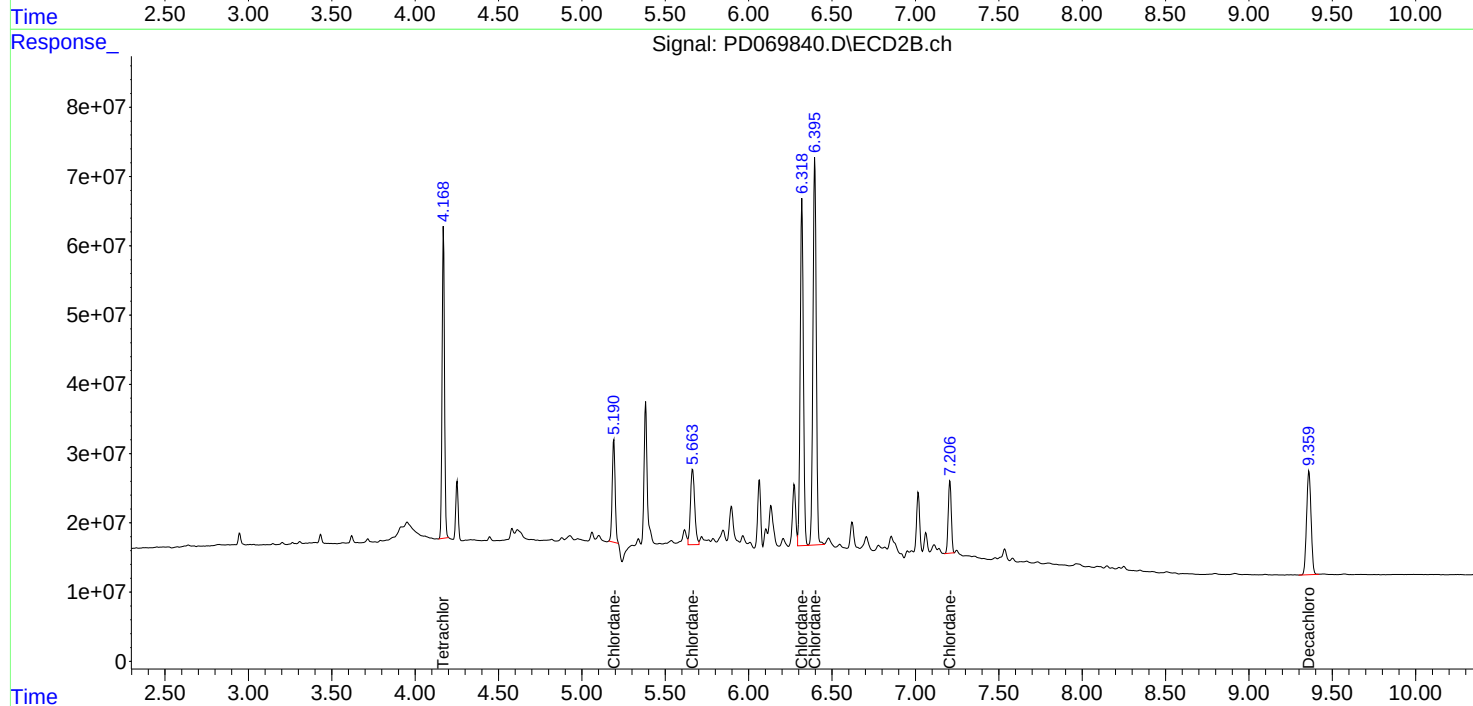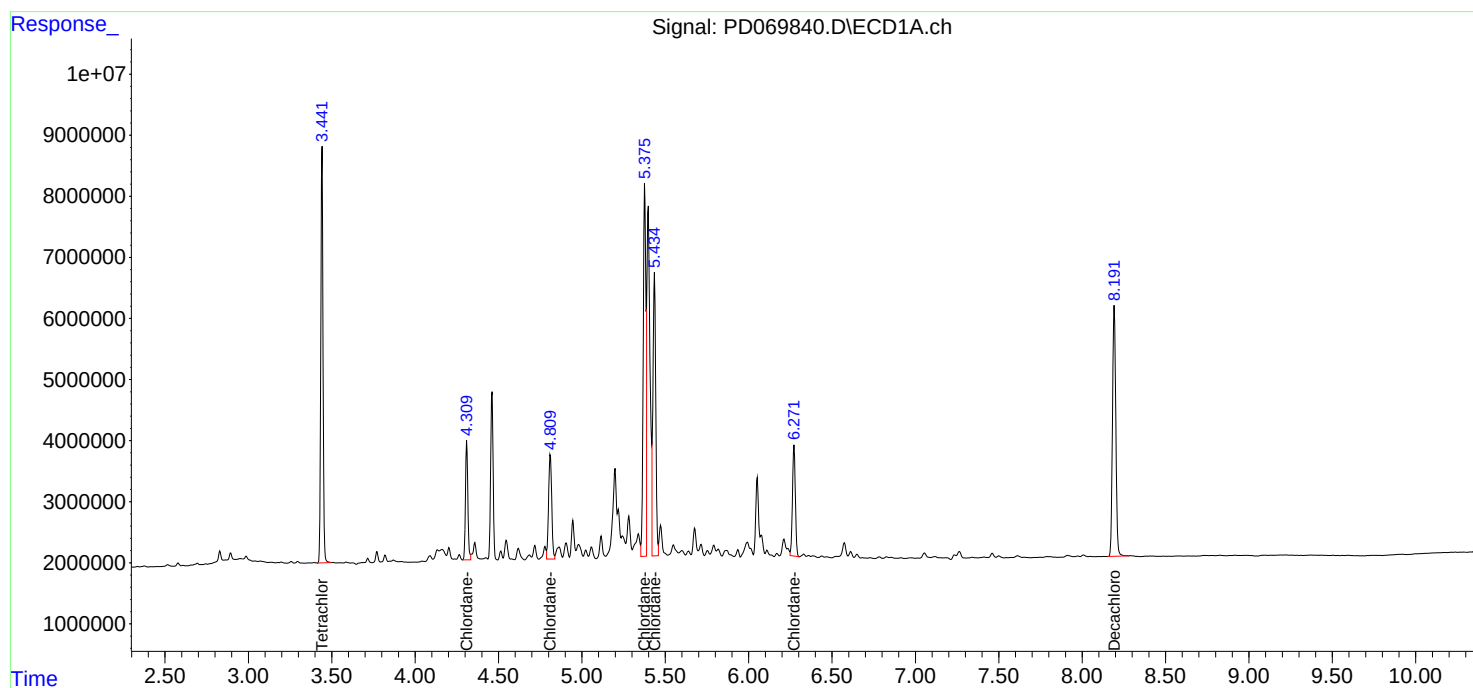


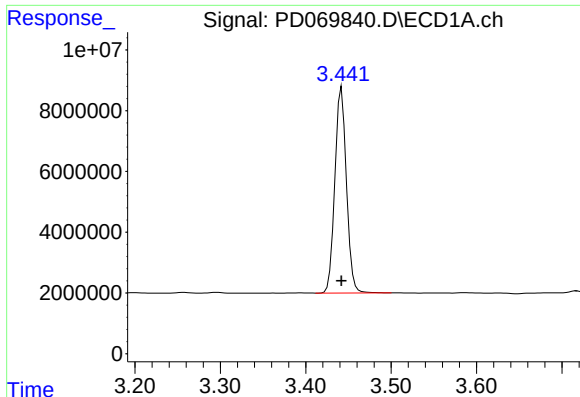

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 63844866
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

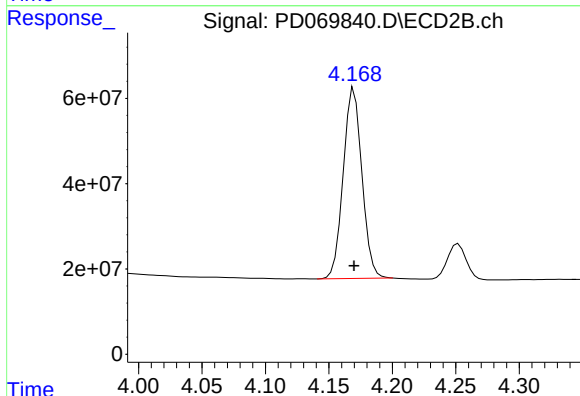


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: 0.000 min
Response: 457269464
Conc: 50.00 ng/ml

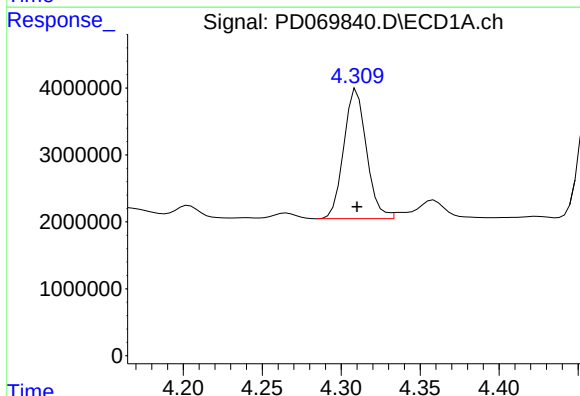


#23 Chlordane-1

R.T.: 4.310 min
Delta R.T.: 0.000 min
Response: 19455927
Conc: 500.00 ng/ml

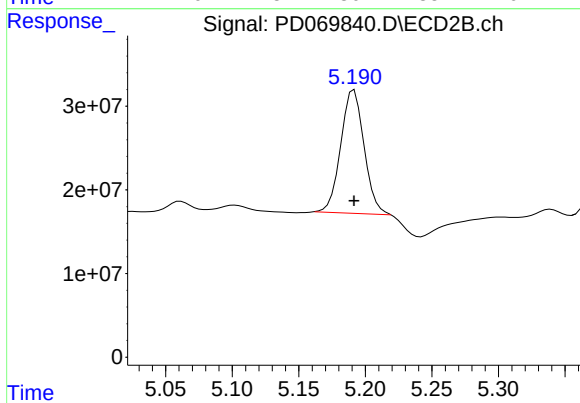

#23 Chlordane-1


R.T.: 5.192 min
Delta R.T.: 0.000 min
Response: 179659582
Conc: 500.00 ng/ml

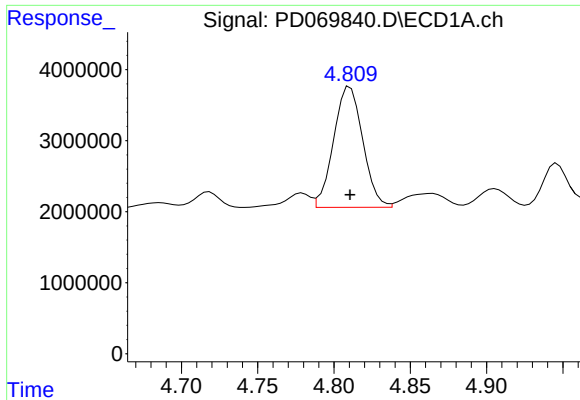

#24 Chlordane-2


R.T.: 4.811 min
Delta R.T.: 0.000 min
Response: 22616315
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

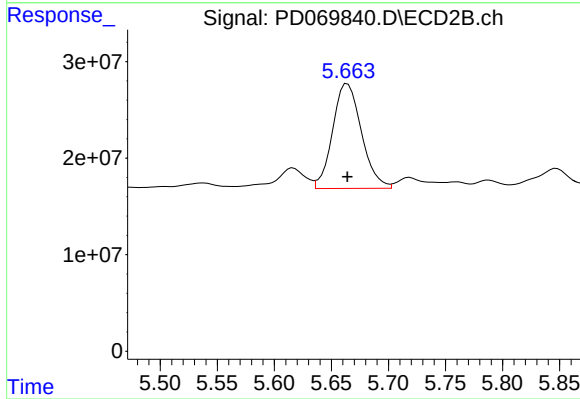


#24 Chlordane-2

R.T.: 5.664 min
Delta R.T.: 0.000 min
Response: 191217233
Conc: 500.00 ng/ml

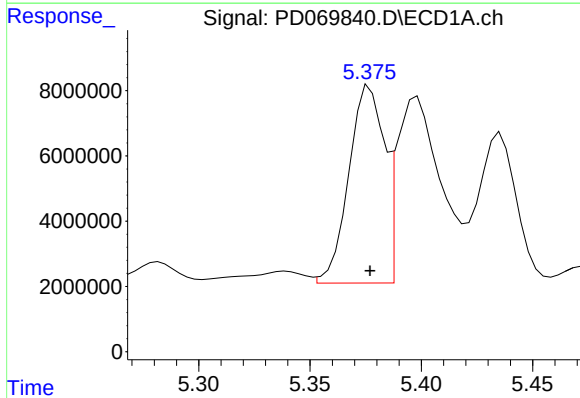


#25 Chlordane-3

R.T.: 5.377 min
Delta R.T.: 0.000 min
Response: 66656480
Conc: 500.00 ng/ml

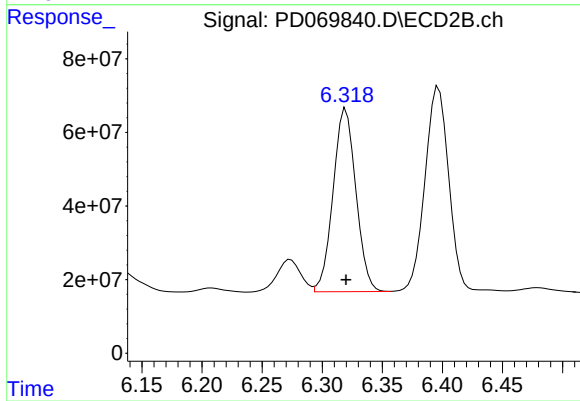

#25 Chlordane-3


R.T.: 6.320 min
Delta R.T.: 0.000 min
Response: 658971932
Conc: 500.00 ng/ml

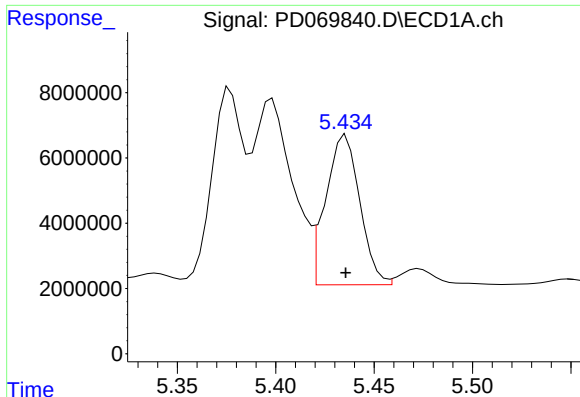

#26 Chlordane-4


R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 55277234
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

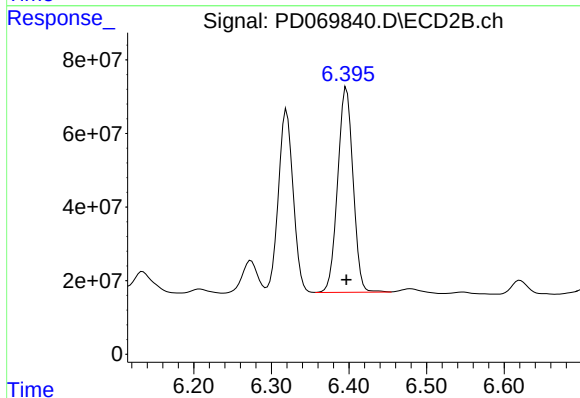


#26 Chlordane-4

R.T.: 6.397 min
Delta R.T.: 0.000 min
Response: 767978401
Conc: 500.00 ng/ml

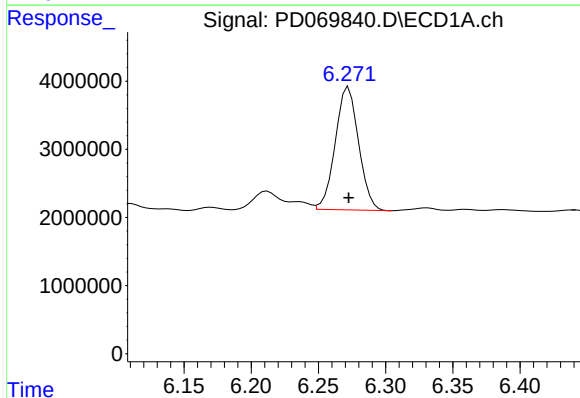


#27 Chlordane-5

R.T.: 6.272 min
Delta R.T.: 0.000 min
Response: 21692992
Conc: 500.00 ng/ml

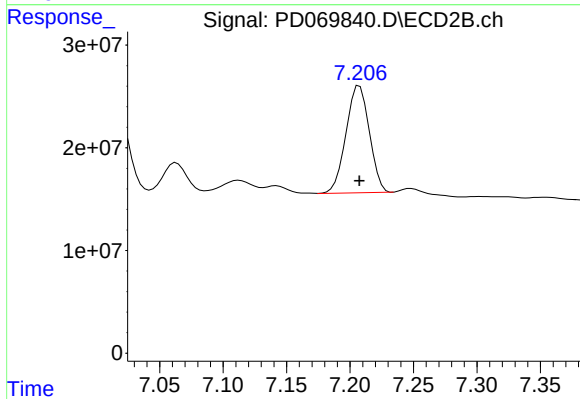

#27 Chlordane-5


R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 133488956
Conc: 500.00 ng/ml

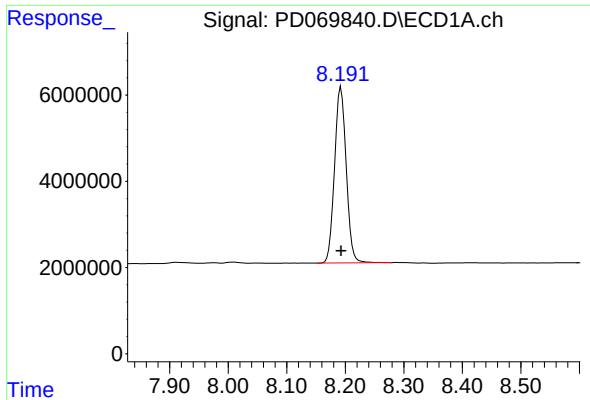

#28 Decachlorobiphenyl

R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 56574375
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

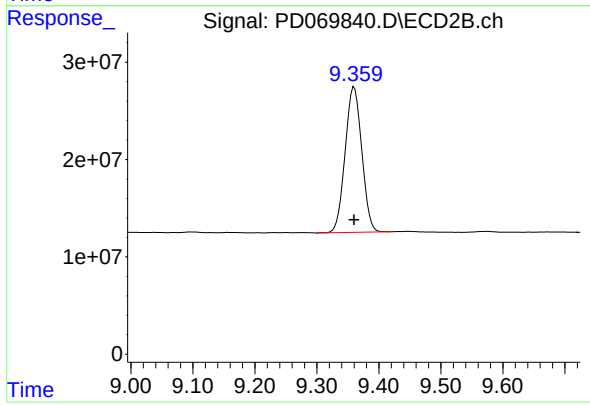

#28 Decachlorobiphenyl

R.T.: 9.360 min
Delta R.T.: 0.000 min
Response: 278200103
Conc: 50.00 ng/ml