

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052622\
 Data File : PD069841.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2022 23:36
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 02:18:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 02:18:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.170	30433030	230.9E6	24.139	25.834
28)	SA Decachlor...	8.192	9.361	28464829	141.4E6	25.808	26.233
Target Compounds							
23)	Chlordane-1	4.310	5.191	9594694	94059177	249.926	264.040
24)	Chlordane-2	4.810	5.664	11368005	105.5E6	257.717	279.345
25)	Chlordane-3	5.377	6.319	30807711	335.1E6	236.884	259.313
26)	Chlordane-4	5.435	6.397	26501866	389.1E6	244.888	259.027
27)	Chlordane-5	6.273	7.207	10421587	69029755	244.044	240.685



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052622\
Data File : PD069841.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2022 23:36
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 02:18:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 02:18:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

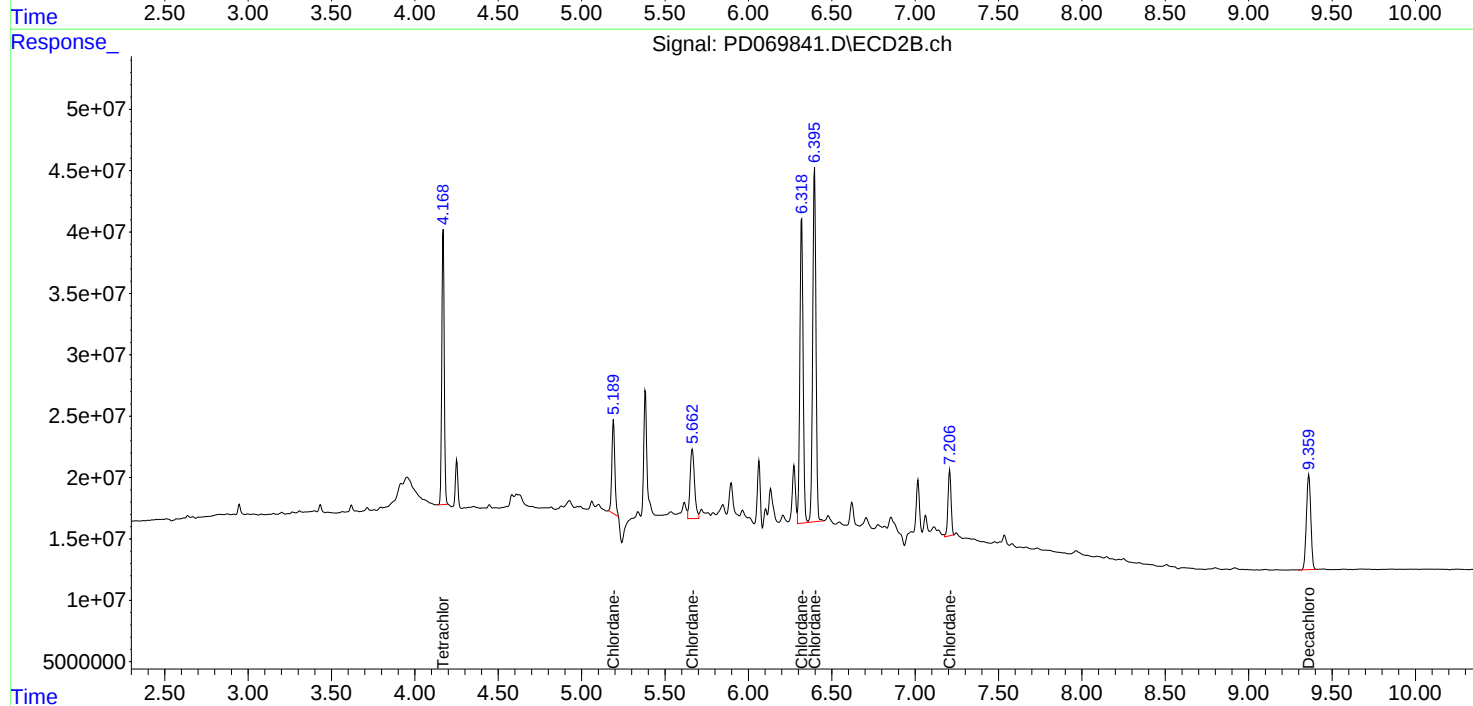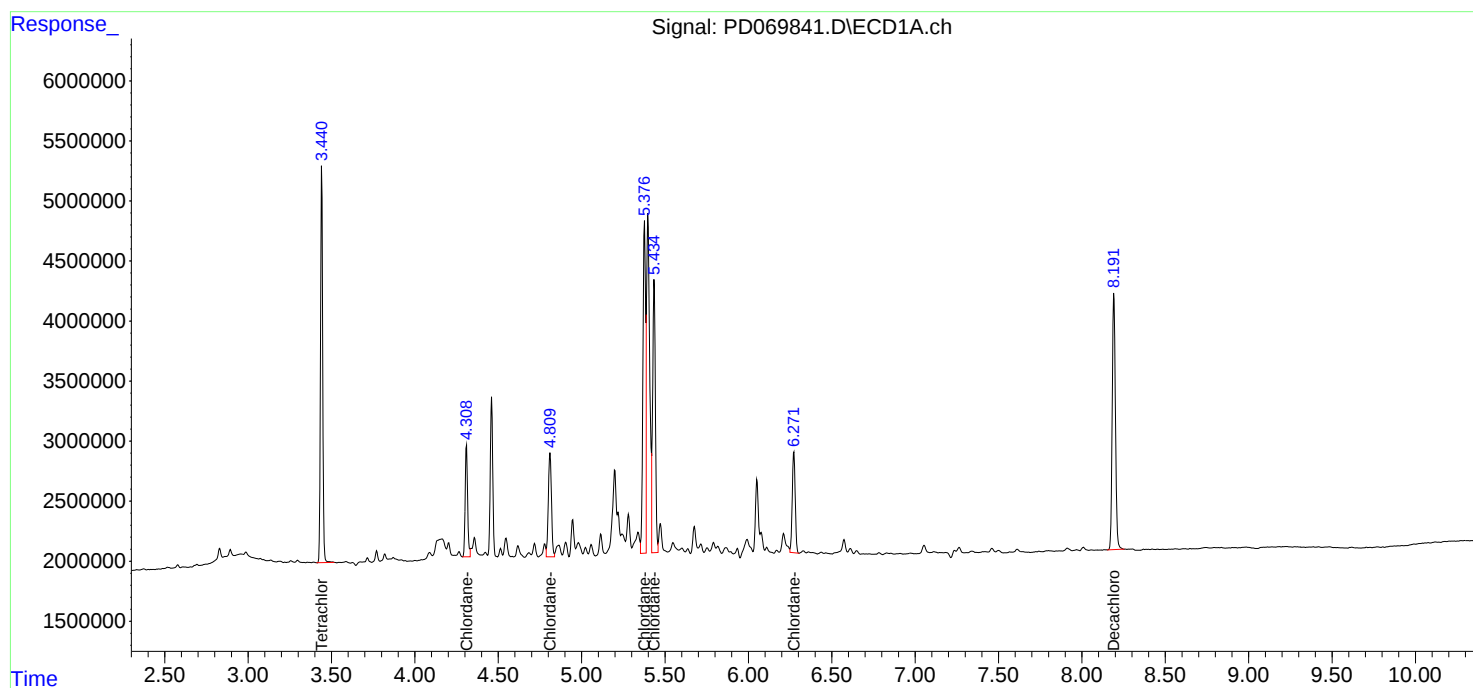


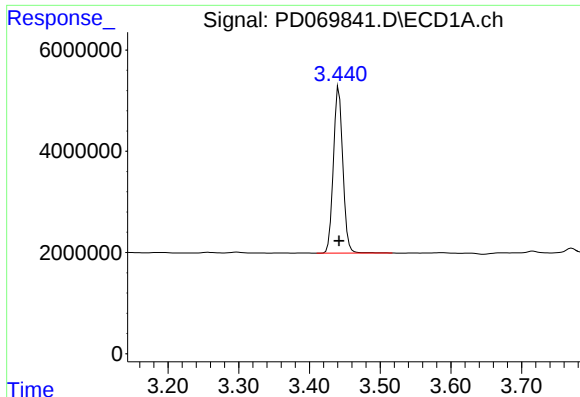

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 30433030
Conc: 24.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

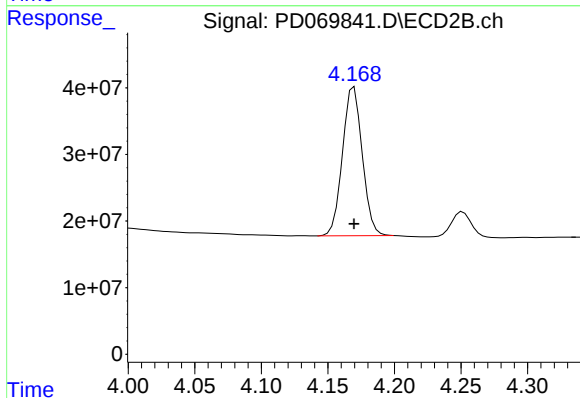


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: 0.000 min
Response: 230860455
Conc: 25.83 ng/ml

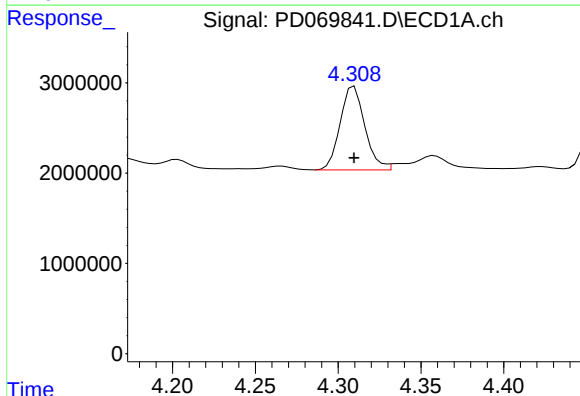


#23 Chlordane-1

R.T.: 4.310 min
Delta R.T.: 0.000 min
Response: 9594694
Conc: 249.93 ng/ml

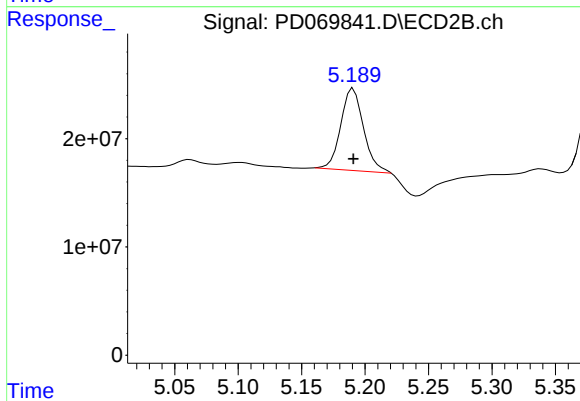

#23 Chlordane-1


R.T.: 5.191 min
Delta R.T.: 0.000 min
Response: 94059177
Conc: 264.04 ng/ml

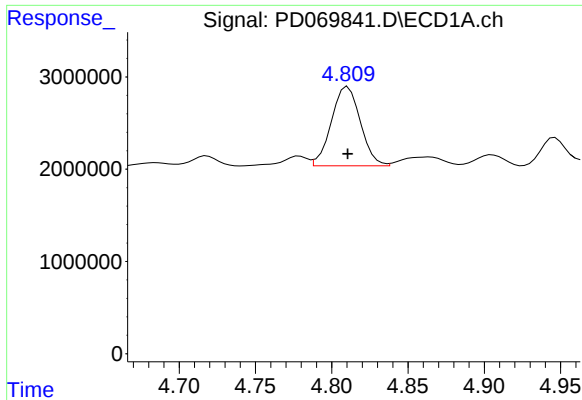

#24 Chlordane-2


R.T.: 4.810 min
Delta R.T.: 0.000 min
Response: 11368005
Conc: 257.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

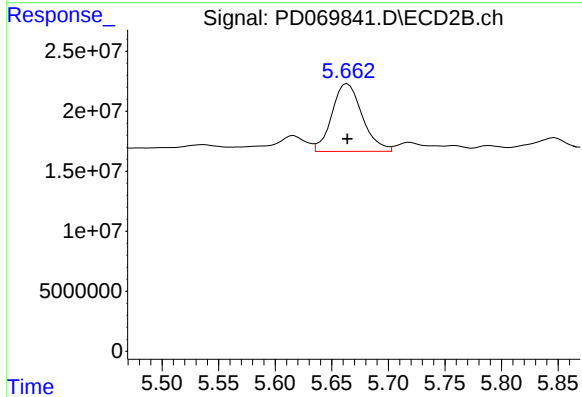


#24 Chlordane-2

R.T.: 5.664 min
Delta R.T.: 0.000 min
Response: 105462499
Conc: 279.35 ng/ml

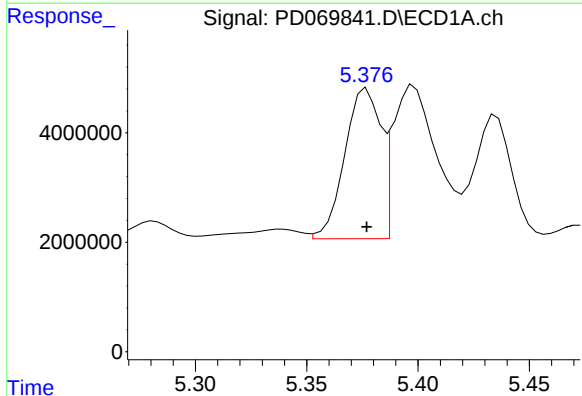


#25 Chlordane-3

R.T.: 5.377 min
Delta R.T.: 0.000 min
Response: 30807711
Conc: 236.88 ng/ml

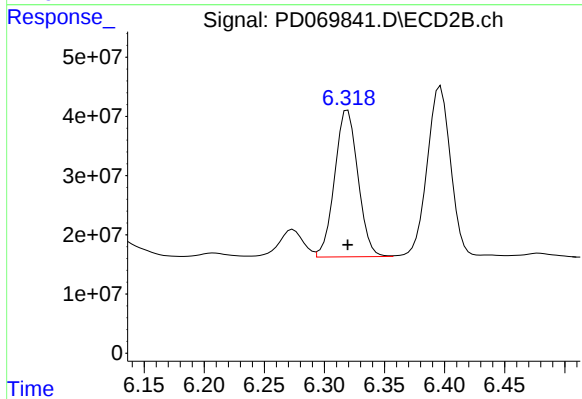

#25 Chlordane-3


R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 335054709
Conc: 259.31 ng/ml

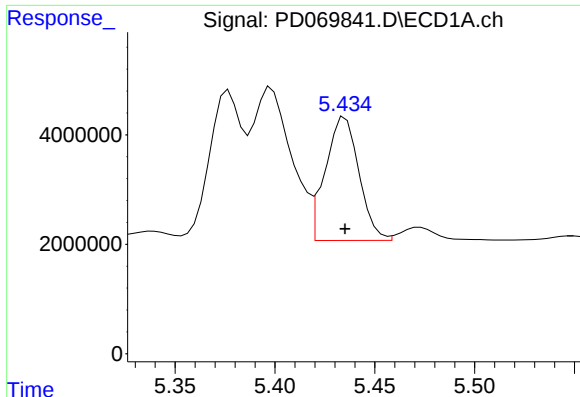

#26 Chlordane-4


R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 26501866
Conc: 244.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

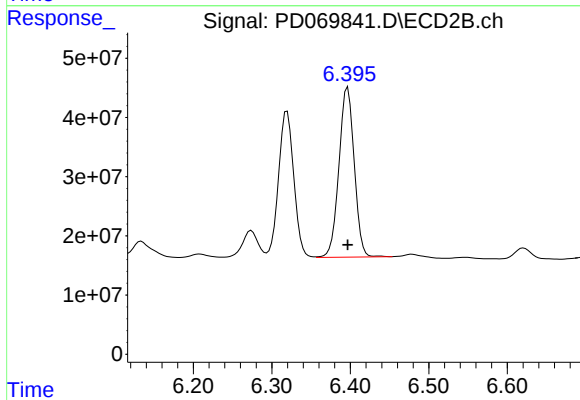


#26 Chlordane-4

R.T.: 6.397 min
Delta R.T.: 0.000 min
Response: 389129466
Conc: 259.03 ng/ml

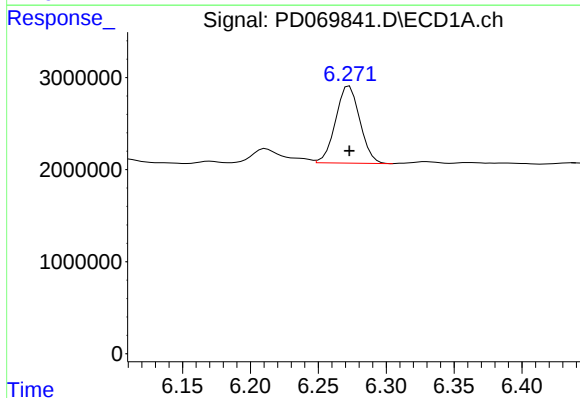


#27 Chlordane-5

R.T.: 6.273 min
Delta R.T.: 0.000 min
Response: 10421587
Conc: 244.04 ng/ml

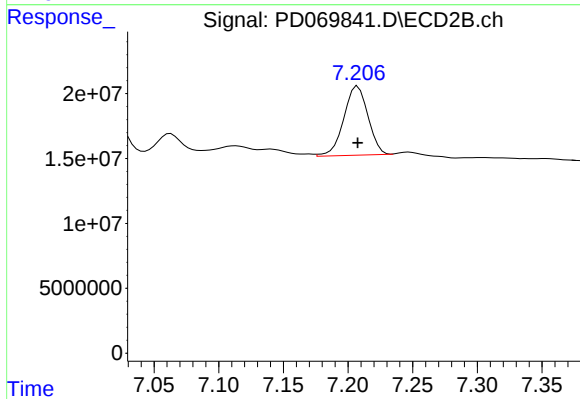

#27 Chlordane-5


R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 69029755
Conc: 240.69 ng/ml

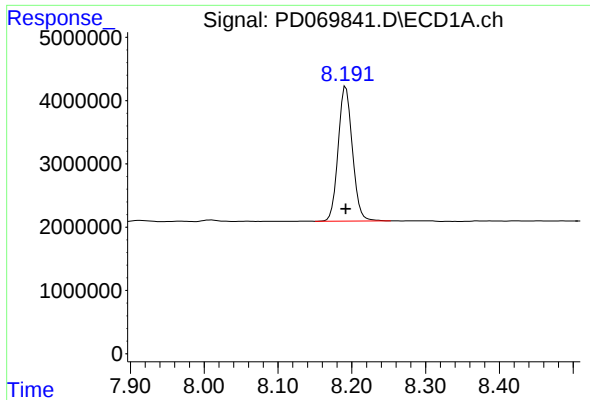

#28 Decachlorobiphenyl

R.T.: 8.192 min
Delta R.T.: 0.000 min
Response: 28464829
Conc: 25.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

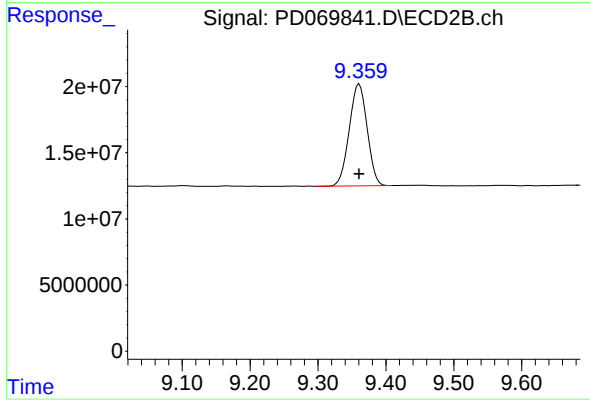

#28 Decachlorobiphenyl

R.T.: 9.361 min
Delta R.T.: 0.000 min
Response: 141372380
Conc: 26.23 ng/ml