

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052624\
 Data File : PD083043.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2024 11:01
 Operator : AR\AJ
 Sample : P2528-04MS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH9S9MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/26/2024
 Supervised By :Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 21:56:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.775	27653718	77910789	18.488	20.035
27)	SA Decachlor...	9.121	7.904	30415325	68197811	15.174	17.237
Target Compounds							
2)	A alpha-BHC	4.021	3.275	137.3E6	345.0E6	53.806m	55.490
3)	MA gamma-BHC...	4.356	3.604	123.2E6	305.0E6	49.934	52.710
4)	MA Heptachlor	4.949	3.943	126.9E6	298.8E6	50.398	53.664
5)	MB Aldrin	5.292	4.222	123.5E6	293.0E6	51.023	53.017
6)	B beta-BHC	4.552	3.899	53107873	128.0E6	48.952	51.046
7)	B delta-BHC	4.801	4.129	124.0E6	308.0E6	50.660	52.060
8)	B Heptachlo...	5.719	4.723	107.7E6	258.1E6	48.247	50.523
9)	A Endosulfan I	6.107	5.092	99905864	242.6E6	48.012	53.792
10)	B trans-Chl...	5.976	4.972	103.3E6	259.0E6	47.733	52.004
11)	B cis-Chlor...	6.056	5.036	104.6E6	259.3E6	46.835	51.048
12)	B 4,4'-DDE	6.228	5.224	206.6E6	503.6E6	94.746	105.607
13)	MA Dieldrin	6.382	5.356	211.7E6	521.3E6	96.309	104.312
14)	MA Endrin	6.614	5.631	175.3E6	454.8E6	98.298	103.980
15)	B Endosulfa...	6.834	5.924	176.8E6	435.5E6	91.774	103.345
16)	A 4,4'-DDD	6.747	5.778	155.8E6	402.6E6	100.450	106.989
17)	MA 4,4'-DDT	7.063	6.029	161.9E6	402.8E6	100.677	104.896
18)	B Endrin al...	6.964	6.104	132.3E6	327.8E6	95.249	103.951
19)	B Endosulfa...	7.199	6.326	165.0E6	412.1E6	93.477	102.500
20)	A Methoxychlor	7.539	6.604	398.7E6	920.6E6	460.915	469.162
21)	B Endrin ke...	7.687	6.832	177.2E6	452.2E6	94.024	100.547

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052624\
Data File : PD083043.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2024 11:01
Operator : AR\AJ
Sample : P2528-04MS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 21:56:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

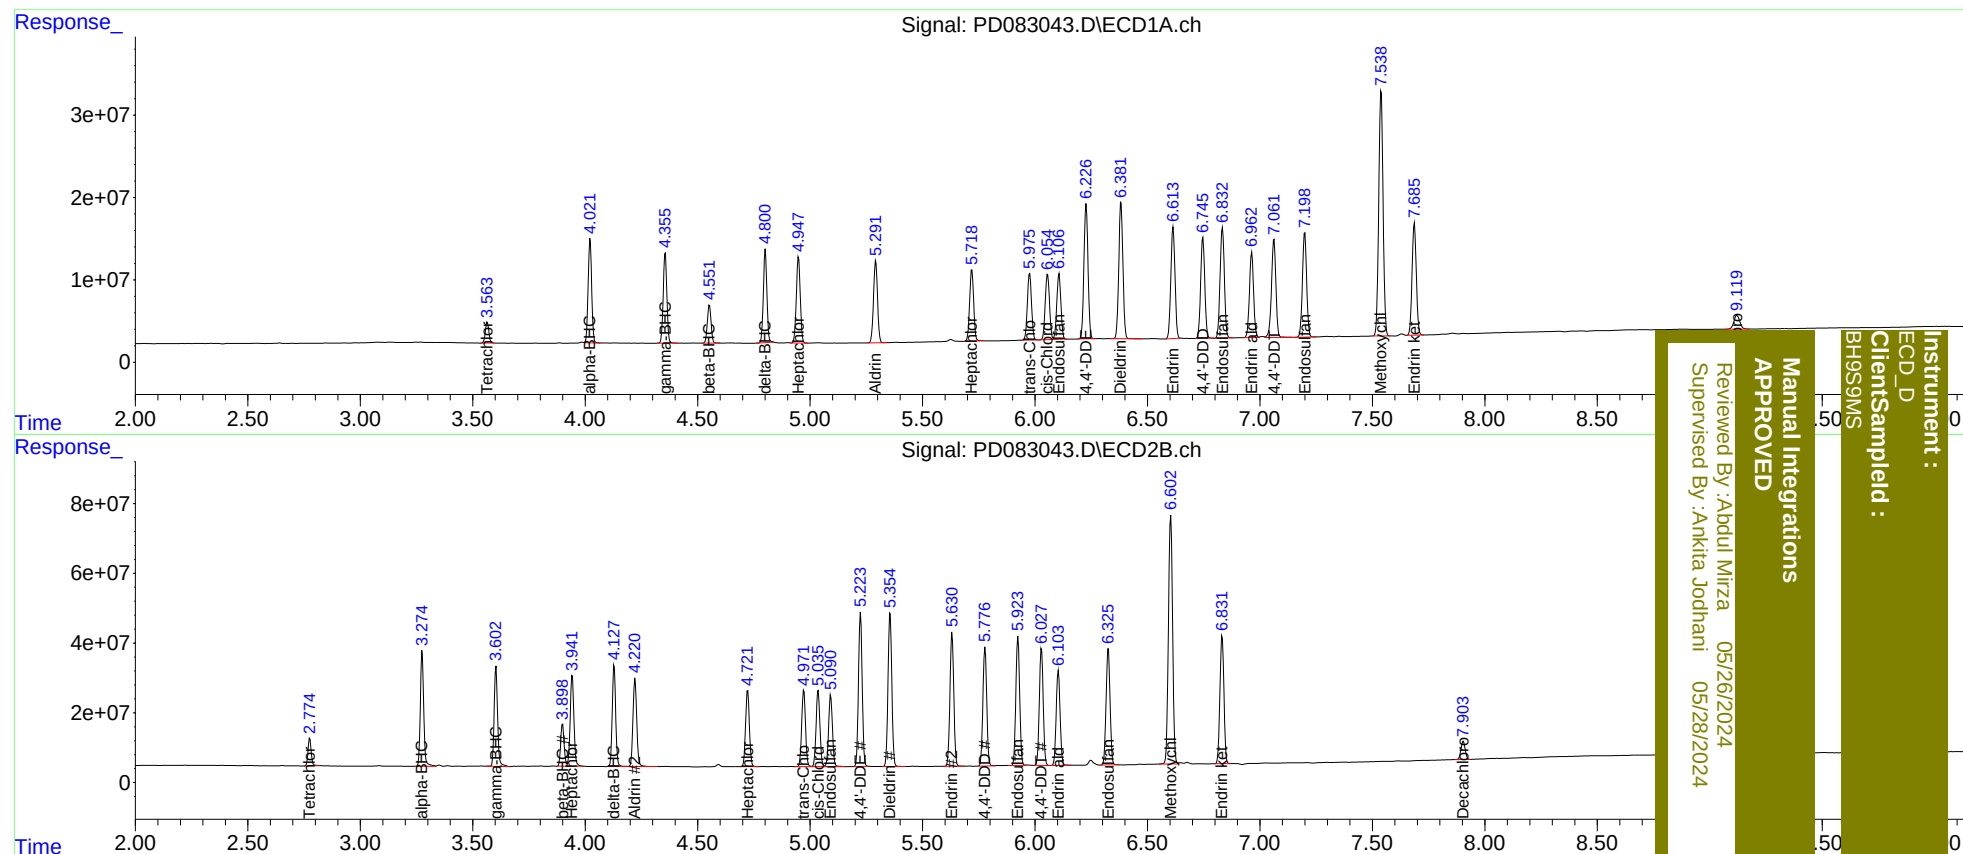

Instrument :
ECD_D
ClientSampled :
BH9S9MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 05/26/2024
Supervised By: Ankita Jodhani 05/28/2024