

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052624\
 Data File : PD083050.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2024 13:49
 Operator : AR\AJ
 Sample : P2548-06DL 2X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH5Y3DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/26/2024
 Supervised By : Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 22:04:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.564	2.776	7495959	26640156	5.012m	6.851 #
2) SA Decachlor...	9.110	7.904	21064683	43979323	10.509m	11.116
Target Compounds						
12) B 4,4'-DDE	6.229	5.226	113.9E6	355.5E6	52.249	74.543 #
13) MA Dieldrin	6.403	5.363	11272586	68685269	5.129m	13.745m#
16) A 4,4'-DDD	6.734	5.779	17159109	24627416	11.064m	6.545m#
17) MA 4,4'-DDT	7.063	6.030	118.6E6	286.2E6	73.737m	74.547

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052624\
Data File : PD083050.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2024 13:49
Operator : AR\AJ
Sample : P2548-06DL 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 22:04:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

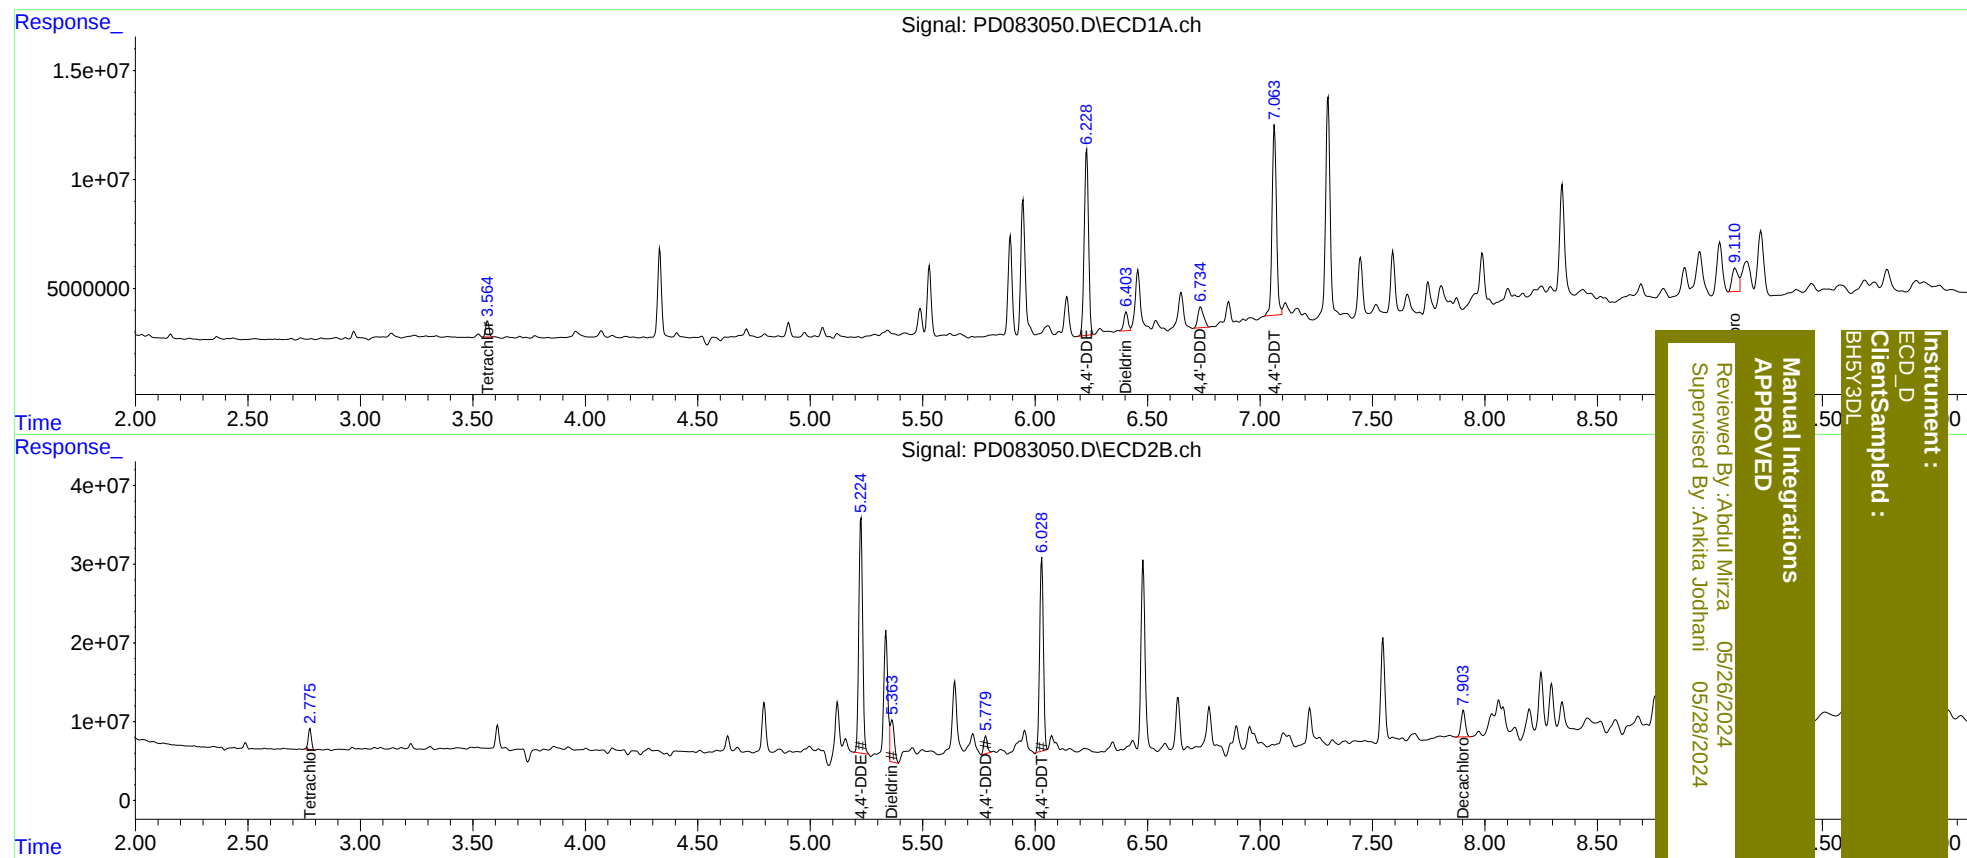

Reviewed By: Abdul Mirza 05/26/2024
Supervised By: Ankita Jodhani 05/28/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
BH5Y3DL