

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052624\
 Data File : PD083062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2024 19:02
 Operator : AR\AJ
 Sample : P2568-04MS
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH5Q6MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/26/2024
 Supervised By :Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 22:18:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.774	20155084	56661561	13.475	14.571m
27)	SA Decachlor...	9.119	7.904	28766555	58665628	14.352m	14.828
Target Compounds							
2)	A alpha-BHC	4.020	3.275	150.4E6	377.8E6	58.950m	60.779
3)	MA gamma-BHC...	4.354	3.603	135.5E6	332.7E6	54.911m	57.501
4)	MA Heptachlor	4.948	3.943	140.2E6	324.2E6	55.681	58.222
5)	MB Aldrin	5.292	4.221	137.6E6	327.3E6	56.833	59.221
6)	B beta-BHC	4.552	3.899	53668917	133.9E6	49.469	53.373
7)	B delta-BHC	4.801	4.129	136.4E6	333.0E6	55.702	56.286
8)	B Heptachlo...	5.719	4.722	118.1E6	281.6E6	52.880	55.126
9)	A Endosulfan I	6.107	5.093	113.2E6	236.0E6	54.384	52.319
10)	B trans-Chl...	5.975	4.972	118.6E6	292.1E6	54.775m	58.664
11)	B cis-Chlor...	6.056	5.036	120.2E6	285.3E6	53.812	56.176
12)	B 4,4'-DDE	6.227	5.224	230.1E6	610.9E6	105.533	128.108
13)	MA Dieldrin	6.383	5.354	240.5E6	634.3E6	109.425	126.940m
14)	MA Endrin	6.614	5.631	193.7E6	513.6E6	108.600	117.436
15)	B Endosulfa...	6.833	5.924	199.2E6	492.5E6	103.416	116.871
16)	A 4,4'-DDD	6.746	5.778	177.3E6	442.5E6	114.334	117.587
17)	MA 4,4'-DDT	7.063	6.028	223.1E6	526.5E6	138.687	137.120
18)	B Endrin al...	6.964	6.104	145.7E6	343.5E6	104.859	108.922
19)	B Endosulfa...	7.200	6.326	184.5E6	447.5E6	104.513	111.316
20)	A Methoxychlor	7.539	6.603	450.3E6	1021.4E6	520.560	520.524
21)	B Endrin ke...	7.687	6.832	194.8E6	467.5E6	103.360	103.952

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052624\
Data File : PD083062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2024 19:02
Operator : AR\AJ
Sample : P2568-04MS
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 22:18:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

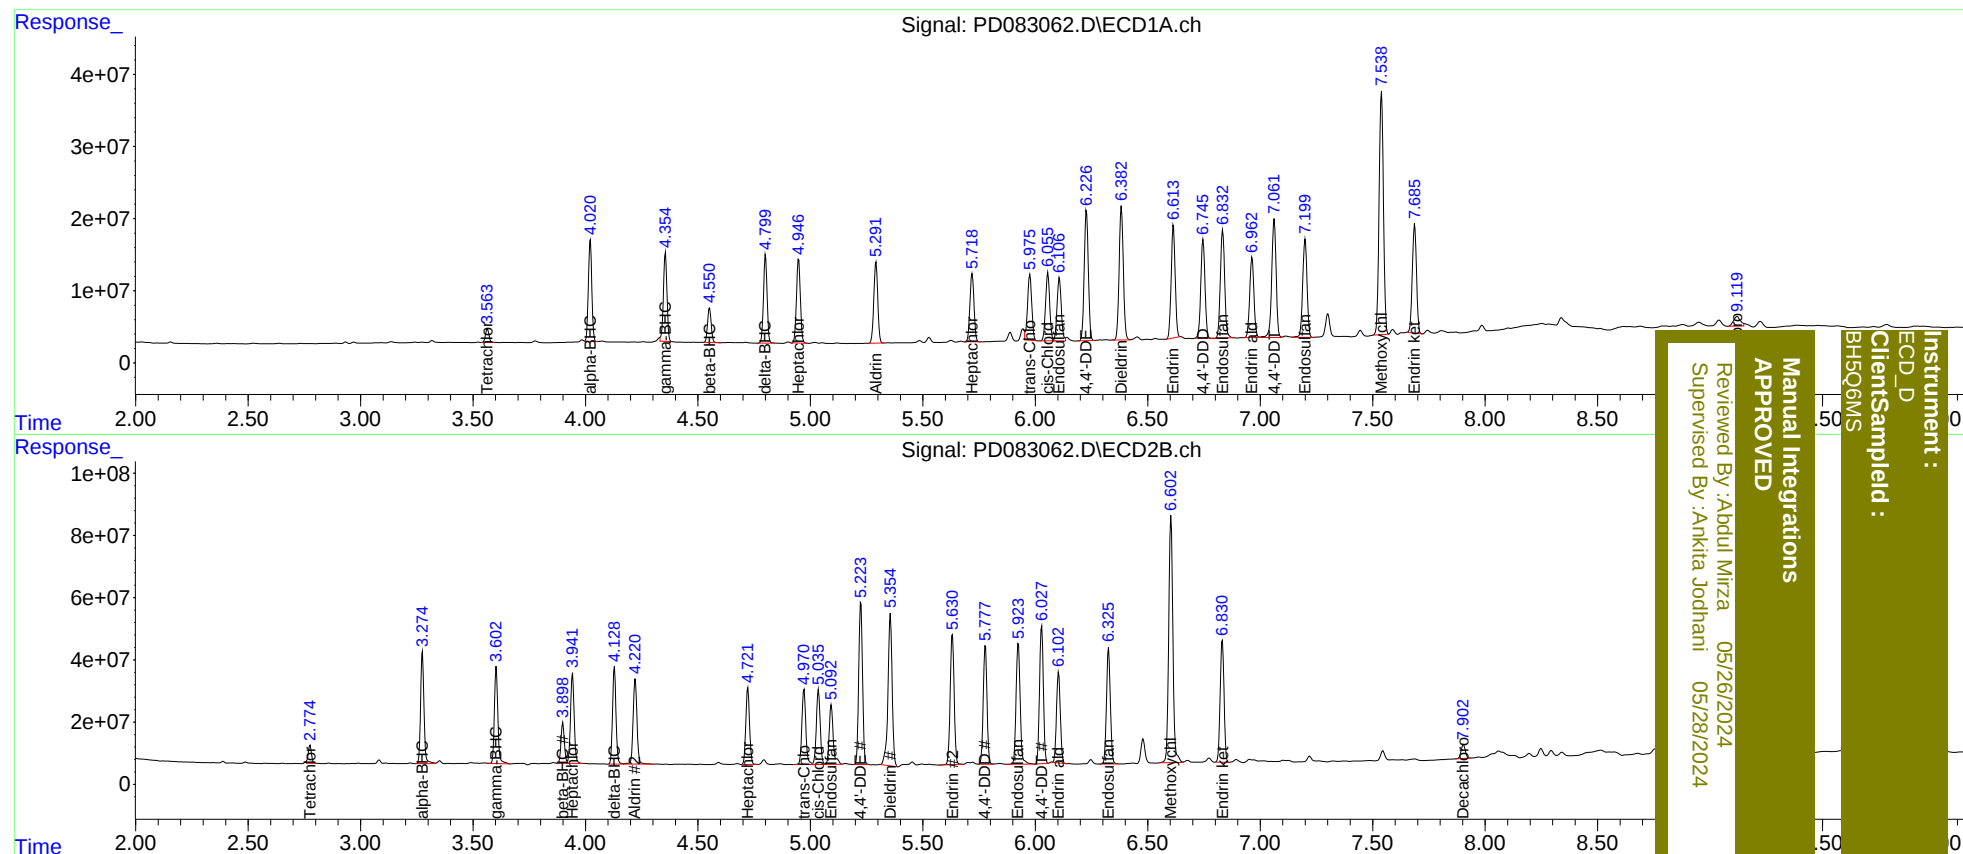

Instrument :
ECD_D
Client Sampled :
BH506MS

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 05/26/2024
Supervised By: Ankita Jodhani 05/28/2024