

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052624\
 Data File : PD083044.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2024 11:14
 Operator : AR\AJ
 Sample : P2528-05MSD
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH9S9MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/26/2024
 Supervised By :Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 21:57:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.776	27634670	78793351	18.475	20.262
27)	SA Decachlor...	9.123	7.906	31402014	69137089	15.666	17.474
Target Compounds							
2)	A alpha-BHC	4.022	3.276	137.2E6	345.2E6	53.789m	55.533
3)	MA gamma-BHC...	4.357	3.604	123.3E6	305.1E6	49.964	52.734
4)	MA Heptachlor	4.950	3.943	126.5E6	297.2E6	50.240	53.376
5)	MB Aldrin	5.294	4.222	122.1E6	292.8E6	50.448	52.980
6)	B beta-BHC	4.553	3.900	53051984	127.6E6	48.901	50.896
7)	B delta-BHC	4.803	4.130	123.2E6	309.3E6	50.329	52.284
8)	B Heptachlo...	5.721	4.723	105.6E6	257.8E6	47.279	50.468
9)	A Endosulfan I	6.109	5.093	98162351	241.7E6	47.174	53.600
10)	B trans-Chl...	5.978	4.973	100.9E6	257.5E6	46.617	51.702
11)	B cis-Chlor...	6.057	5.037	102.2E6	258.3E6	45.774	50.862
12)	B 4,4'-DDE	6.230	5.226	204.8E6	502.4E6	93.902	105.349
13)	MA Dieldrin	6.385	5.357	209.1E6	520.1E6	95.136	104.078
14)	MA Endrin	6.615	5.633	173.2E6	454.3E6	97.146	103.877
15)	B Endosulfa...	6.835	5.926	175.0E6	437.6E6	90.855	103.842
16)	A 4,4'-DDD	6.748	5.779	153.6E6	402.6E6	99.046	106.998
17)	MA 4,4'-DDT	7.064	6.030	158.8E6	403.0E6	98.762	104.962
18)	B Endrin al...	6.966	6.105	131.0E6	328.3E6	94.297	104.094
19)	B Endosulfa...	7.201	6.328	163.1E6	411.7E6	92.392	102.418
20)	A Methoxychlor	7.541	6.606	394.8E6	921.2E6	456.420	469.468
21)	B Endrin ke...	7.688	6.834	175.5E6	453.0E6	93.077	100.732

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052624\
Data File : PD083044.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2024 11:14
Operator : AR\AJ
Sample : P2528-05MSD
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 21:57:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

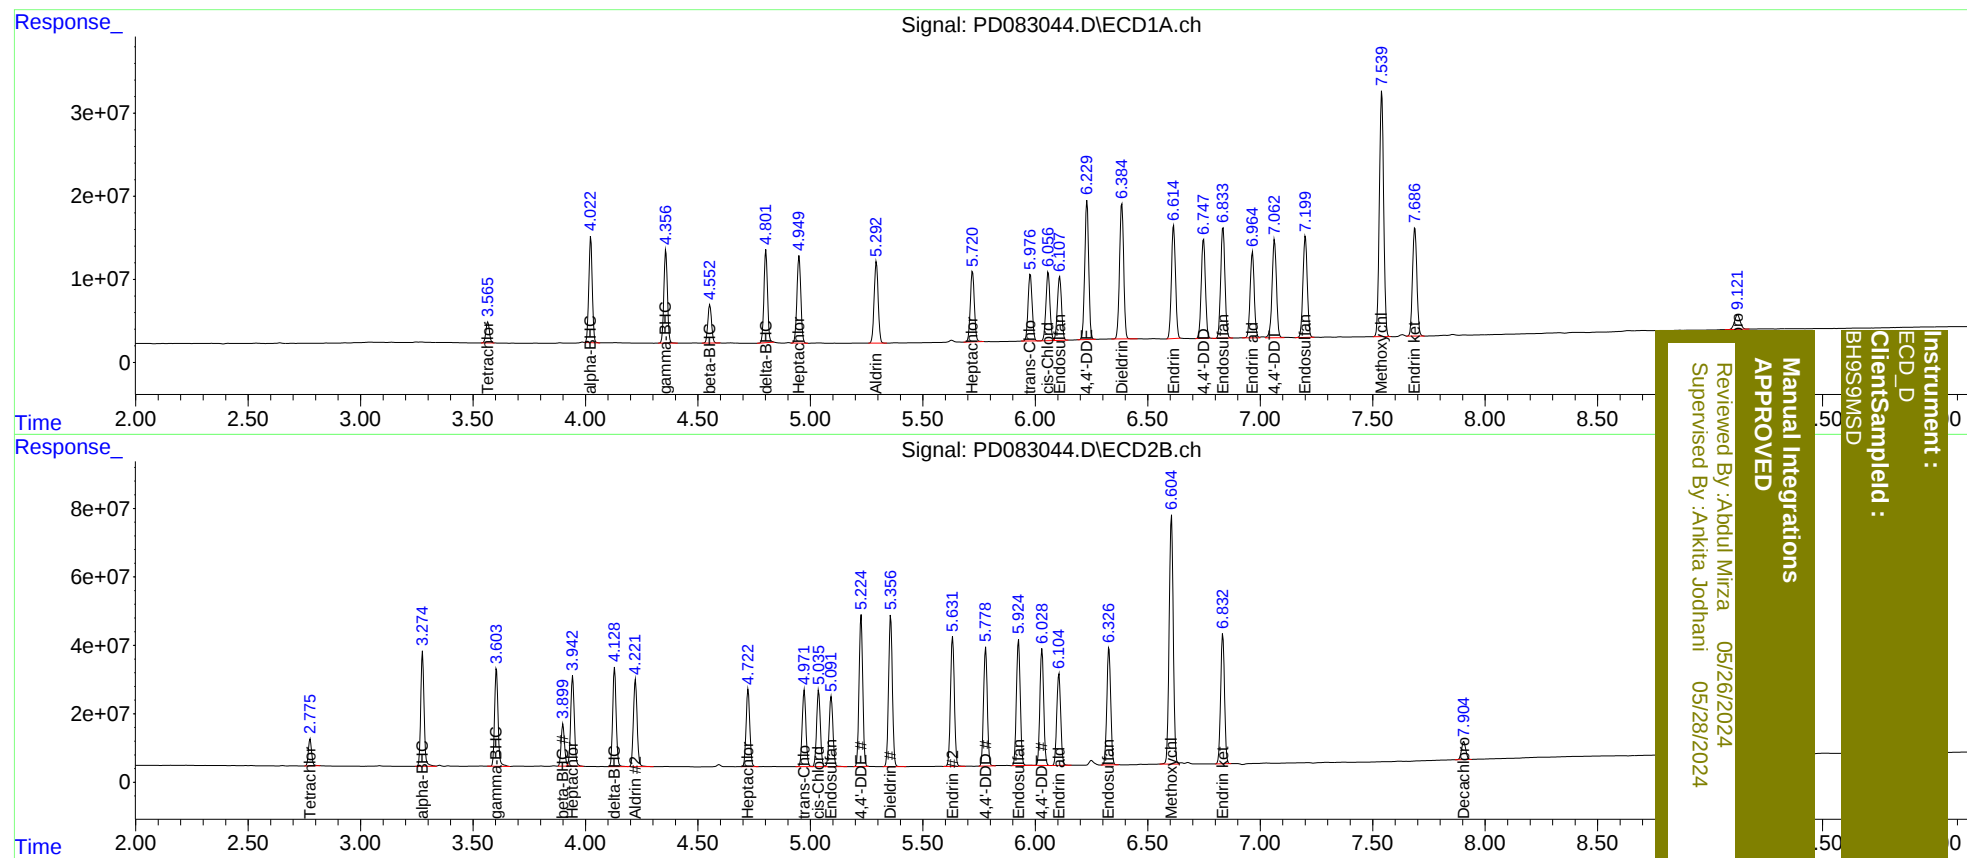

Instrument :
ECD_D
Client Sampled :
BH9S9MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 05/26/2024
Supervised By: Ankita Jodhani 05/28/2024