

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052624\
 Data File : PD083065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2024 20:08
 Operator : AR\AJ
 Sample : P2568-05MSD
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH5Q6MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/26/2024
 Supervised By : Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 22:22:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.774	19958555	57184276	13.344	14.705m
2)	SA Decachlor...	9.120	7.903	32842140	59551623	16.385m	15.052
Target Compounds							
2)	A alpha-BHC	4.021	3.275	149.3E6	376.8E6	58.509m	60.615
3)	MA gamma-BHC...	4.354	3.603	134.9E6	331.6E6	54.654m	57.305
4)	MA Heptachlor	4.948	3.942	138.3E6	322.4E6	54.929	57.897
5)	MB Aldrin	5.292	4.221	135.7E6	325.6E6	56.057	58.902
6)	B beta-BHC	4.552	3.899	53675334	133.6E6	49.475	53.272
7)	B delta-BHC	4.801	4.128	135.2E6	331.4E6	55.233	56.023
8)	B Heptachlo...	5.720	4.722	117.0E6	280.4E6	52.373	54.876
9)	A Endosulfan I	6.107	5.092	113.5E6	235.9E6	54.536	52.306
10)	B trans-Chl...	5.975	4.971	121.9E6	291.9E6	56.331m	58.620
11)	B cis-Chlor...	6.056	5.035	120.9E6	285.1E6	54.112	56.134
12)	B 4,4'-DDE	6.228	5.224	230.7E6	612.8E6	105.789	128.498
13)	MA Dieldrin	6.383	5.354	240.1E6	637.5E6	109.256	127.568m
14)	MA Endrin	6.615	5.631	191.2E6	513.5E6	107.242	117.403
15)	B Endosulfa...	6.833	5.924	198.2E6	494.0E6	102.899	117.213
16)	A 4,4'-DDD	6.746	5.778	175.7E6	444.1E6	113.300	118.025
17)	MA 4,4'-DDT	7.063	6.028	218.2E6	528.0E6	135.652	137.523
18)	B Endrin al...	6.964	6.103	143.5E6	344.4E6	103.322	109.191
19)	B Endosulfa...	7.199	6.326	183.6E6	447.5E6	104.019	111.315
20)	A Methoxychlor	7.539	6.604	441.6E6	1022.4E6	510.508	521.043
21)	B Endrin ke...	7.687	6.831	192.9E6	473.2E6	102.326	105.224

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052624\
Data File : PD083065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2024 20:08
Operator : AR\AJ
Sample : P2568-05MSD
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 22:22:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

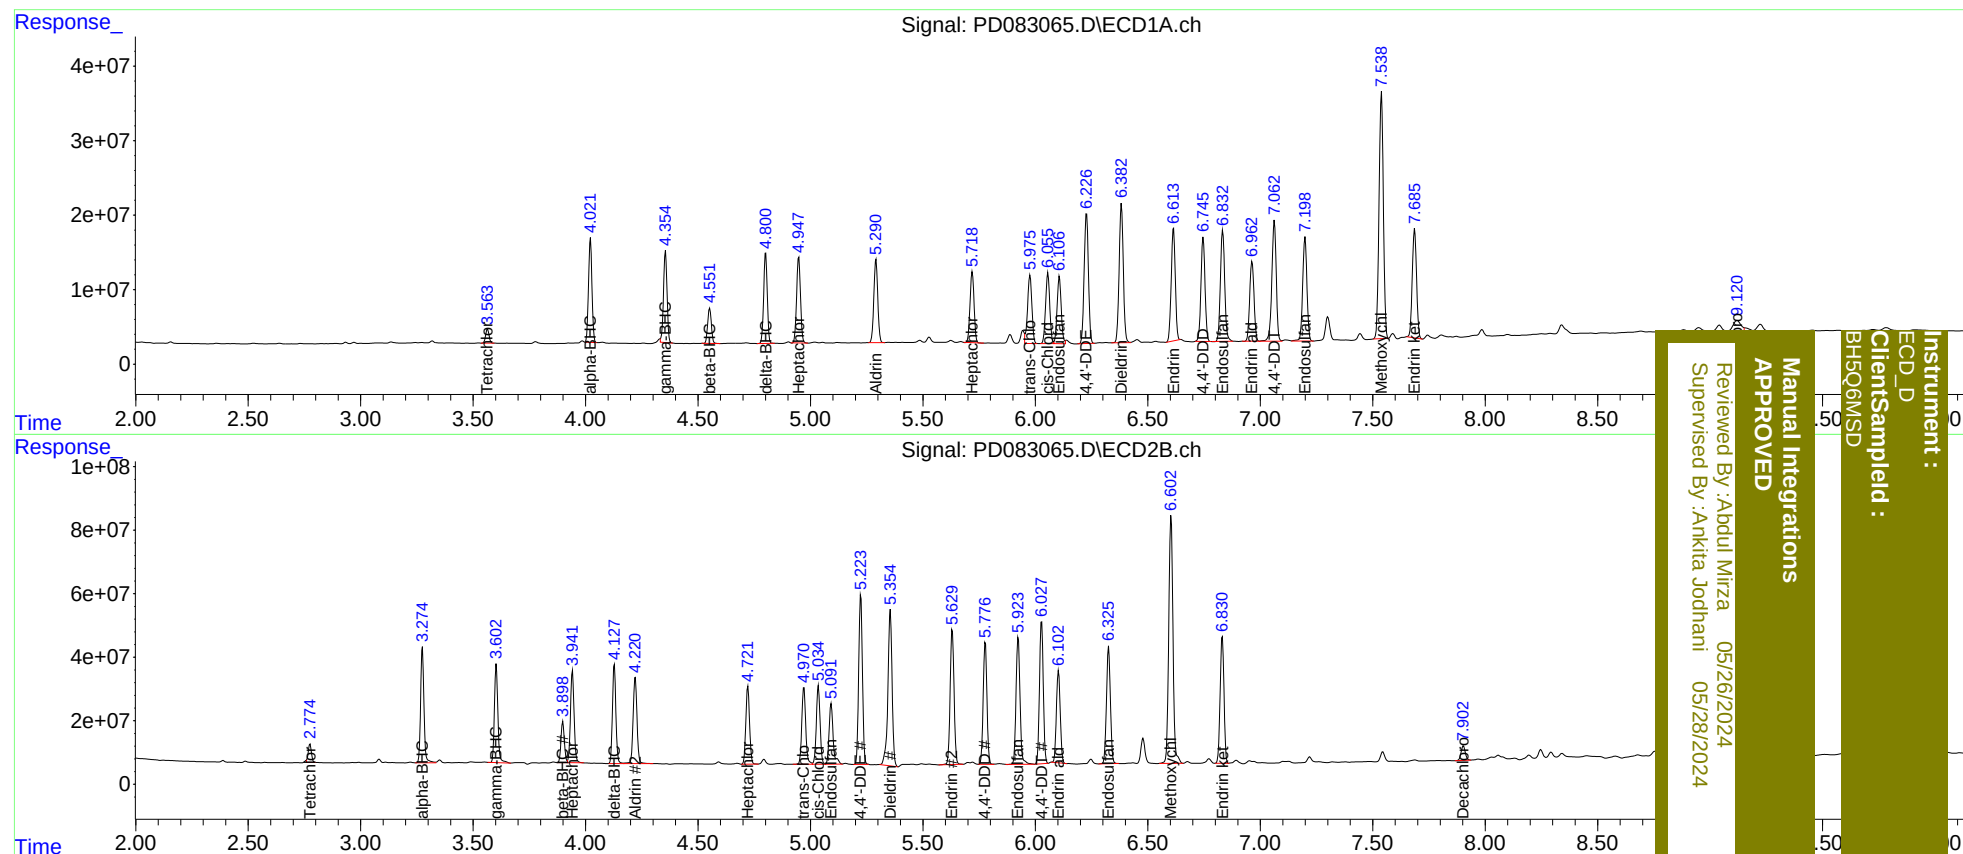

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/26/2024
Supervised By: Ankita Jodhani 05/28/2024

Instrument :
ECD_D
Client Sampled :
BH506MSD