

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052720\
 Data File : PD058126.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2020 09:03
 Operator : AJ\MA
 Sample : PB129082BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB129082BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 12:50:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.215	3.866	17602981	24638118	22.524	21.633
28)	SA Decachlor...	7.856	8.852	18394823	22932324	23.006	22.120
Target Compounds							
8)	B Heptachlo...	4.820f	0.000	135207	0	0.138	N.D. #
10)	B gamma-Chl...	5.078	0.000	79131	0	0.080	N.D. #
11)	B alpha-Chl...	5.131	0.000	32141	0	0.032	N.D. #
23)	Chlordane-1	4.046	0.000	749049	0	28.816	N.D. #
25)	Chlordane-3	5.078	0.000	79131	0	0.883	N.D. #
26)	Chlordane-4	5.131	0.000	32141	0	0.376	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052720\
Data File : PD058126.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2020 09:03
Operator : AJ\MA
Sample : PB129082BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB129082BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 12:50:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

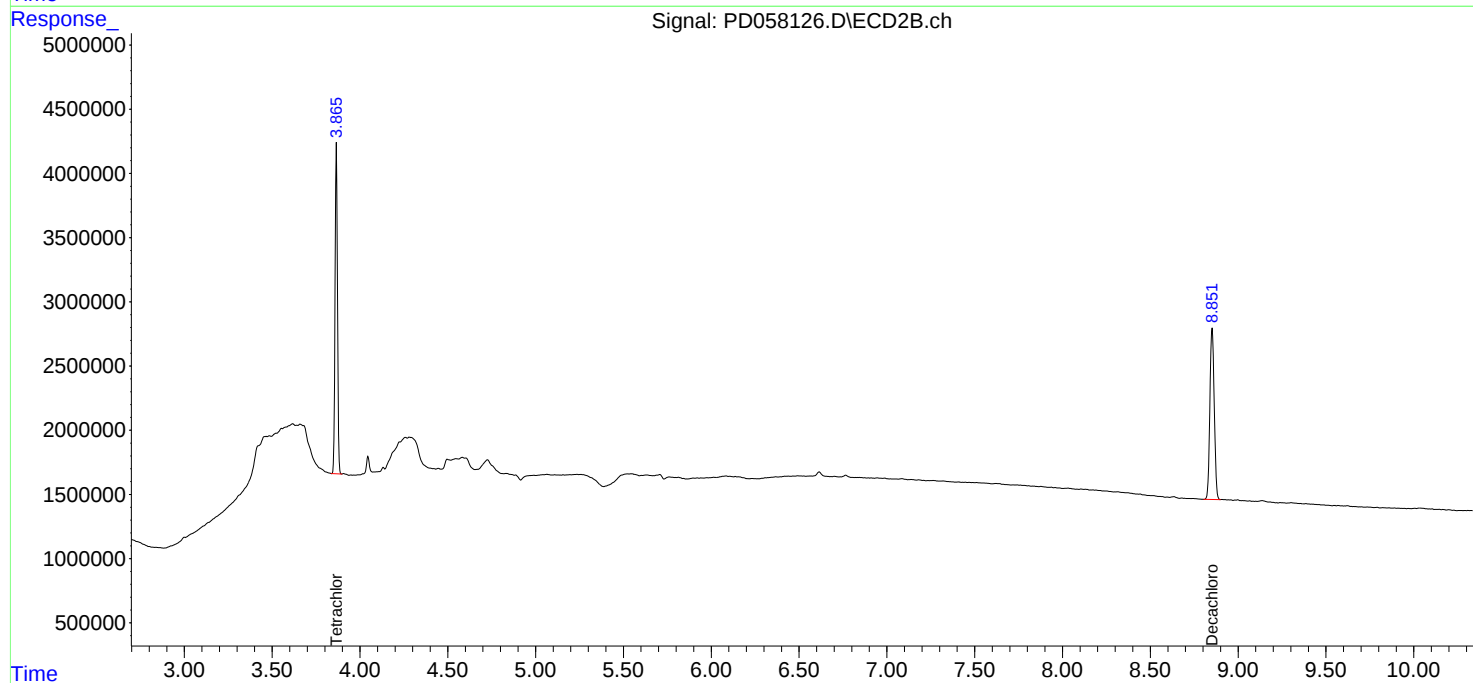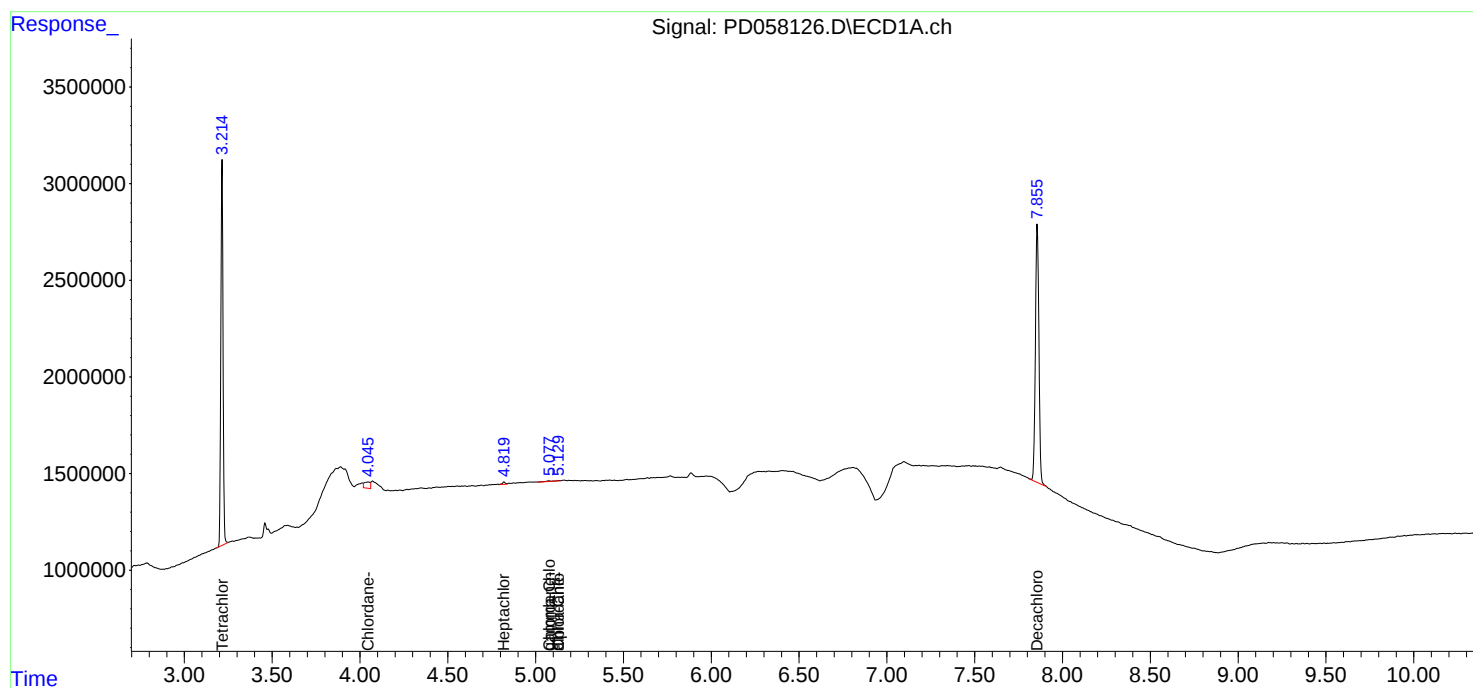


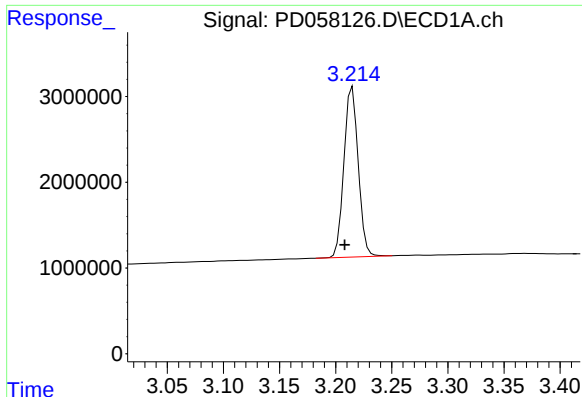

#1 Tetrachloro-m-xylene


R.T.: 3.215 min
Delta R.T.: 0.007 min
Response: 17602981
Conc: 22.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB129082BL

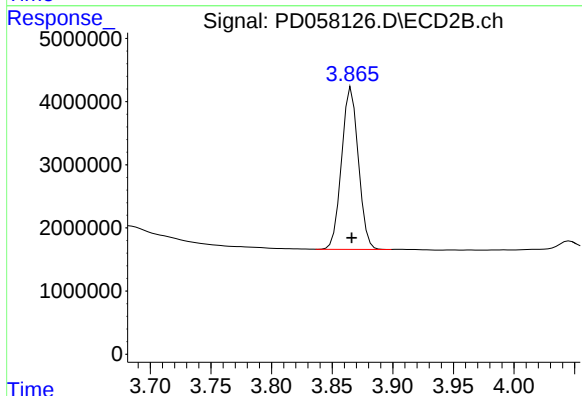


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 24638118
Conc: 21.63 ng/ml

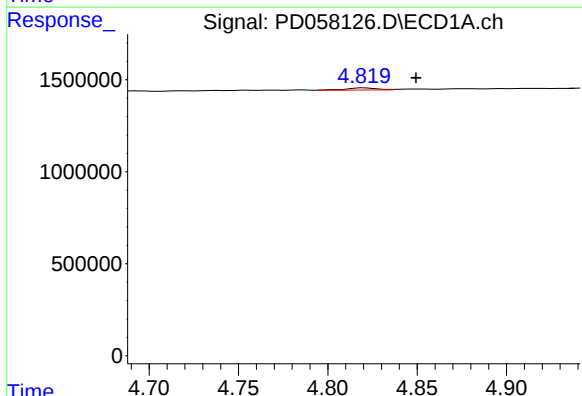


#8 Heptachlor epoxide

R.T.: 4.820 min
Delta R.T.: -0.029 min
Response: 135207
Conc: 0.14 ng/ml

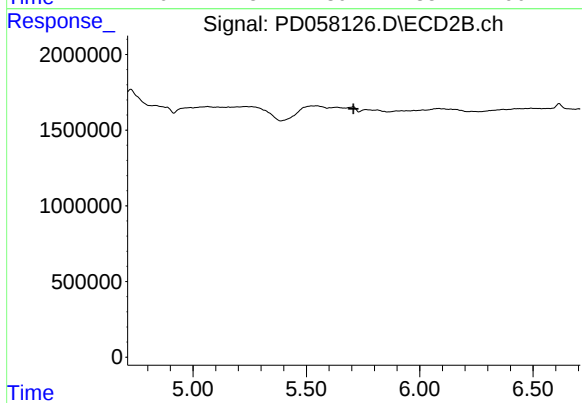

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.708 min
Response: 0
Conc: N.D.

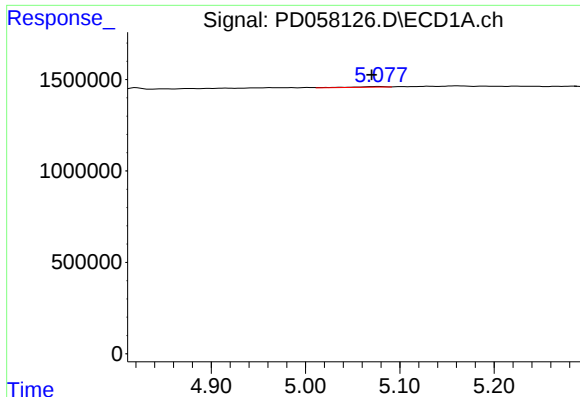

#10 gamma-Chlordane


R.T.: 5.078 min
Delta R.T.: 0.008 min
Response: 79131
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB129082BL

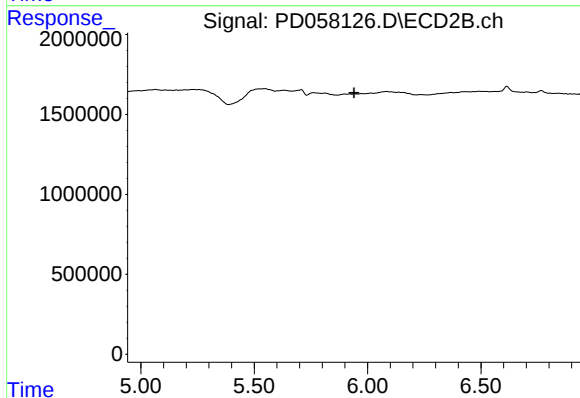


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.940 min
Response: 0
Conc: N.D.

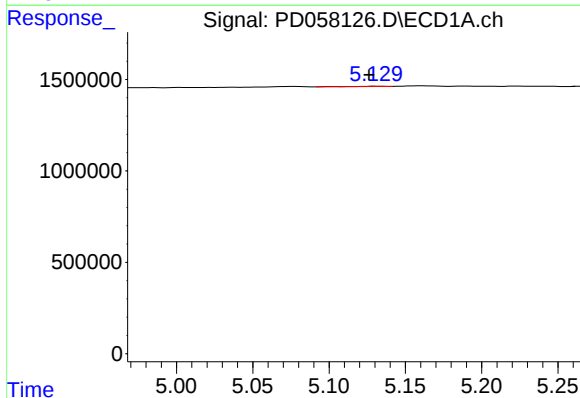


#11 alpha-Chlordane

R.T.: 5.131 min
Delta R.T.: 0.005 min
Response: 32141
Conc: 0.03 ng/ml

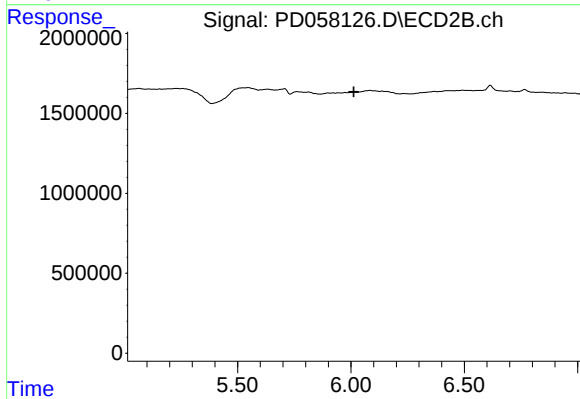

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.012 min
Response: 0
Conc: N.D.

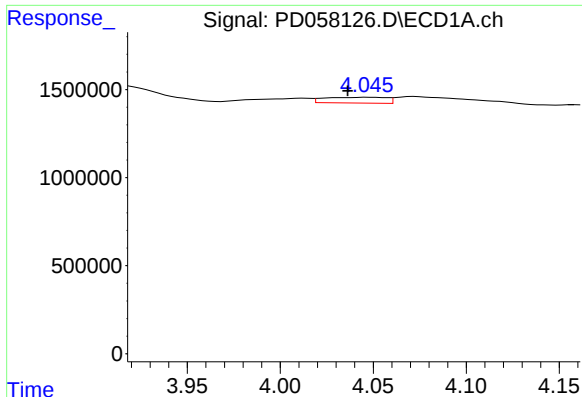

#23 Chlordane-1


R.T.: 4.046 min
Delta R.T.: 0.010 min
Response: 749049
Conc: 28.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB129082BL

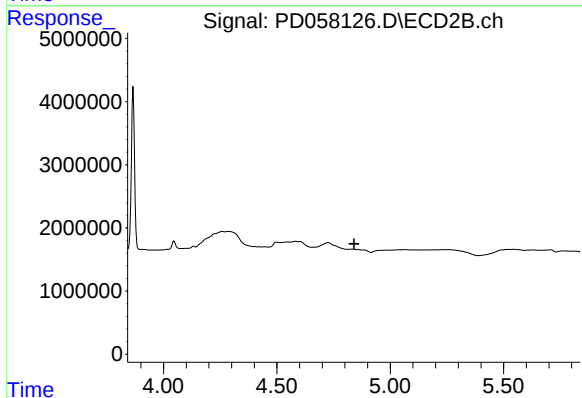


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.840 min
Response: 0
Conc: N.D.

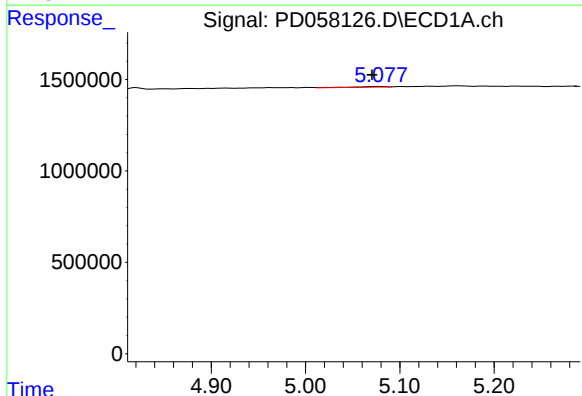


#25 Chlordane-3

R.T.: 5.078 min
Delta R.T.: 0.008 min
Response: 79131
Conc: 0.88 ng/ml

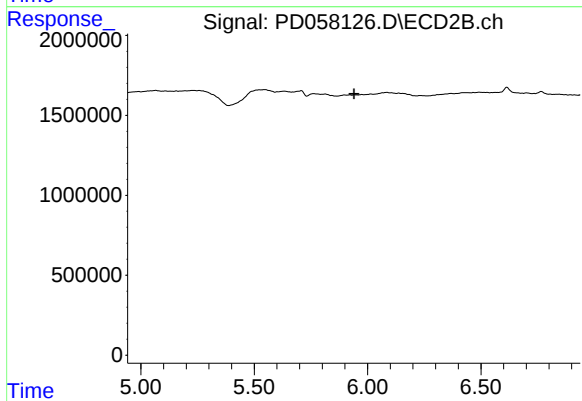

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.941 min
Response: 0
Conc: N.D.

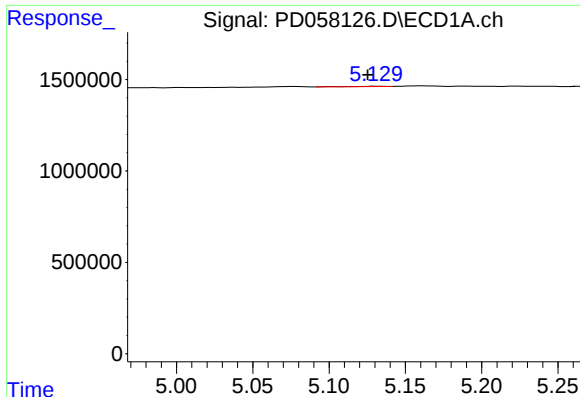

#26 Chlordane-4


R.T.: 5.131 min
Delta R.T.: 0.006 min
Response: 32141
Conc: 0.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB129082BL

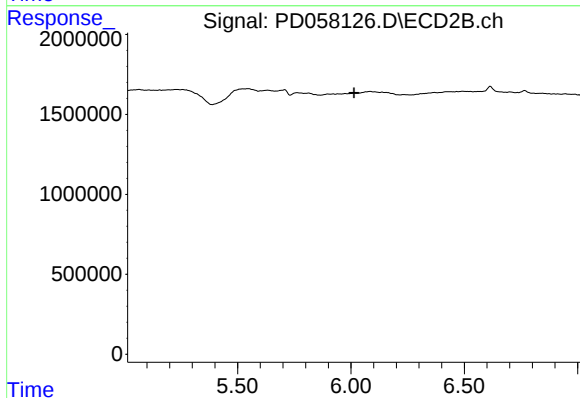


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.015 min
Response: 0
Conc: N.D.

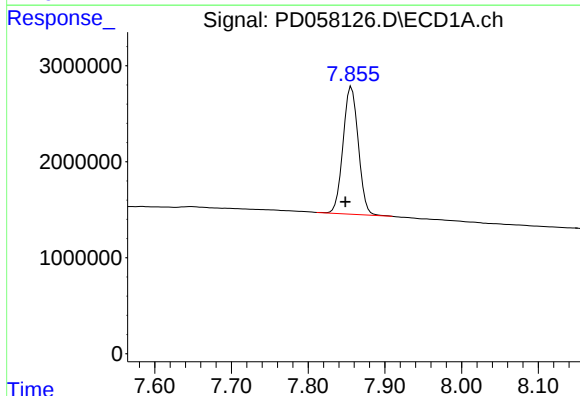

#28 Decachlorobiphenyl

R.T.: 7.856 min
Delta R.T.: 0.008 min
Response: 18394823
Conc: 23.01 ng/ml

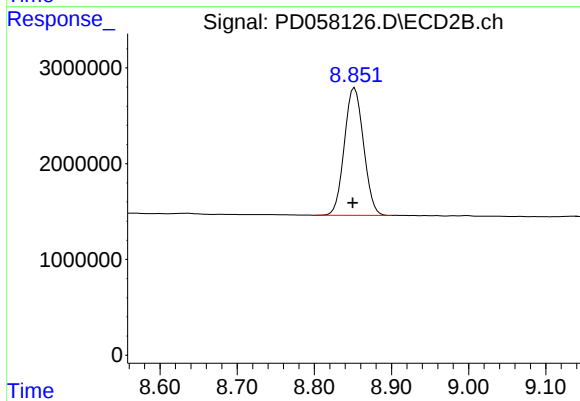

#28 Decachlorobiphenyl

R.T.: 8.852 min
Delta R.T.: 0.002 min
Response: 22932324
Conc: 22.12 ng/ml