

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052720\
 Data File : PD058136.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2020 12:44
 Operator : AJ\MA
 Sample : PB129111BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB129111BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 14:17:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.866	16548152	23138289	21.174	20.316
28)	SA Decachlor...	7.849	8.850	17467884	21831204	21.846	21.058
Target Compounds							
3)	MA gamma-BHC...	3.912	0.000	1076326	0	0.917	N.D. #
5)	MB Aldrin	4.397f	0.000	350102	0	0.334	N.D. #
9)	A Endosulfan I	5.149f	0.000	19903	0	0.022	N.D. #
11)	B alpha-Chl...	5.125	0.000	187449	0	0.190	N.D. #
14)	MA Endrin	5.692f	0.000	194736	0	0.243	N.D. #
24)	Chlordane-2	4.522	0.000	116924	0	3.657	N.D. #
25)	Chlordane-3	5.125f	0.000	187449	0	2.091	N.D. #
26)	Chlordane-4	5.125	0.000	187449	0	2.194	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052720\
Data File : PD058136.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2020 12:44
Operator : AJ\MA
Sample : PB129111BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB129111BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 14:17:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

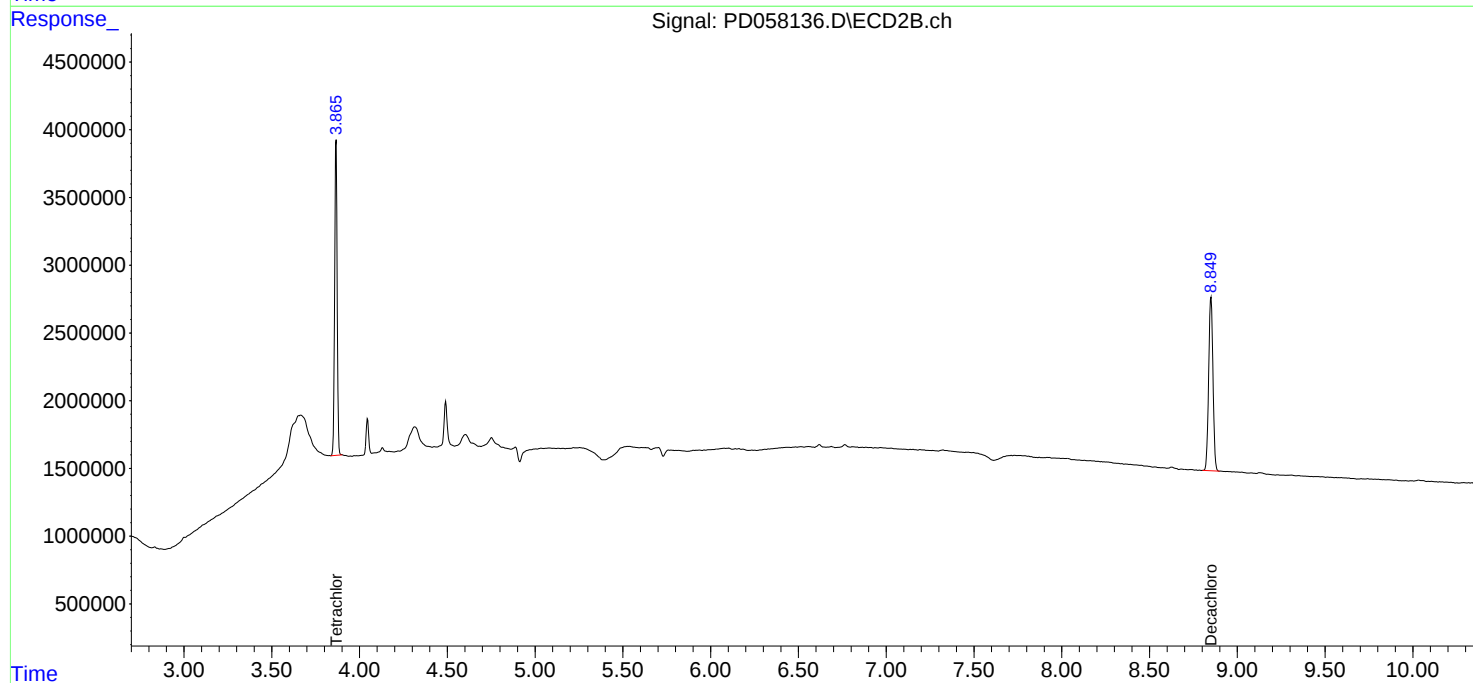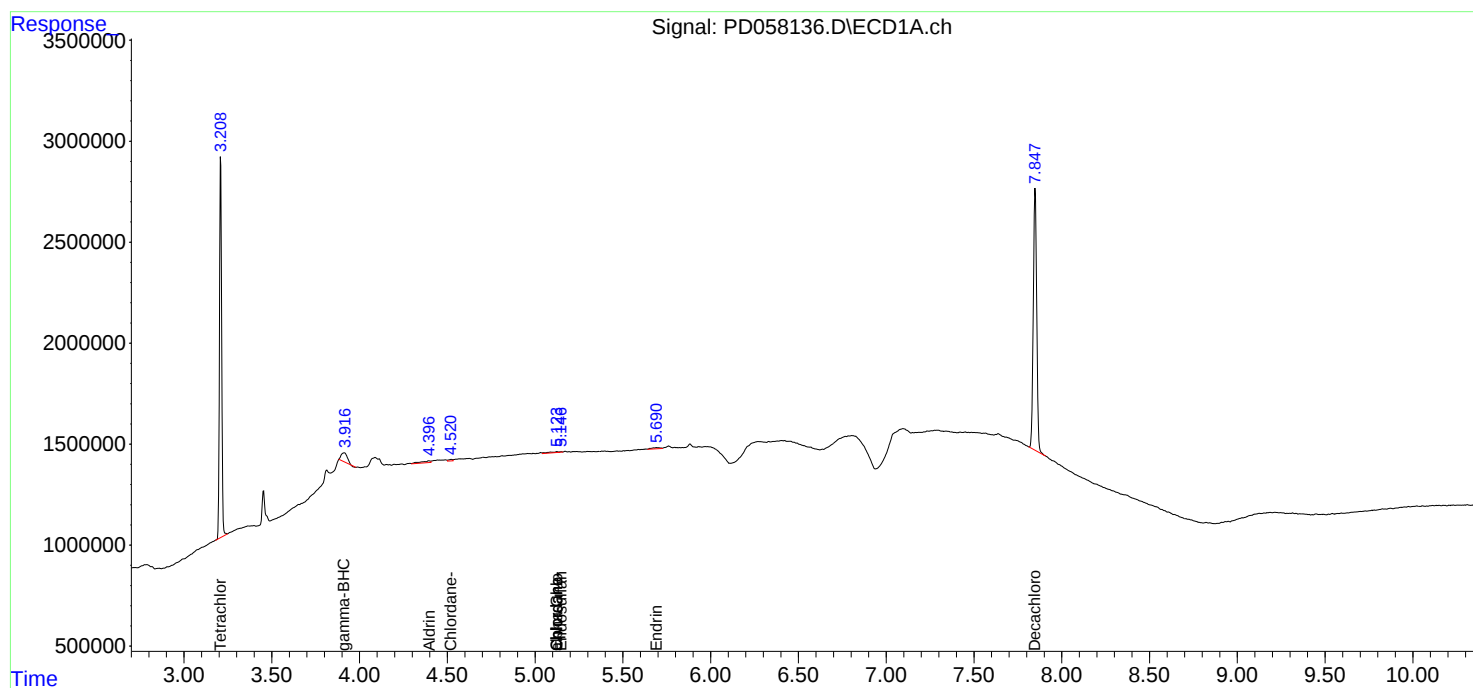


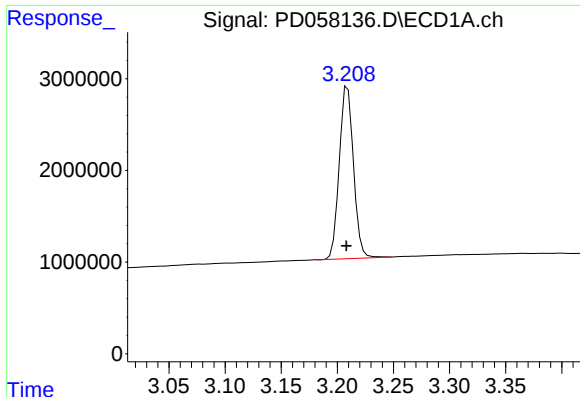

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.001 min
Response: 16548152
Conc: 21.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB129111BL

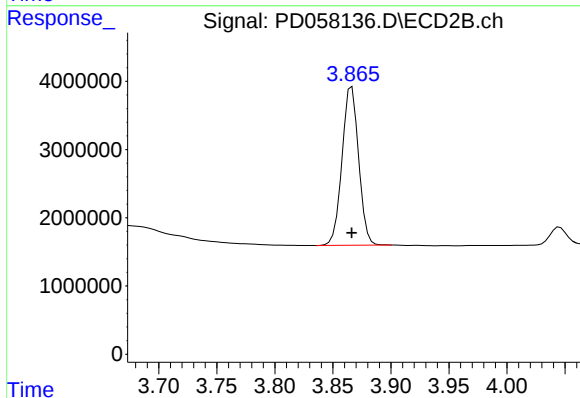


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 23138289
Conc: 20.32 ng/ml

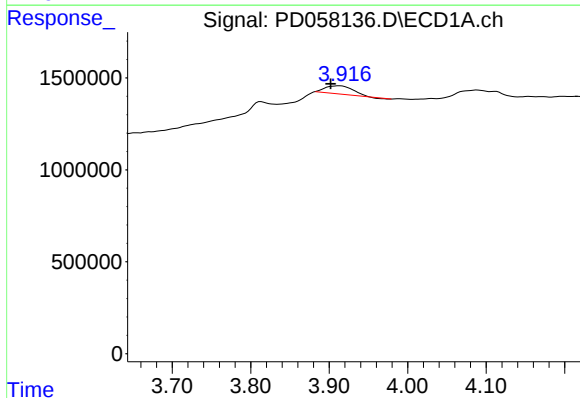


#3 gamma-BHC (Lindane)

R.T.: 3.912 min
Delta R.T.: 0.010 min
Response: 1076326
Conc: 0.92 ng/ml

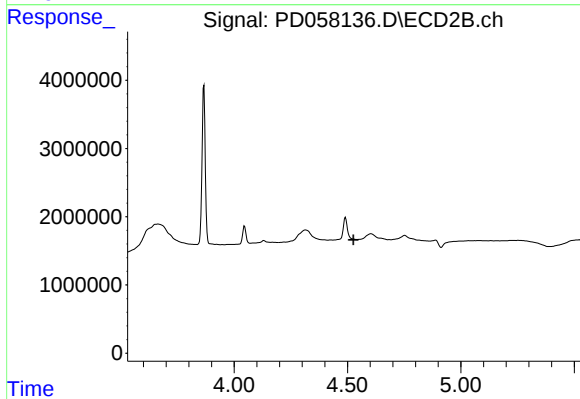

#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 4.527 min
Response: 0
Conc: N.D.

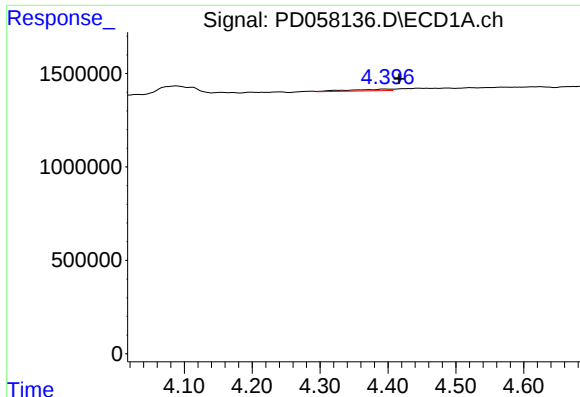

#5 Aldrin


R.T.: 4.397 min

Delta R.T.: -0.020 min

Response: 350102

Conc: 0.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB129111BL

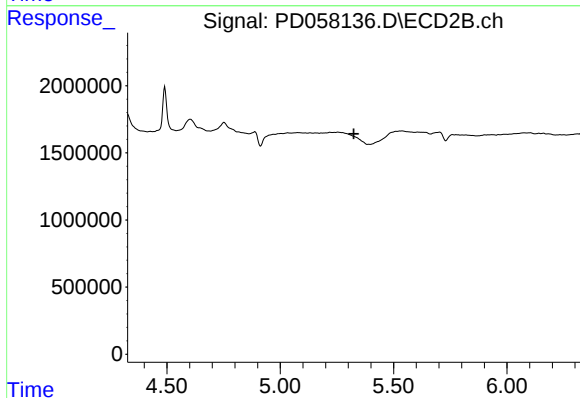


#5 Aldrin

R.T.: 0.000 min

Exp R.T. : 5.325 min

Response: 0

Conc: N.D.

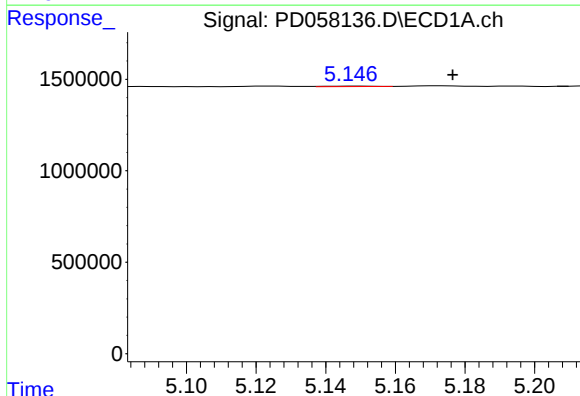


#9 Endosulfan I

R.T.: 5.149 min

Delta R.T.: -0.027 min

Response: 19903

Conc: 0.02 ng/ml

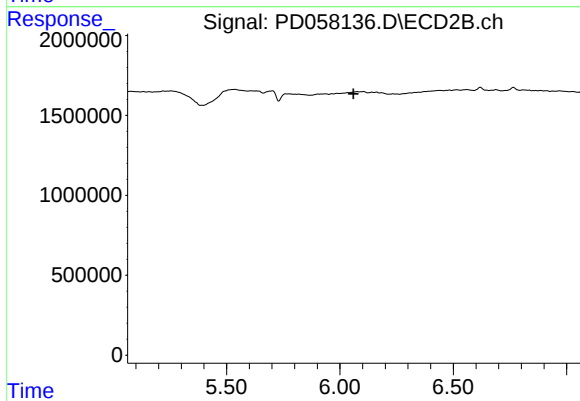


#9 Endosulfan I

R.T.: 0.000 min

Exp R.T. : 6.060 min

Response: 0


Conc: N.D.

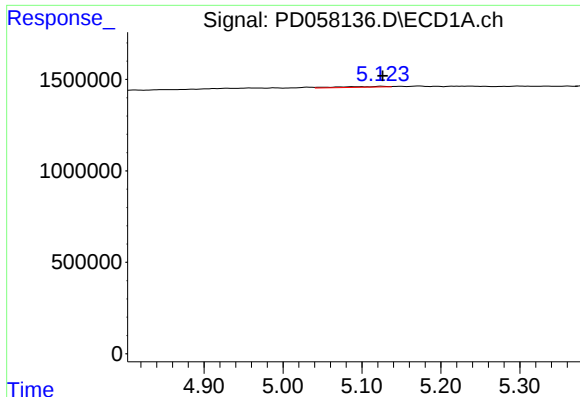

#11 alpha-Chlordane


R.T.: 5.125 min
Delta R.T.: -0.001 min
Response: 187449
Conc: 0.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB129111BL

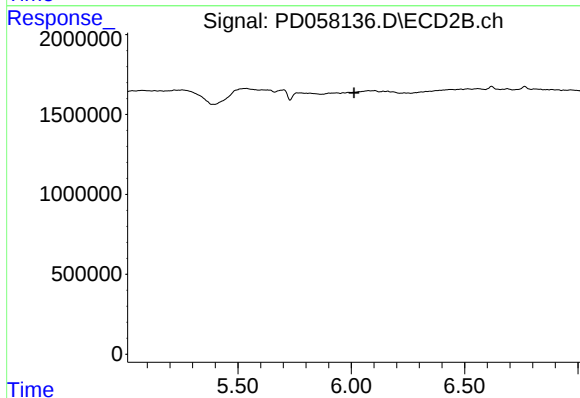


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.012 min
Response: 0
Conc: N.D.

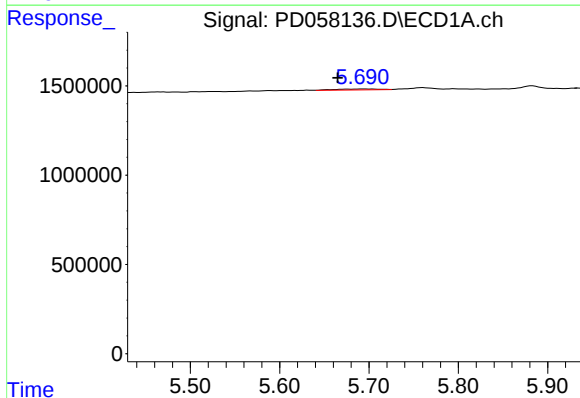


#14 Endrin

R.T.: 5.692 min
Delta R.T.: 0.027 min
Response: 194736
Conc: 0.24 ng/ml

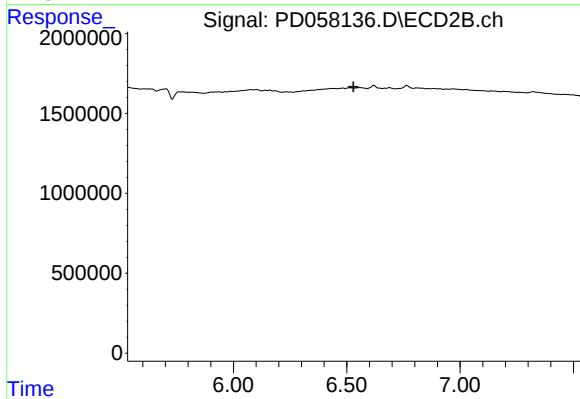

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.530 min
Response: 0
Conc: N.D.

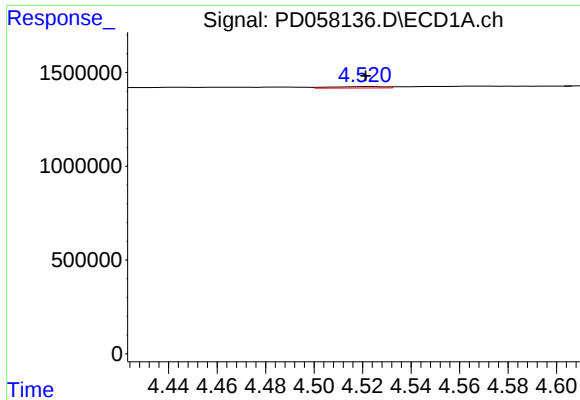

#24 Chlordane-2


R.T.: 4.522 min
Delta R.T.: 0.000 min
Response: 116924
Conc: 3.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB129111BL

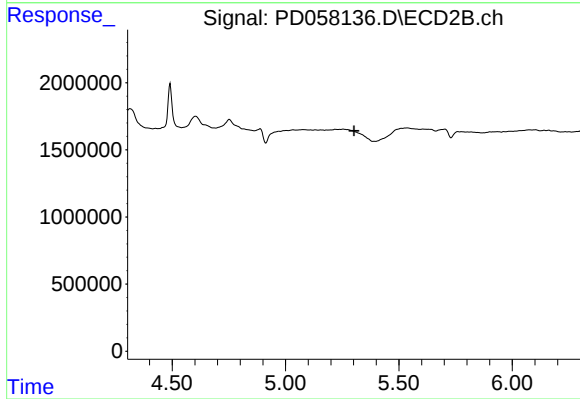


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.302 min
Response: 0
Conc: N.D.

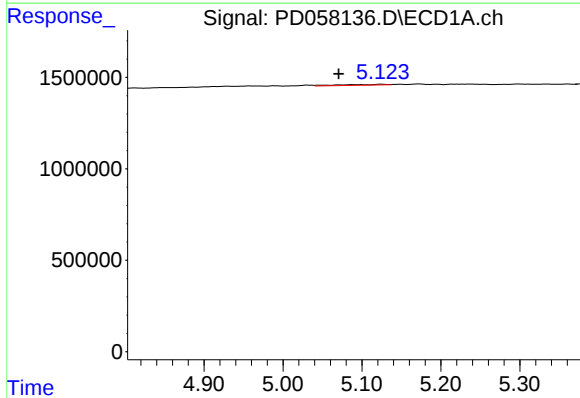


#25 Chlordane-3

R.T.: 5.125 min
Delta R.T.: 0.054 min
Response: 187449
Conc: 2.09 ng/ml

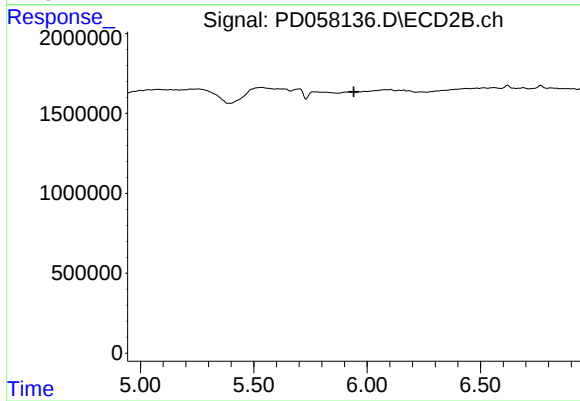

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.941 min
Response: 0
Conc: N.D.

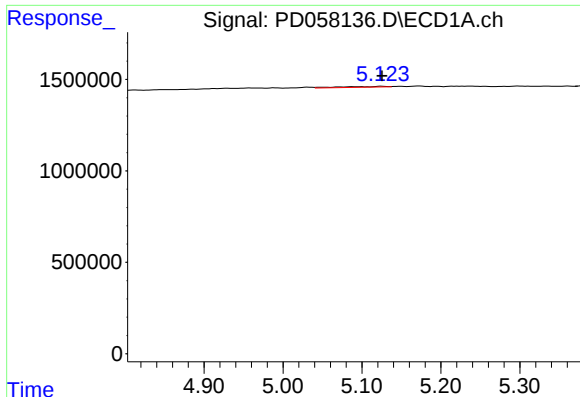

#26 Chlordane-4


R.T.: 5.125 min
Delta R.T.: 0.000 min
Response: 187449
Conc: 2.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB129111BL

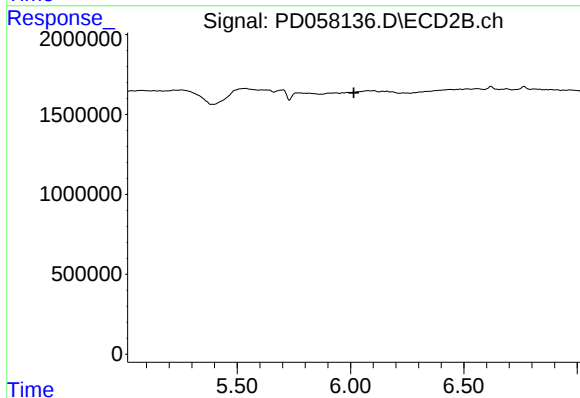


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.015 min
Response: 0
Conc: N.D.

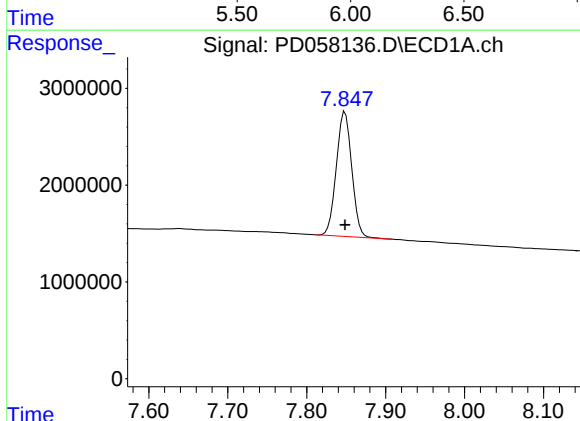

#28 Decachlorobiphenyl

R.T.: 7.849 min
Delta R.T.: 0.000 min
Response: 17467884
Conc: 21.85 ng/ml

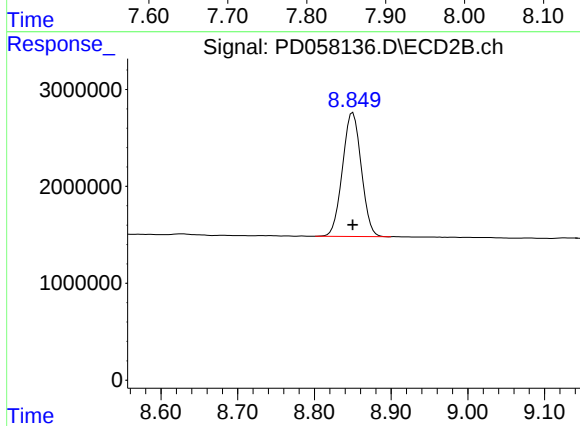

#28 Decachlorobiphenyl

R.T.: 8.850 min
Delta R.T.: 0.000 min
Response: 21831204
Conc: 21.06 ng/ml