

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052720\
 Data File : PD058148.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2020 15:34
 Operator : AJ\MA
 Sample : L2500-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 OK-03-052220

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 02:20:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.867	16670458	23186018	21.330	20.358
28)	SA Decachlor...	7.849	8.851	15937027	19585671	19.932	18.892
Target Compounds							
2)	A alpha-BHC	3.642	0.000	95406	0	0.079	N.D. #
3)	MA gamma-BHC...	3.913	0.000	1877135	0	1.600	N.D. #
4)	MA Heptachlor	4.184	0.000	95308	0	0.089	N.D. #
13)	MA Dieldrin	5.405	0.000	296624	0	0.302	N.D. #
16)	A 4,4'-DDD	5.818	0.000	220858	0	0.274	N.D. #
24)	Chlordane-2	4.541f	0.000	347864	0	10.881	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052720\
Data File : PD058148.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2020 15:34
Operator : AJ\MA
Sample : L2500-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
OK-03-052220

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 02:20:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

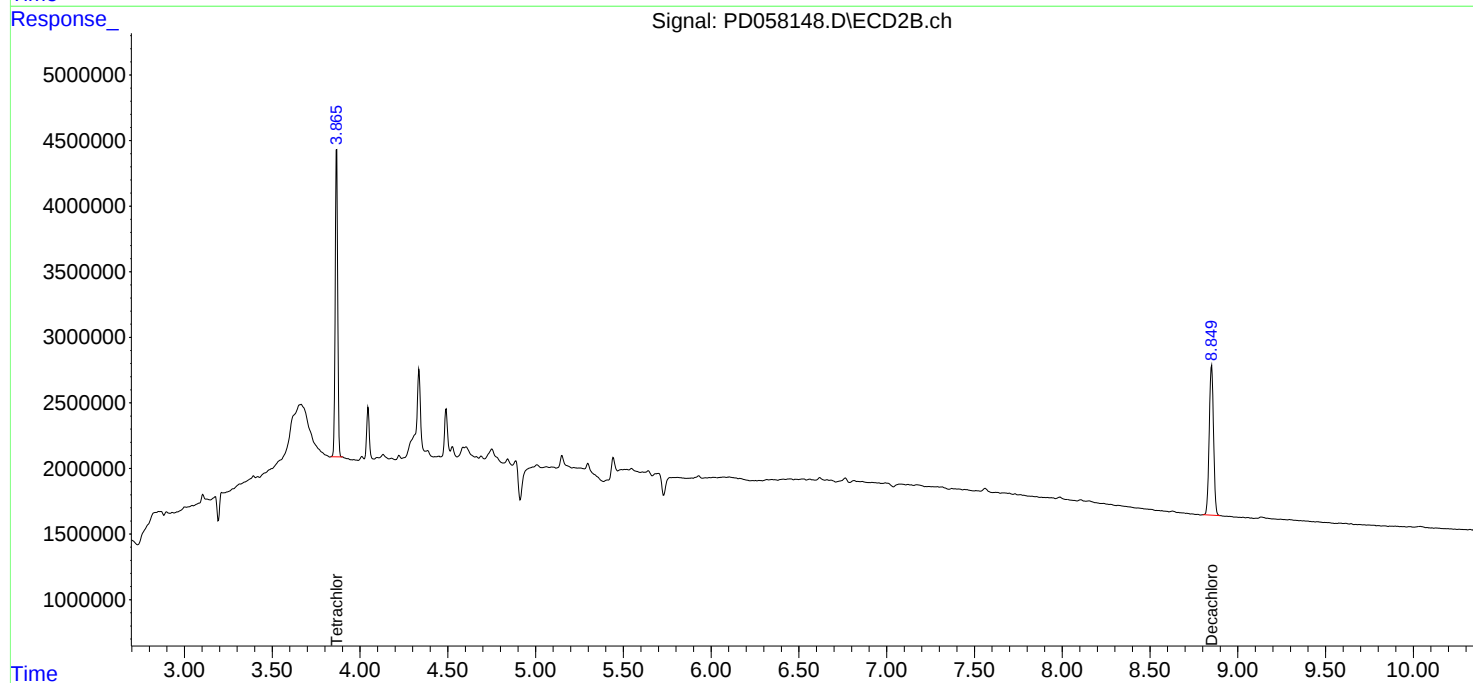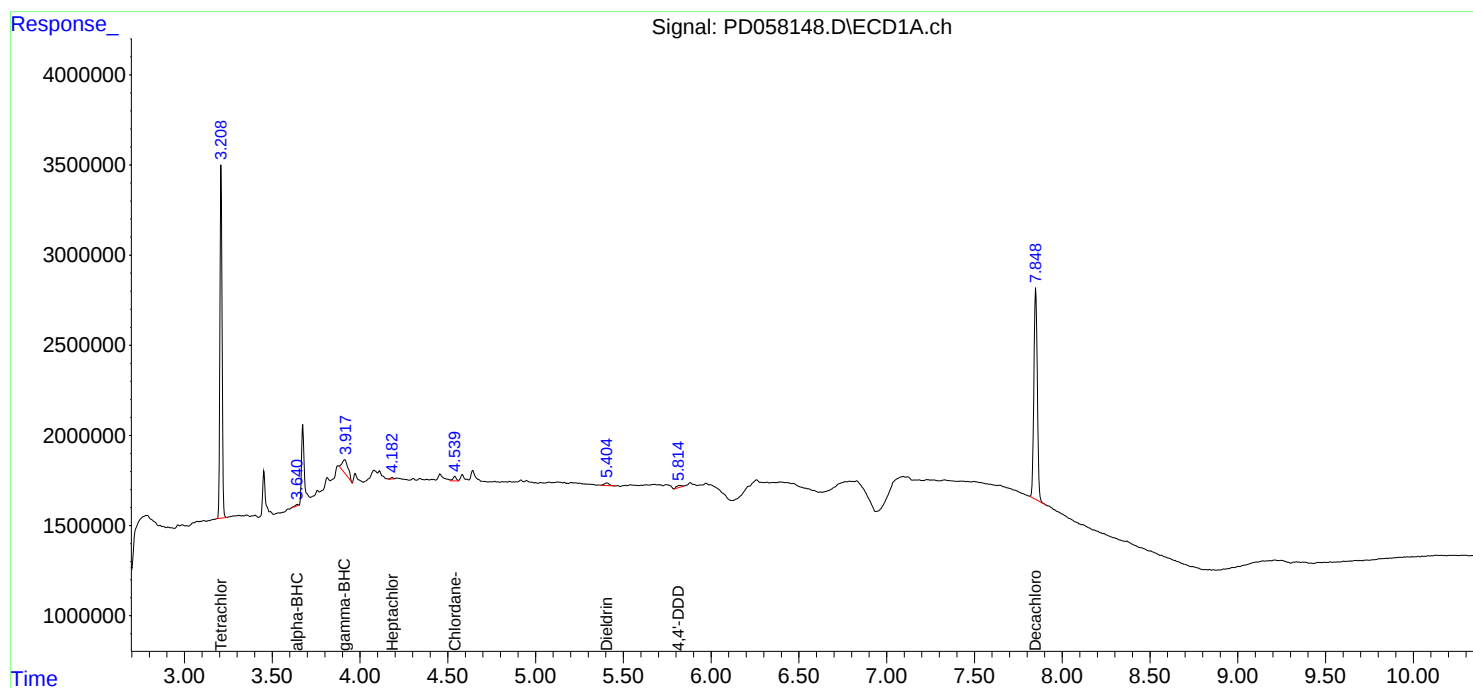


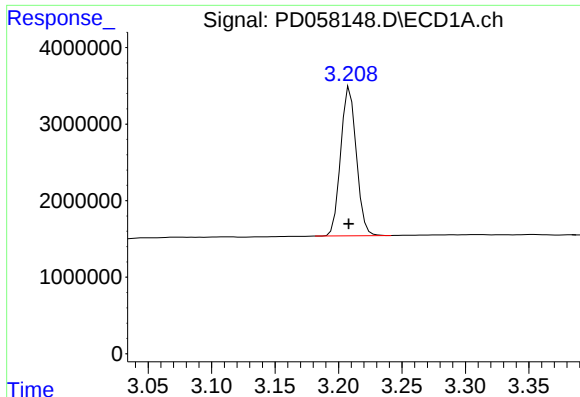

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.001 min
Response: 16670458
Conc: 21.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
OK-03-052220

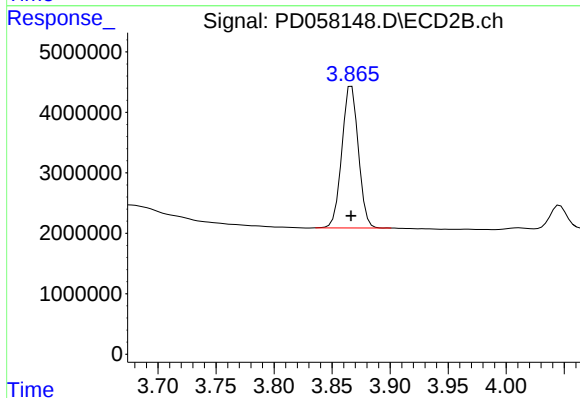


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 23186018
Conc: 20.36 ng/ml

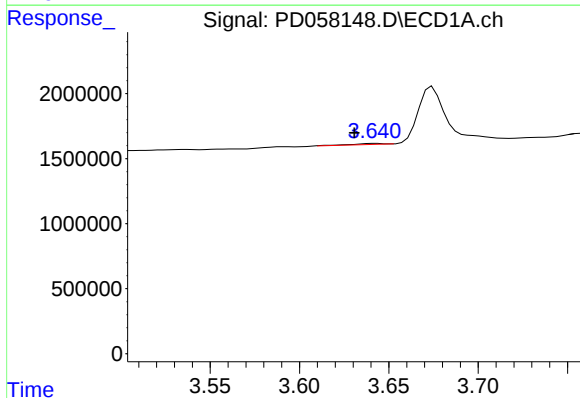


#2 alpha-BHC

R.T.: 3.642 min
Delta R.T.: 0.011 min
Response: 95406
Conc: 0.08 ng/ml

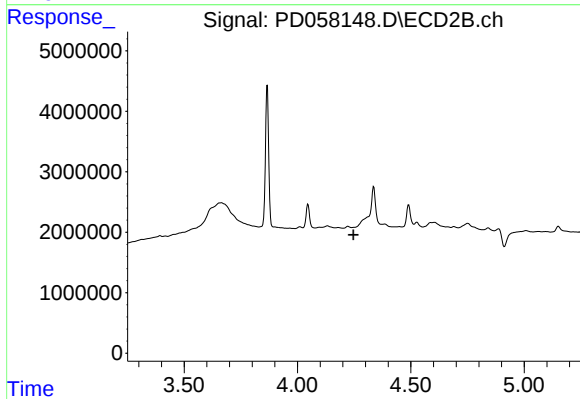

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.247 min
Response: 0
Conc: N.D.

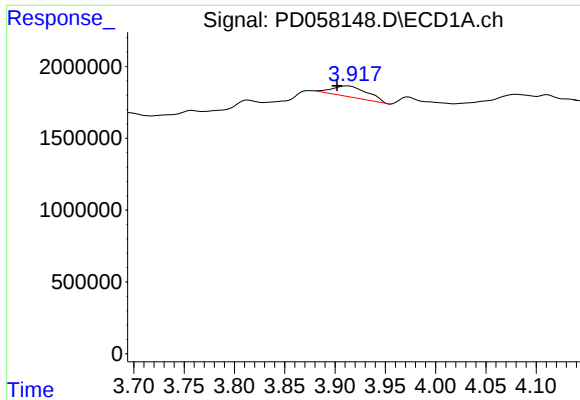

#3 gamma-BHC (Lindane)


R.T.: 3.913 min
Delta R.T.: 0.011 min
Response: 1877135
Conc: 1.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
OK-03-052220

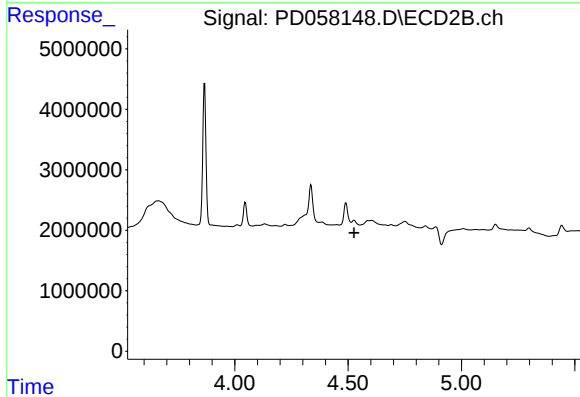


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.527 min
Response: 0
Conc: N.D.

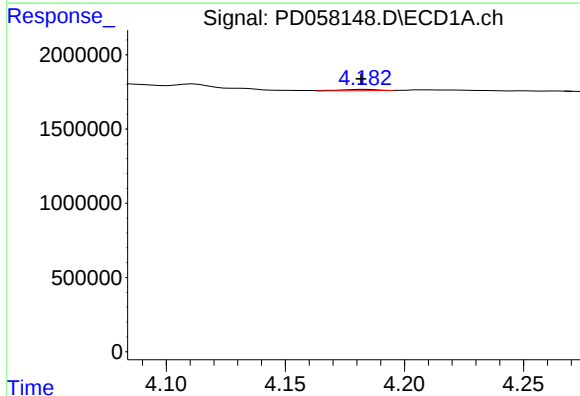


#4 Heptachlor

R.T.: 4.184 min
Delta R.T.: 0.002 min
Response: 95308
Conc: 0.09 ng/ml

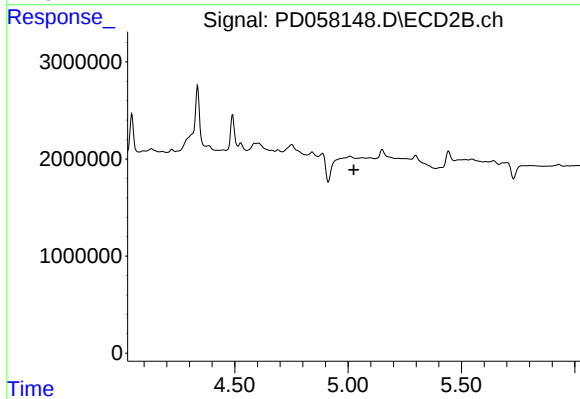

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.026 min
Response: 0
Conc: N.D.

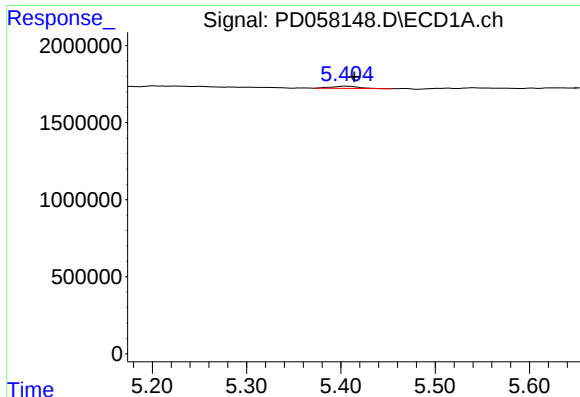

#13 Dieldrin


R.T.: 5.405 min
Delta R.T.: -0.009 min
Response: 296624
Conc: 0.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
OK-03-052220

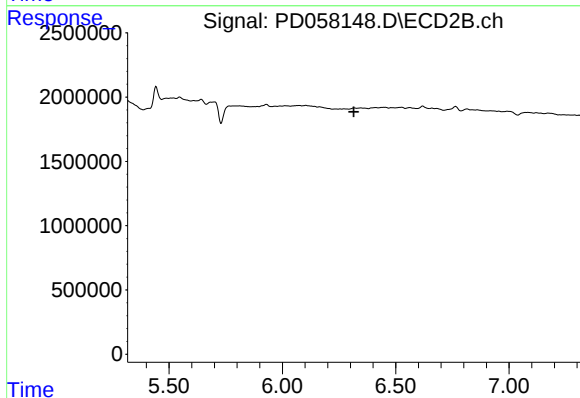


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.315 min
Response: 0
Conc: N.D.

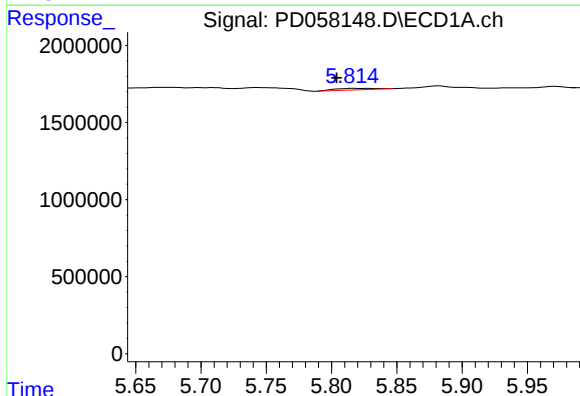


#16 4,4'-DDD

R.T.: 5.818 min
Delta R.T.: 0.014 min
Response: 220858
Conc: 0.27 ng/ml

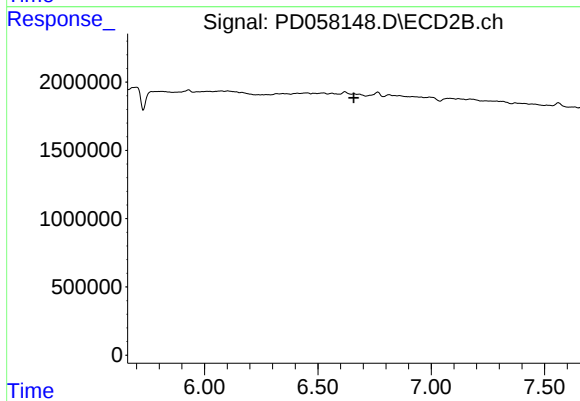

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.658 min
Response: 0
Conc: N.D.

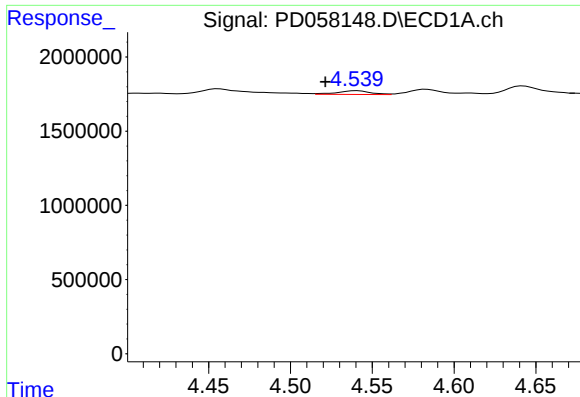

#24 Chlordane-2


R.T.: 4.541 min
Delta R.T.: 0.019 min
Response: 347864
Conc: 10.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
OK-03-052220

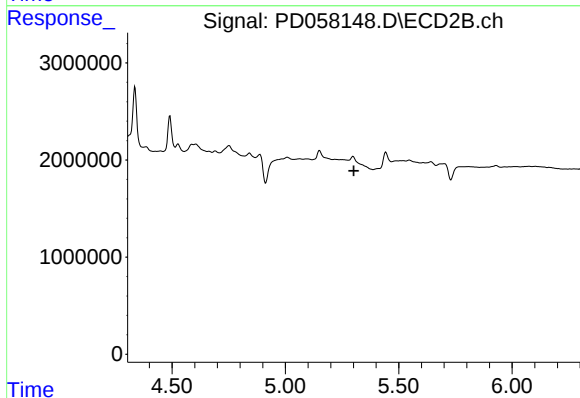


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.302 min
Response: 0
Conc: N.D.

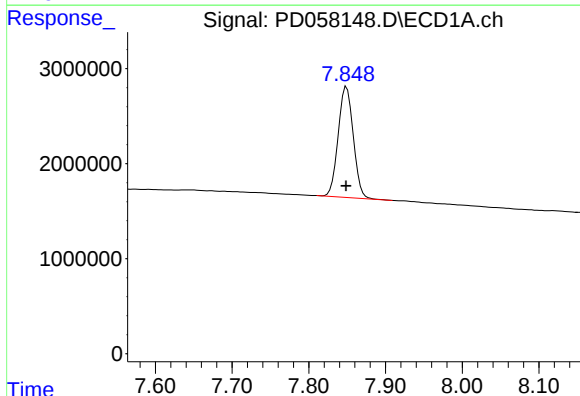

#28 Decachlorobiphenyl

R.T.: 7.849 min
Delta R.T.: 0.000 min
Response: 15937027
Conc: 19.93 ng/ml

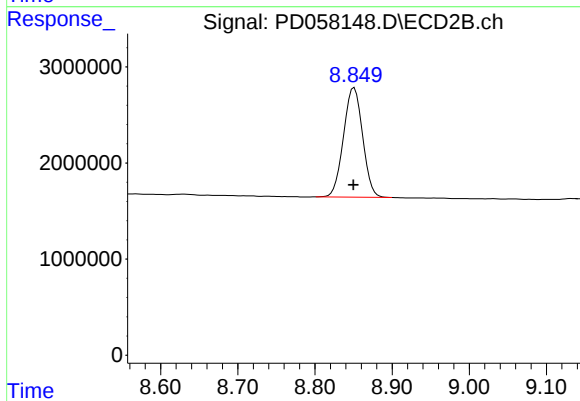

#28 Decachlorobiphenyl

R.T.: 8.851 min
Delta R.T.: 0.000 min
Response: 19585671
Conc: 18.89 ng/ml