

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052720\
 Data File : PD058130.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2020 10:14
 Operator : AJ\MA
 Sample : L2744-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 NM65-COMP-2020-0-6

Manual Integrations
 APPROVED

mohammad
 5/29/2020 12:32:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 14:14:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.866	10418173	14563761	13.330	12.788
28)	SA Decachlor...	7.849	8.849	9463129	11975392	11.835	11.551
Target Compounds							
12)	B 4,4'-DDE	5.295	6.168	891230	1159737	0.957m	0.908m
17)	MA 4,4'-DDT	6.032	6.953	1385653	731941	2.009m	0.735m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052720\
Data File : PD058130.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2020 10:14
Operator : AJ\MA
Sample : L2744-07
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
NM65-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/29/2020 12:32:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 14:14:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

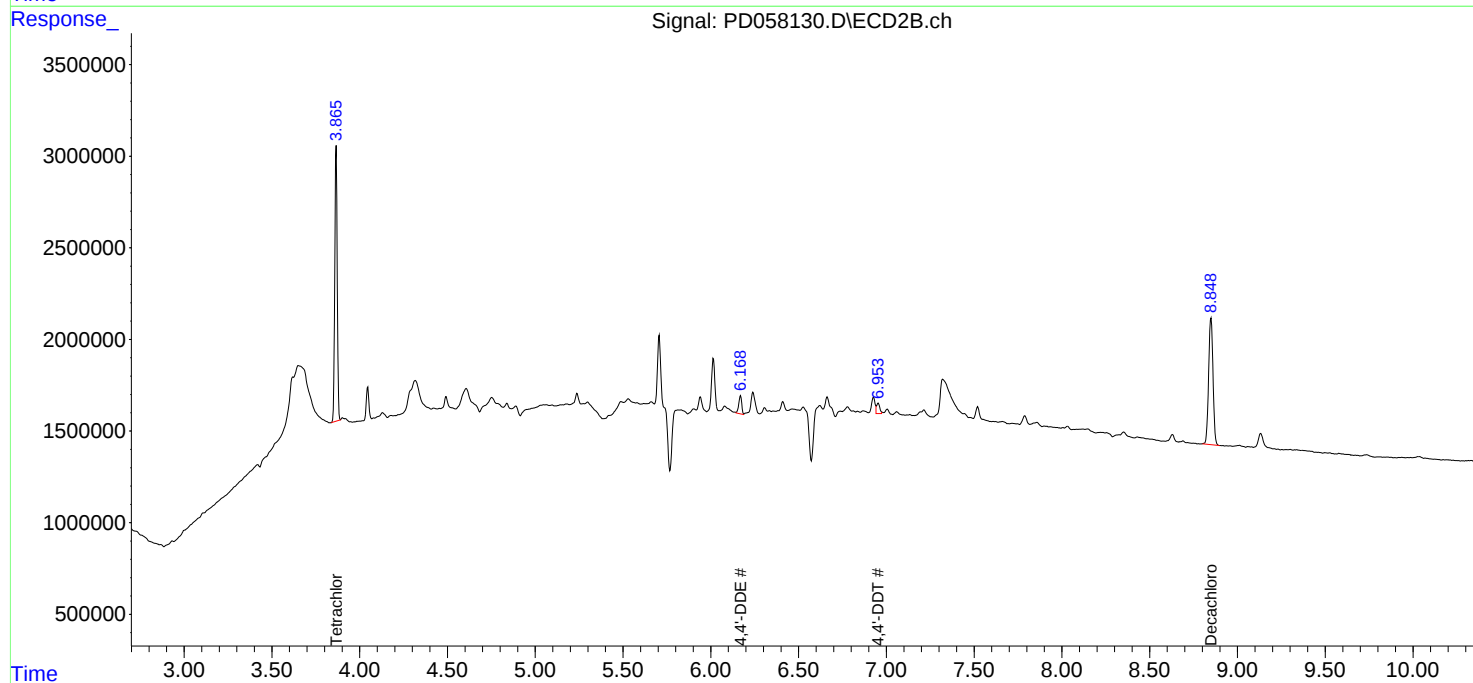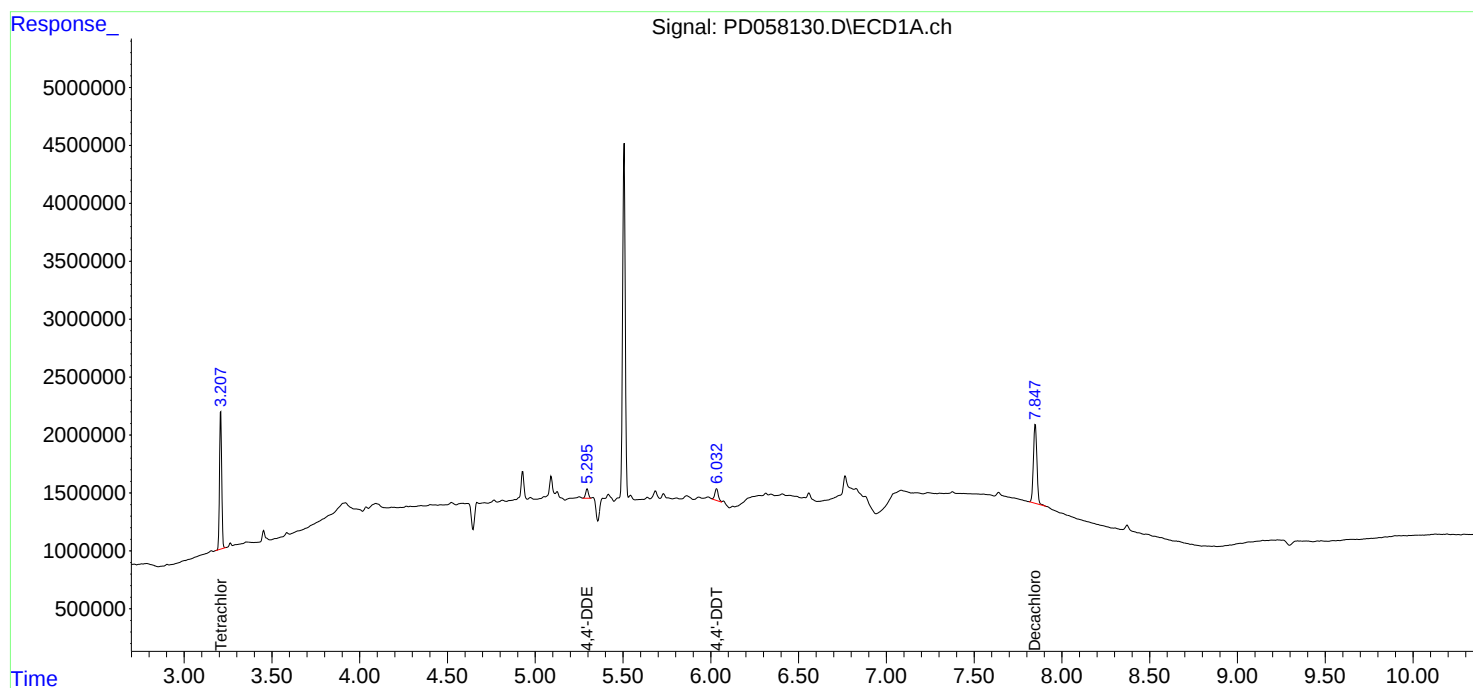

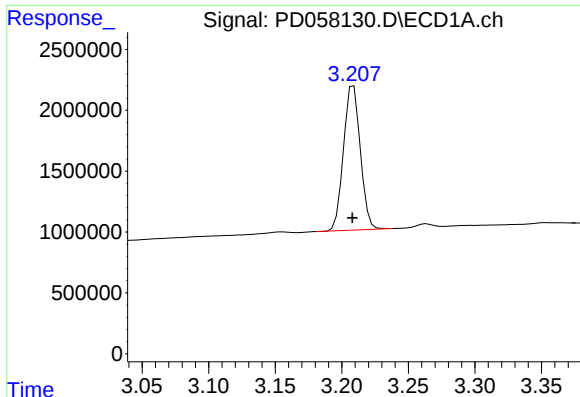


#1 Tetrachloro-m-xylene

R.T.: 3.209 min
Delta R.T.: 0.000 min
Response: 10418173
Conc: 13.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM65-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/29/2020 12:32:53 PM

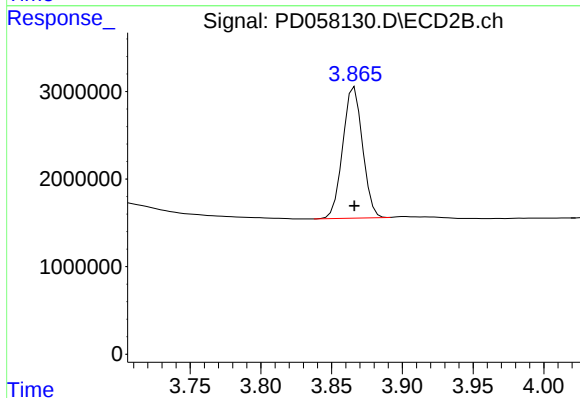


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 14563761
Conc: 12.79 ng/ml

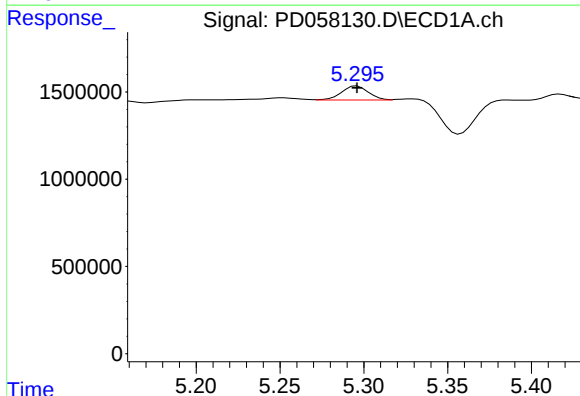


#12 4,4'-DDE

R.T.: 5.295 min
Delta R.T.: -0.001 min
Response: 891230
Conc: 0.96 ng/ml m

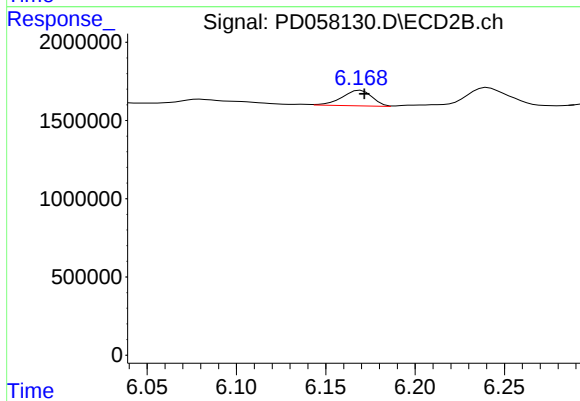

#12 4,4'-DDE

R.T.: 6.168 min
Delta R.T.: -0.003 min
Response: 1159737
Conc: 0.91 ng/ml m

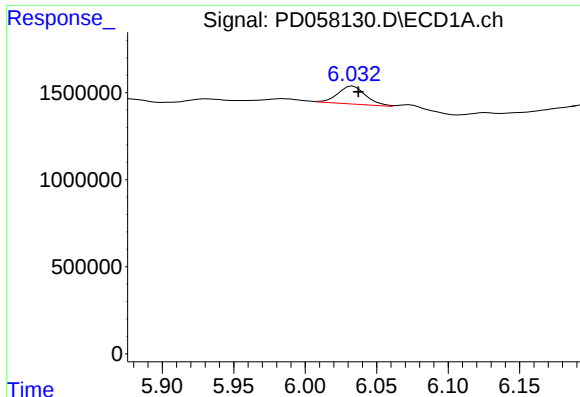


#17 4,4'-DDT

R.T.: 6.032 min
Delta R.T.: -0.005 min
Response: 1385653
Conc: 2.01 ng/ml m

Instrument :
ECD_D
ClientSampleId :
NM65-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/29/2020 12:32:53 PM

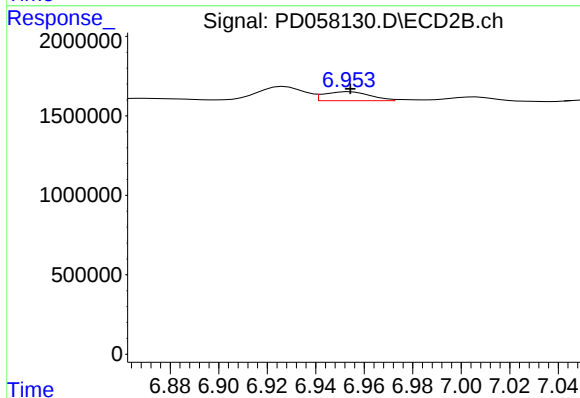


#17 4,4'-DDT

R.T.: 6.953 min
Delta R.T.: -0.002 min
Response: 731941
Conc: 0.74 ng/ml m

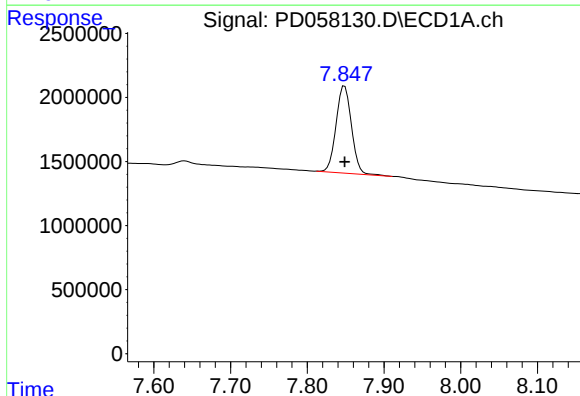

#28 Decachlorobiphenyl

R.T.: 7.849 min
Delta R.T.: 0.000 min
Response: 9463129
Conc: 11.84 ng/ml

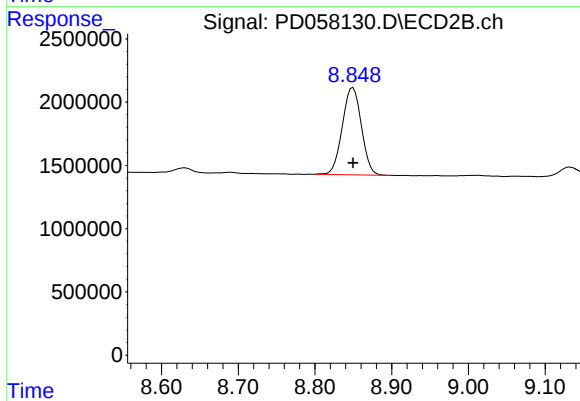

#28 Decachlorobiphenyl

R.T.: 8.849 min
Delta R.T.: 0.000 min
Response: 11975392
Conc: 11.55 ng/ml