

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052720\
 Data File : PD058134.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2020 11:10
 Operator : AJ\MA
 Sample : L2745-16
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 NM36-COMP-2020-0-6

Manual Integrations
 APPROVED

mohammad
 5/29/2020 12:33:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 12:52:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.866	6348235	8795524	8.123	7.723
28)	SA Decachlor...	7.849	8.850	5342936	6662554	6.682	6.427
Target Compounds							
12)	B 4,4'-DDE	5.294	6.170	342044	451164	0.367m	0.353m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052720\
Data File : PD058134.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2020 11:10
Operator : AJ\MA
Sample : L2745-16
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
NM36-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/29/2020 12:33:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 12:52:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

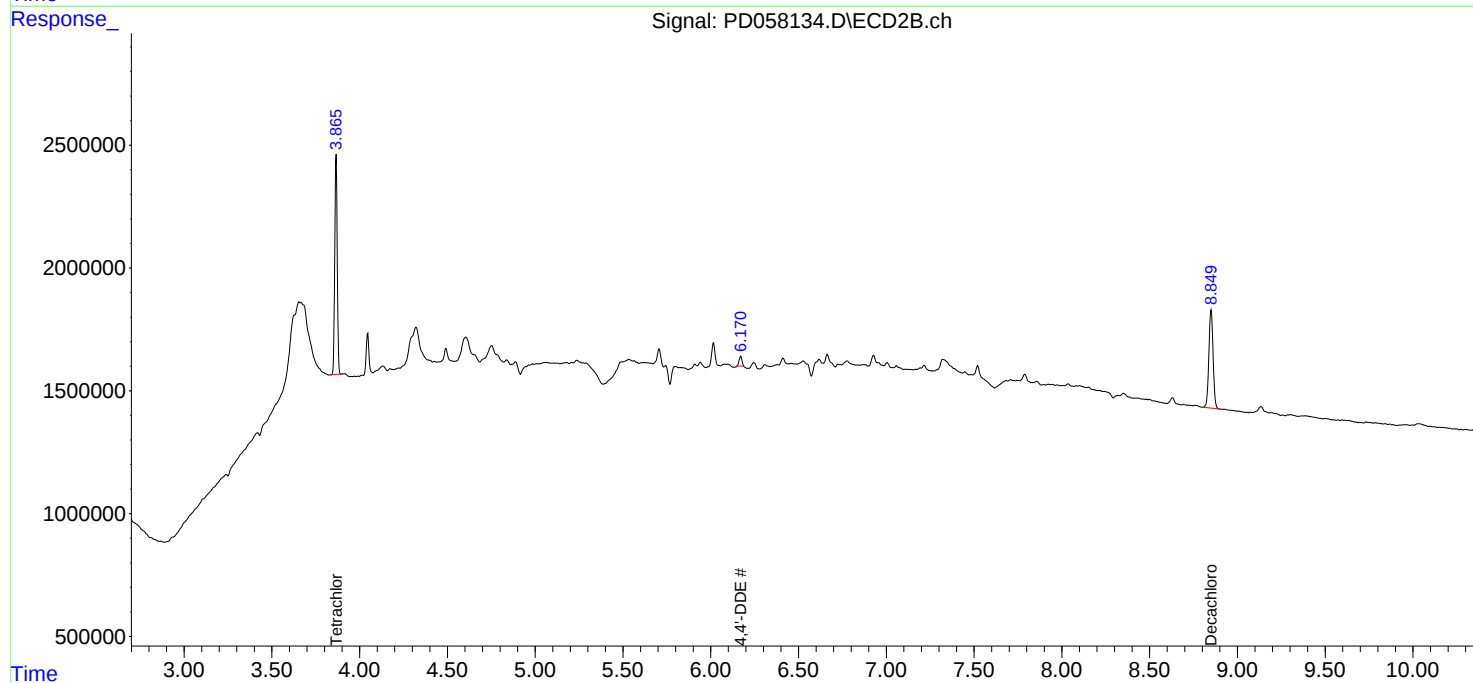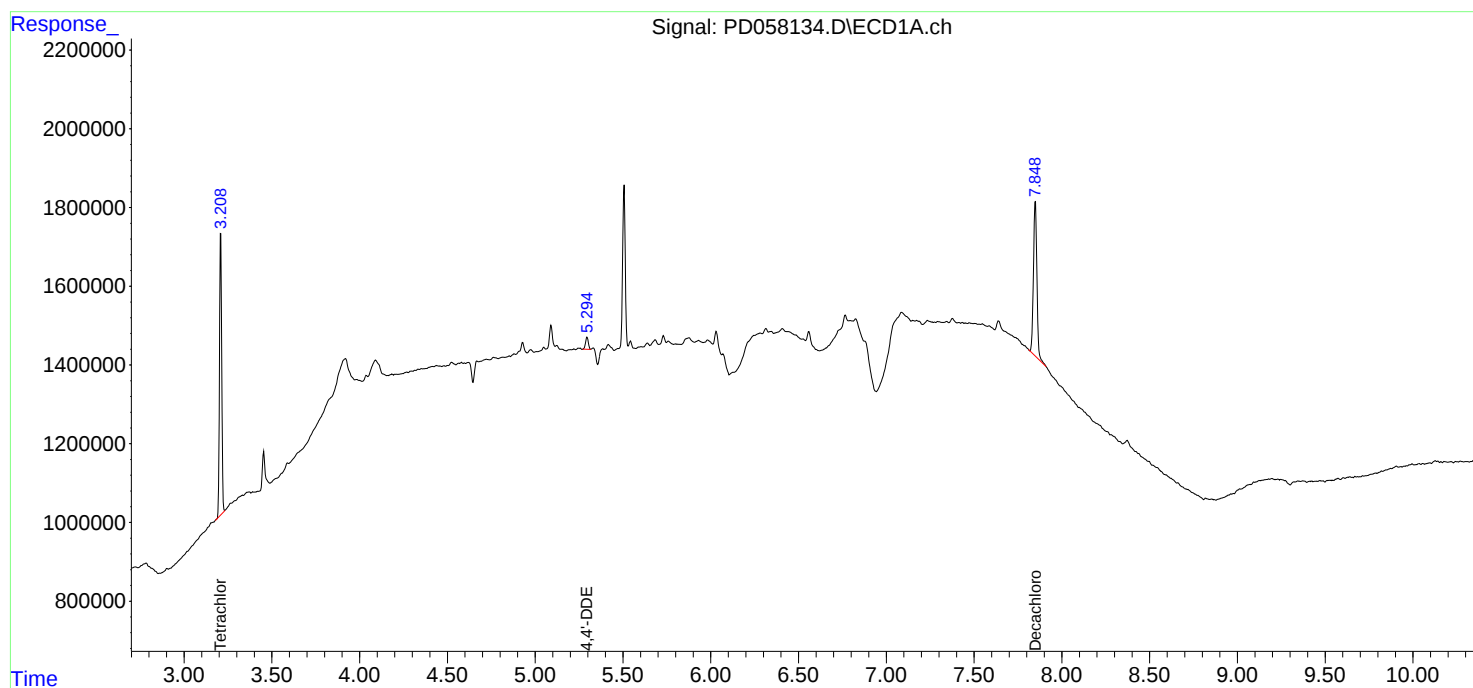

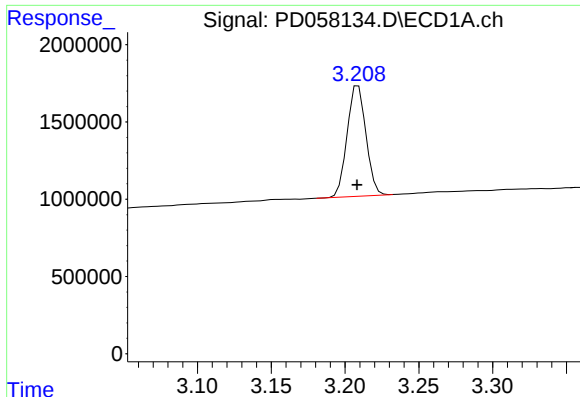


#1 Tetrachloro-m-xylene

R.T.: 3.209 min
Delta R.T.: 0.001 min
Response: 6348235
Conc: 8.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM36-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/29/2020 12:33:07 PM

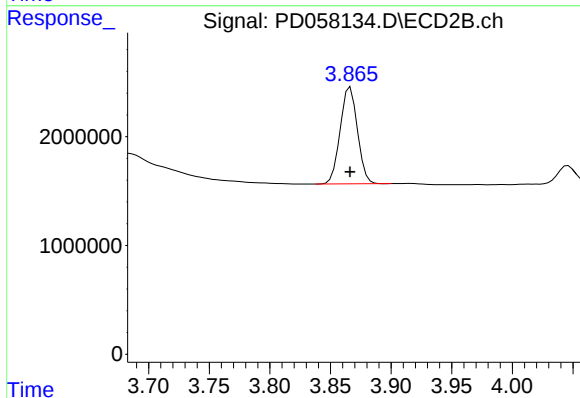


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 8795524
Conc: 7.72 ng/ml

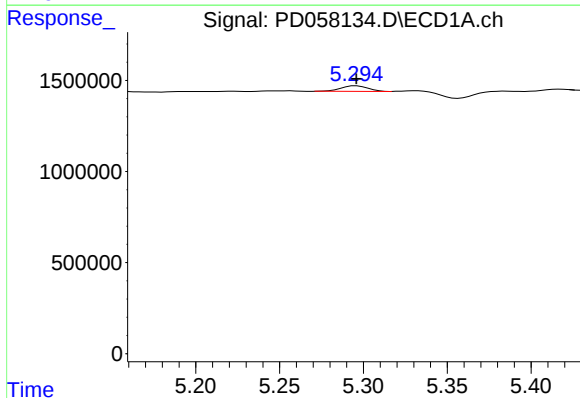


#12 4,4'-DDE

R.T.: 5.294 min
Delta R.T.: -0.002 min
Response: 342044
Conc: 0.37 ng/ml m

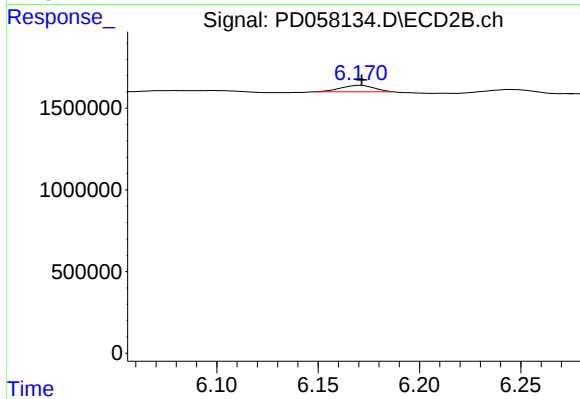

#12 4,4'-DDE

R.T.: 6.170 min
Delta R.T.: -0.002 min
Response: 451164
Conc: 0.35 ng/ml m

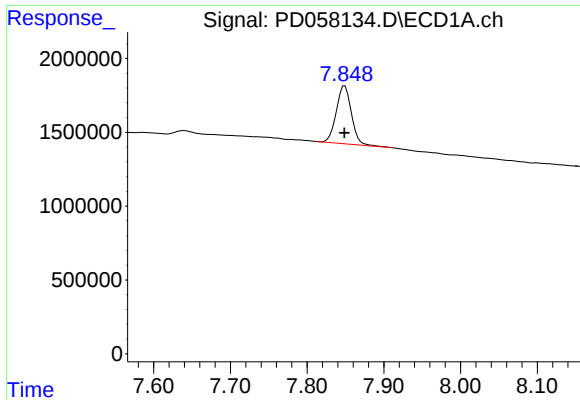


#28 Decachlorobiphenyl

R.T.: 7.849 min
Delta R.T.: 0.000 min
Response: 5342936
Conc: 6.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM36-COMP-2020-0-6

Manual Integrations
APPROVED

mohammad
5/29/2020 12:33:07 PM

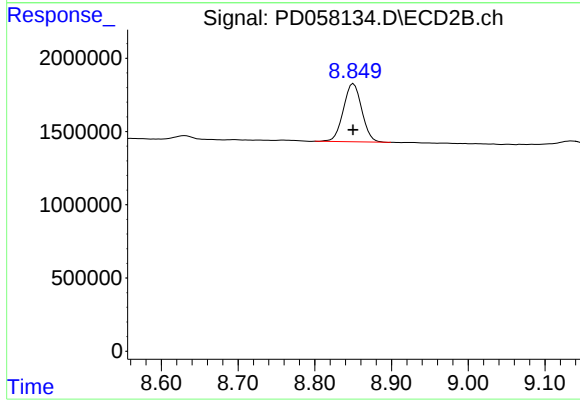

#28 Decachlorobiphenyl

R.T.: 8.850 min
Delta R.T.: 0.000 min
Response: 6662554
Conc: 6.43 ng/ml