

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052720\
 Data File : PD058163.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2020 19:06
 Operator : AJ\MA
 Sample : L2746-15
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 NM83-COMP-2020-0-6

Manual Integrations
 APPROVED

mohammad
 5/29/2020 12:34:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 02:23:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.209	3.867	9008248	12458327	11.526	10.939
28) SA Decachlor...	7.849	8.850	9135993	9766311	11.426	9.420
Target Compounds						
11) B alpha-Chl...	5.124	6.016	848804	4498721	0.858m	3.241 #
12) B 4,4'-DDE	5.297	6.171	3265718	3798357	3.506	2.974

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052720\
Data File : PD058163.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2020 19:06
Operator : AJ\MA
Sample : L2746-15
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
NM83-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/29/2020 12:34:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 02:23:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

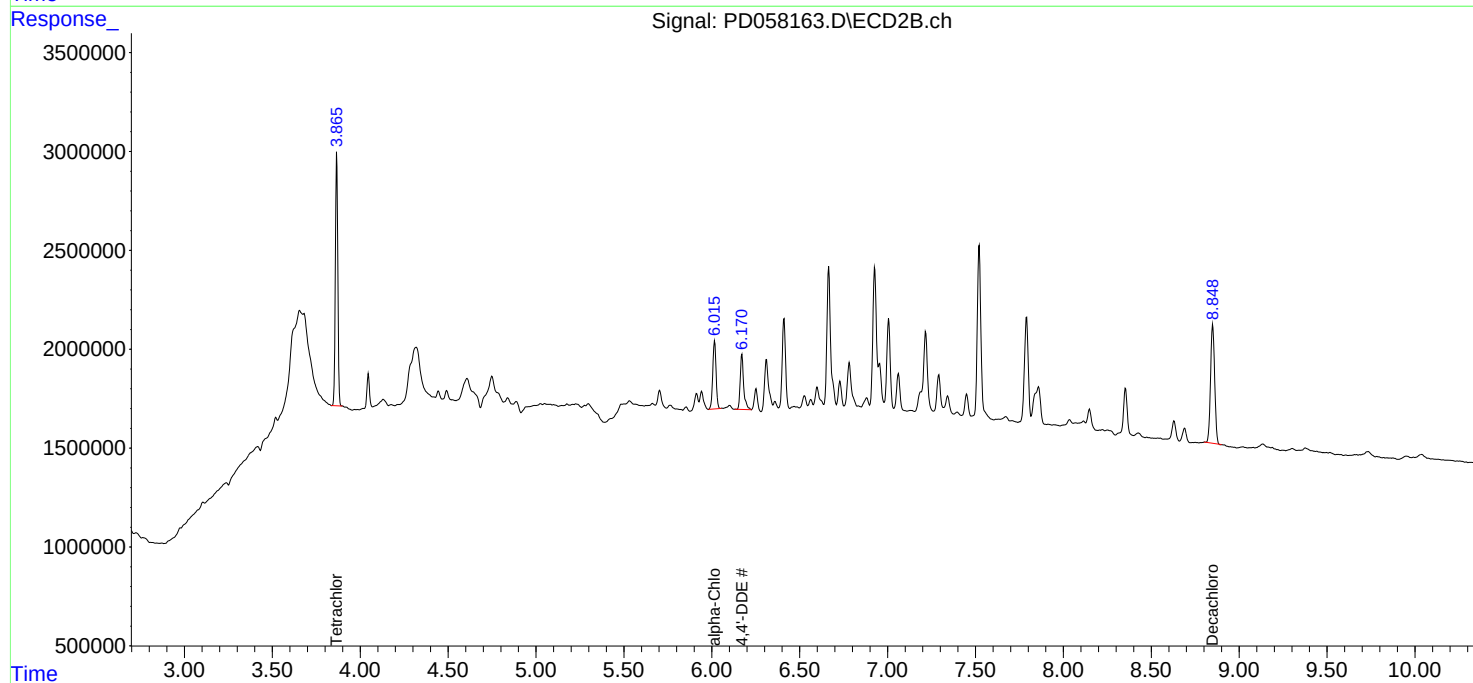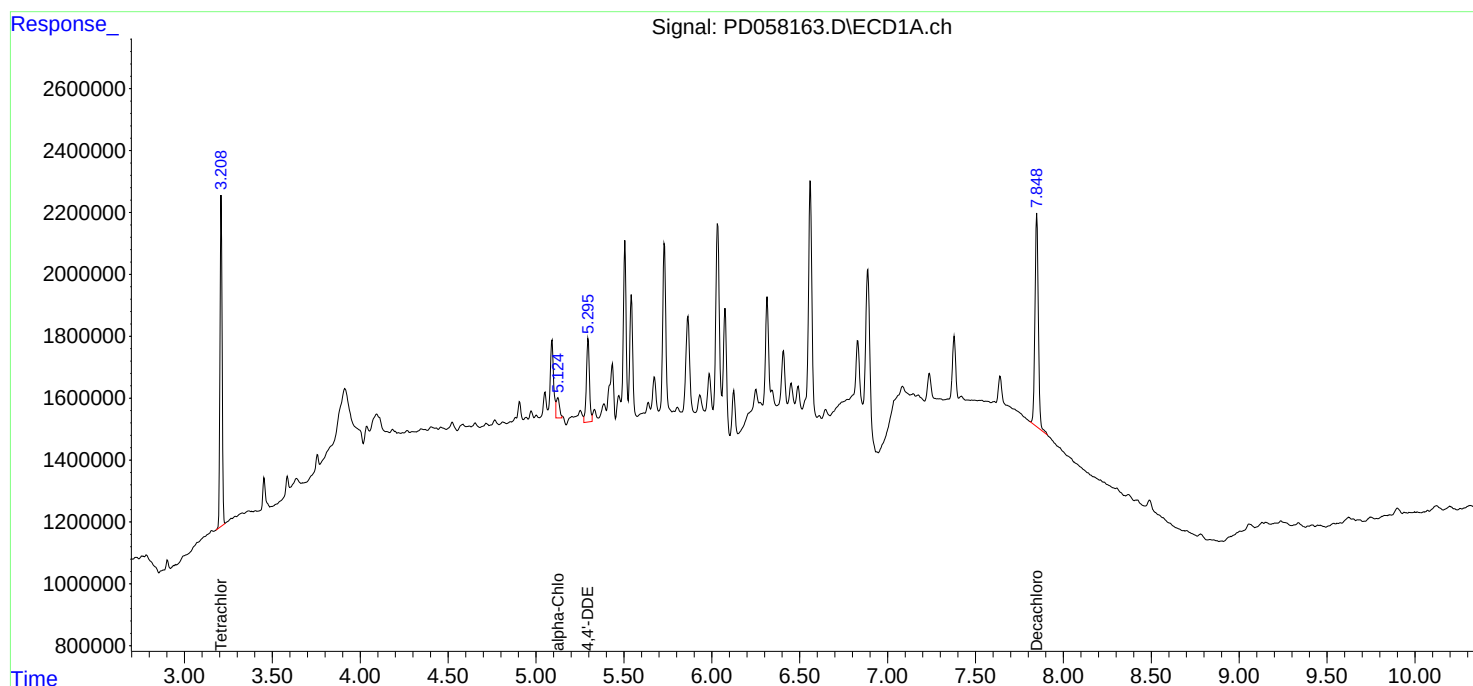

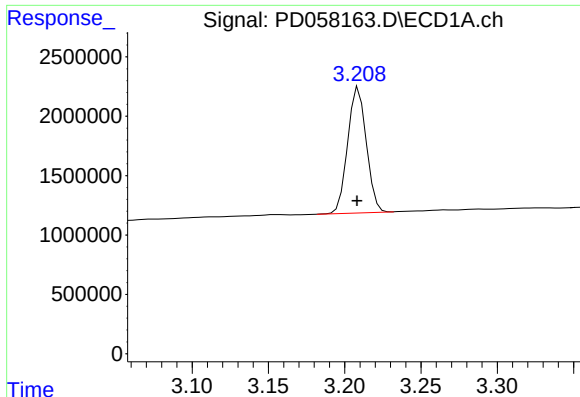


#1 Tetrachloro-m-xylene

R.T.: 3.209 min
Delta R.T.: 0.001 min
Response: 9008248
Conc: 11.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM83-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/29/2020 12:34:00 PM

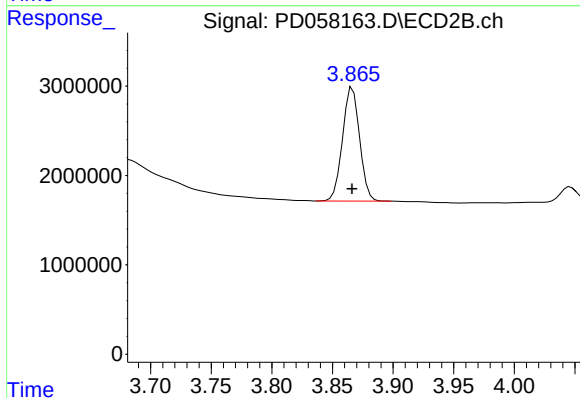


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 12458327
Conc: 10.94 ng/ml

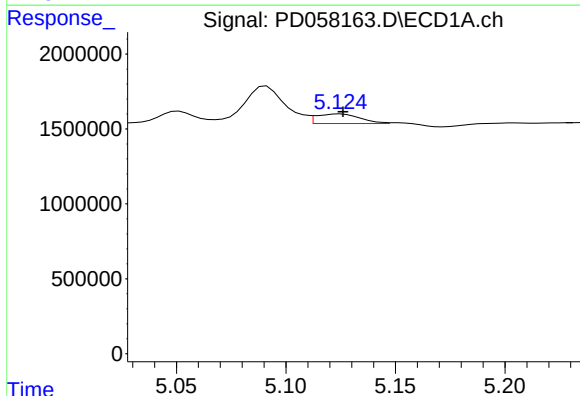


#11 alpha-Chlordane

R.T.: 5.124 min
Delta R.T.: -0.003 min
Response: 848804
Conc: 0.86 ng/ml m

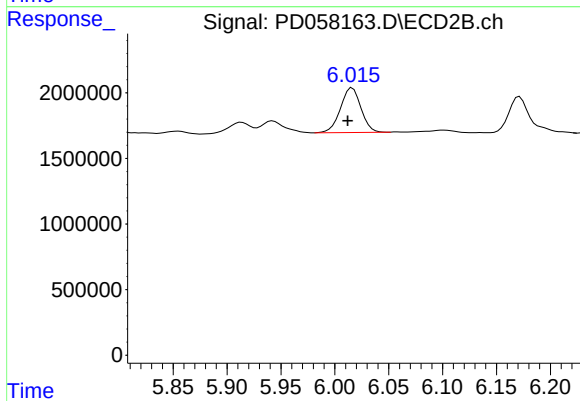

#11 alpha-Chlordane

R.T.: 6.016 min
Delta R.T.: 0.004 min
Response: 4498721
Conc: 3.24 ng/ml

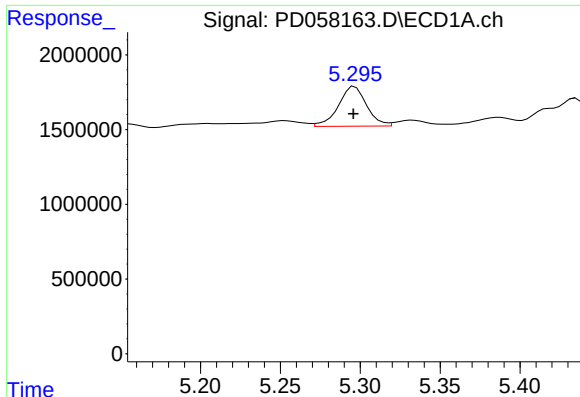


#12 4,4'-DDE

R.T.: 5.297 min
Delta R.T.: 0.000 min
Response: 3265718
Conc: 3.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM83-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/29/2020 12:34:00 PM

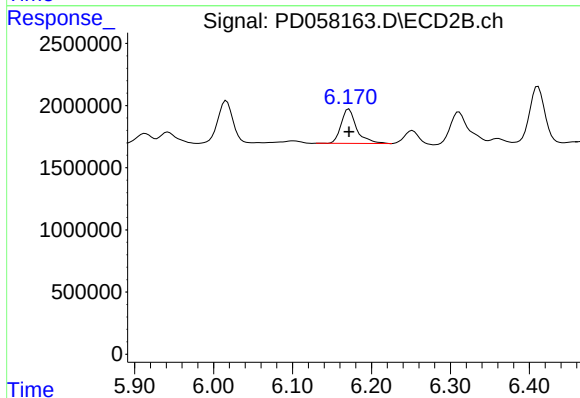


#12 4,4'-DDE

R.T.: 6.171 min
Delta R.T.: 0.000 min
Response: 3798357
Conc: 2.97 ng/ml

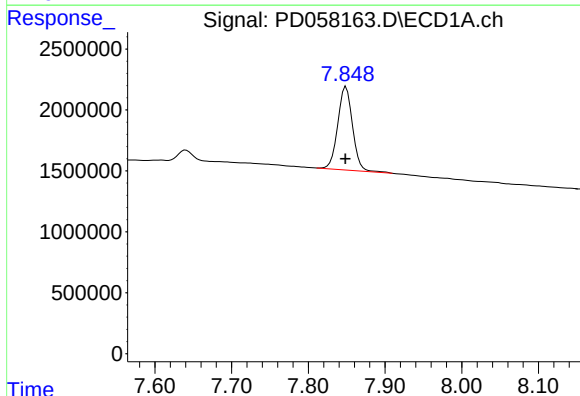

#28 Decachlorobiphenyl

R.T.: 7.849 min
Delta R.T.: 0.000 min
Response: 9135993
Conc: 11.43 ng/ml

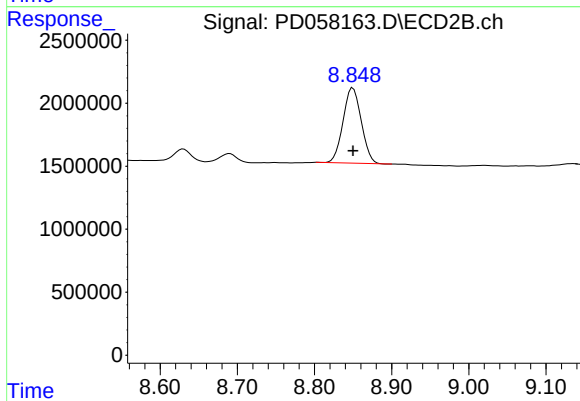

#28 Decachlorobiphenyl

R.T.: 8.850 min
Delta R.T.: 0.000 min
Response: 9766311
Conc: 9.42 ng/ml