

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052721\
 Data File : PD063302.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2021 08:43
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 17:03:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Mon May 24 14:48:18 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	8.207	0.000	6133352	0	4.873	N.D. #
Target Compounds							
7)	B delta-BHC	0.000	5.026	0	51147332	N.D.	3.661 #
8)	B Heptachlo...	0.000	5.851	0	17480433	N.D.	1.143 #
9)	A Endosulfan I	0.000	6.187	0	3295591	N.D.	0.232 #
10)	B gamma-Chl...	0.000	6.083	0	1299513	N.D.	0.083 #
12)	B 4,4'-DDE	0.000	6.301	0	952215	N.D.	0.063 #
13)	MA Dieldrin	0.000	6.453	0	1093634	N.D.	0.072 #
14)	MA Endrin	5.996	6.666	1070950	9826247	0.801	0.770
17)	MA 4,4'-DDT	0.000	7.098	0	940401	N.D.	0.083 #
19)	B Endosulfa...	0.000	7.226	0	325493	N.D.	0.027 #
21)	B Endrin ke...	0.000	7.697	0	923361	N.D.	0.077 #
25)	Chlordane-3	0.000	6.083	0	1299513	N.D.	0.550 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052721\
Data File : PD063302.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2021 08:43
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 17:03:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Mon May 24 14:48:18 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

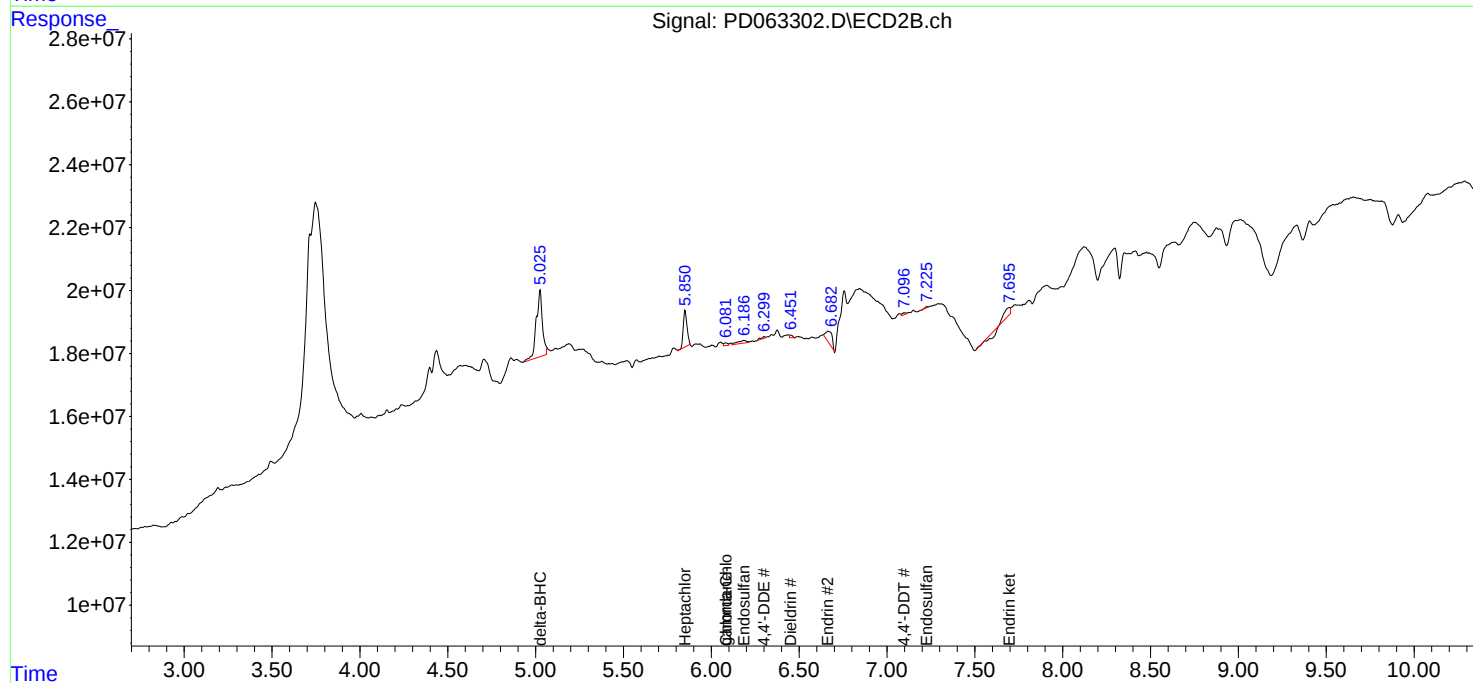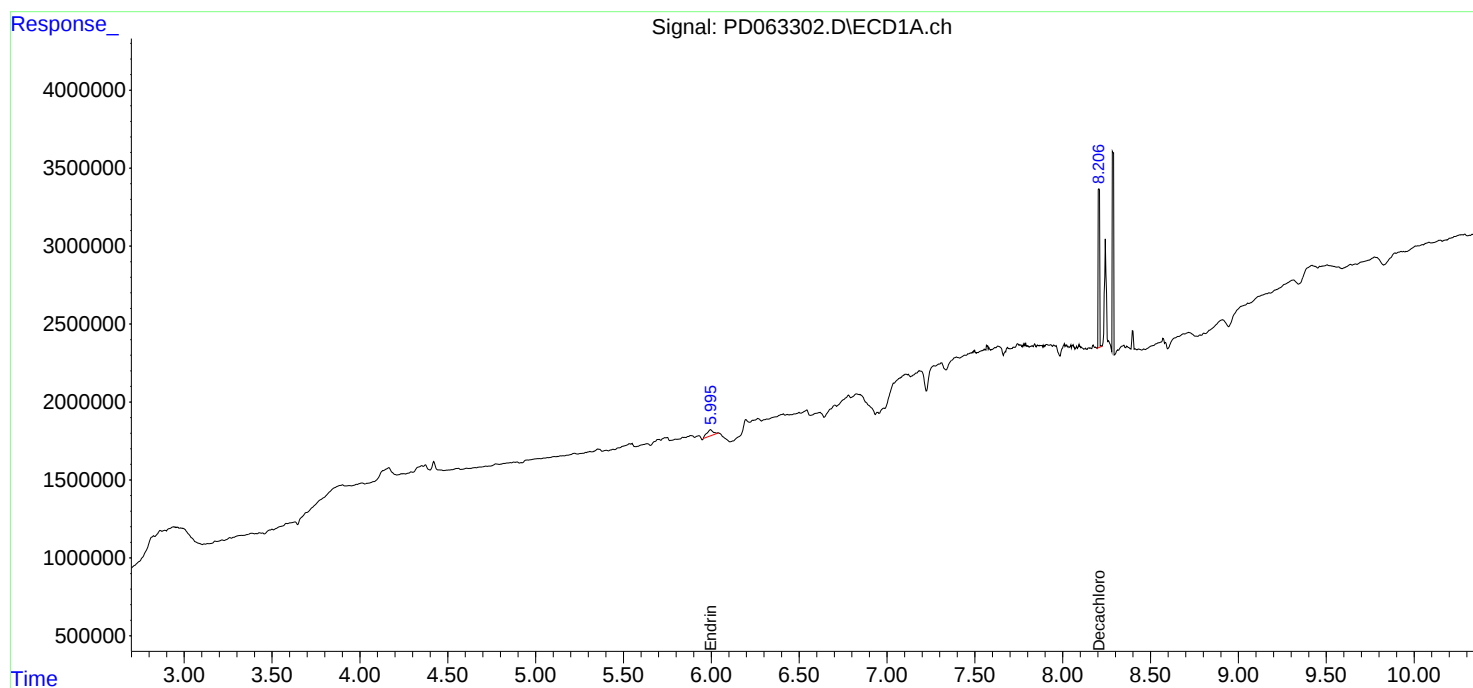


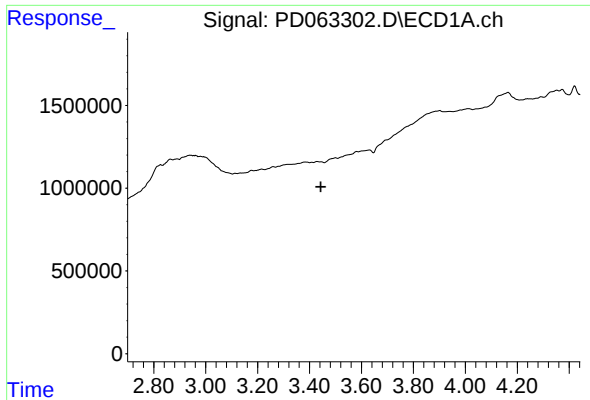

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.443 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

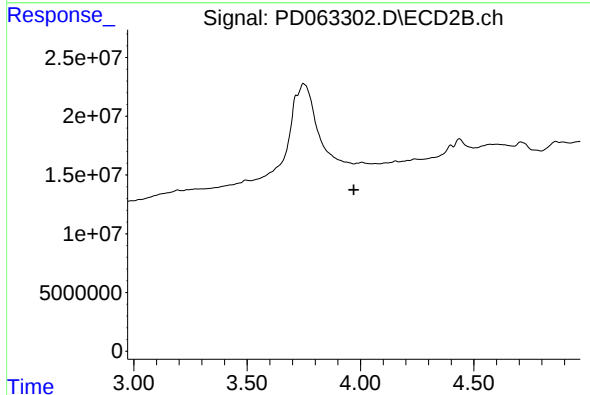


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.970 min
Response: 0
Conc: N.D.

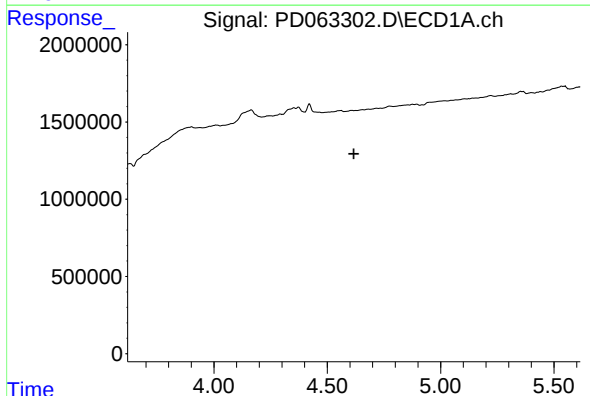


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.617 min
Response: 0
Conc: N.D.

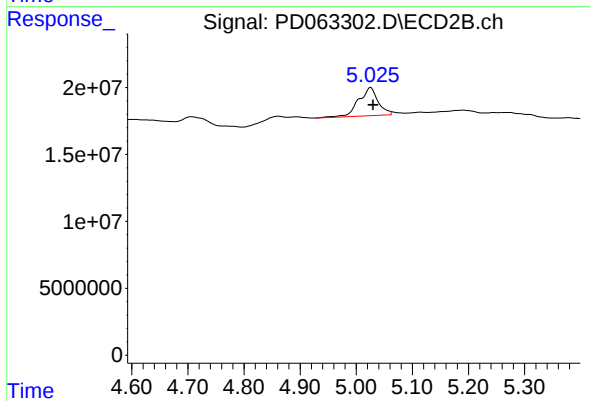

#7 delta-BHC


R.T.: 5.026 min
Delta R.T.: -0.004 min
Response: 51147332
Conc: 3.66 ng/ml

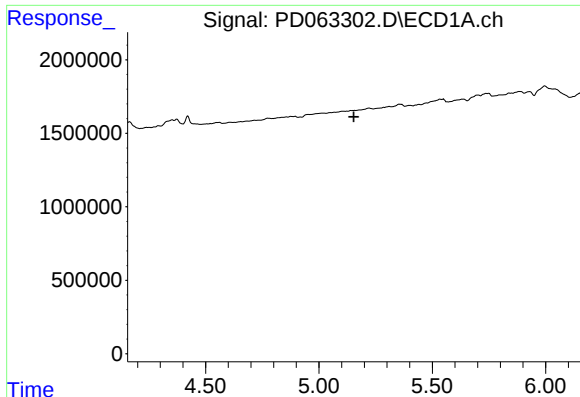

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.154 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

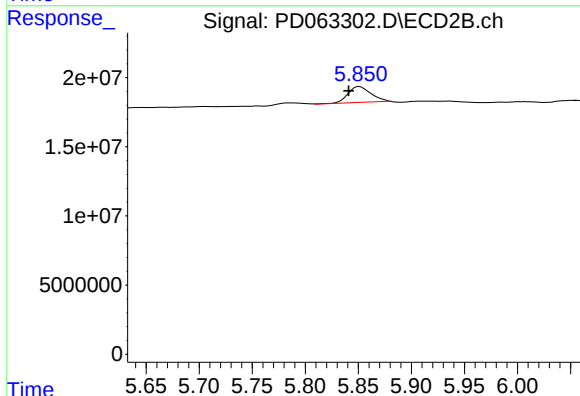


#8 Heptachlor epoxide

R.T.: 5.851 min
Delta R.T.: 0.010 min
Response: 17480433
Conc: 1.14 ng/ml

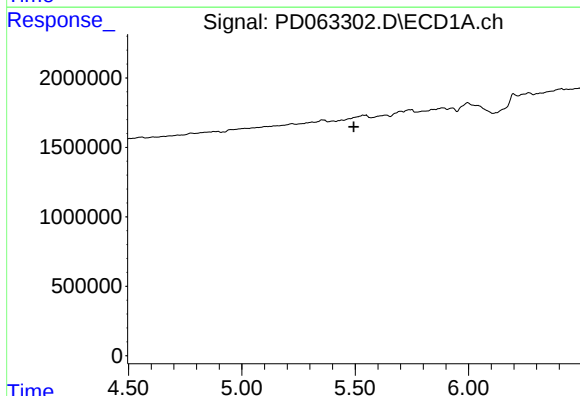


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.493 min
Response: 0
Conc: N.D.

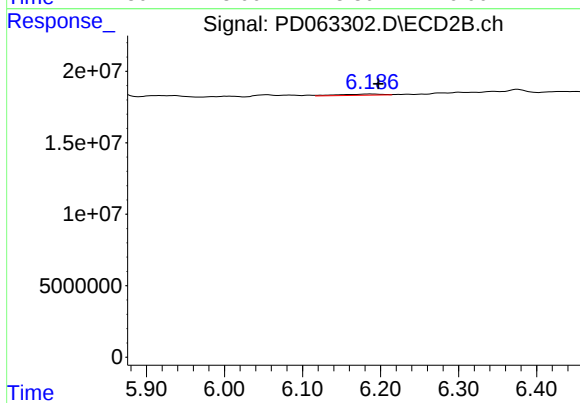

#9 Endosulfan I


R.T.: 6.187 min
Delta R.T.: -0.011 min
Response: 3295591
Conc: 0.23 ng/ml

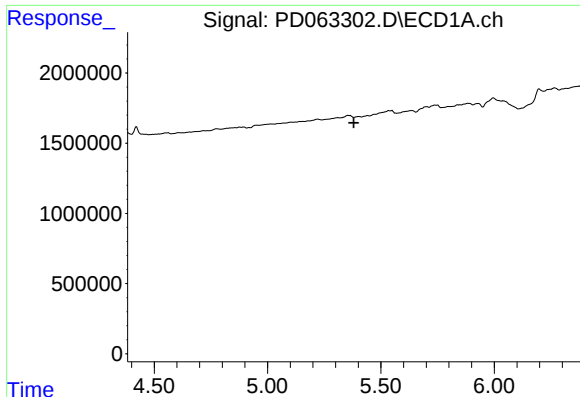

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.381 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

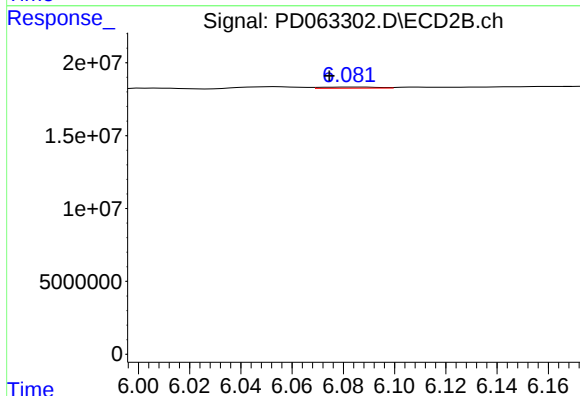


#10 gamma-Chlordane

R.T.: 6.083 min
Delta R.T.: 0.008 min
Response: 1299513
Conc: 0.08 ng/ml

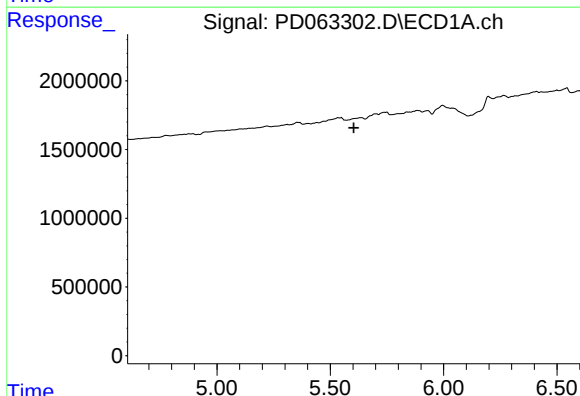


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.604 min
Response: 0
Conc: N.D.

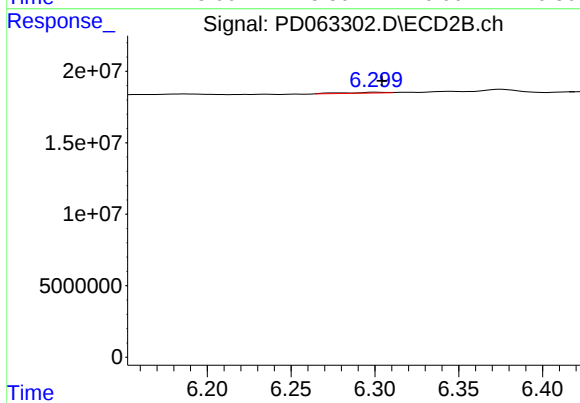

#12 4,4'-DDE


R.T.: 6.301 min
Delta R.T.: -0.003 min
Response: 952215
Conc: 0.06 ng/ml

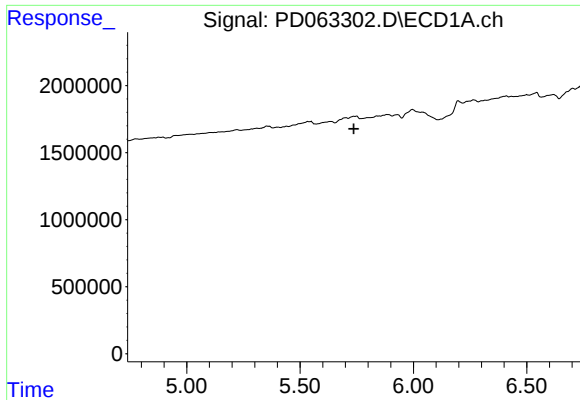

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.737 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

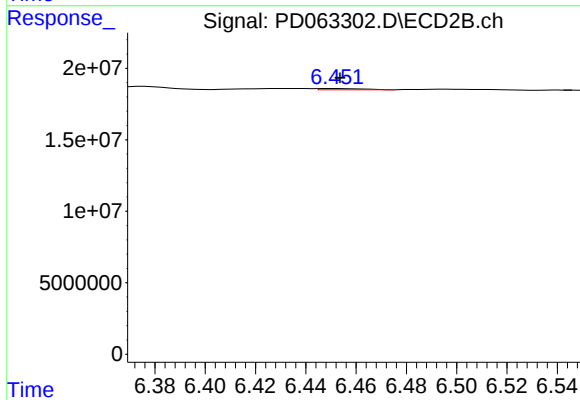


#13 Dieldrin

R.T.: 6.453 min
Delta R.T.: 0.000 min
Response: 1093634
Conc: 0.07 ng/ml

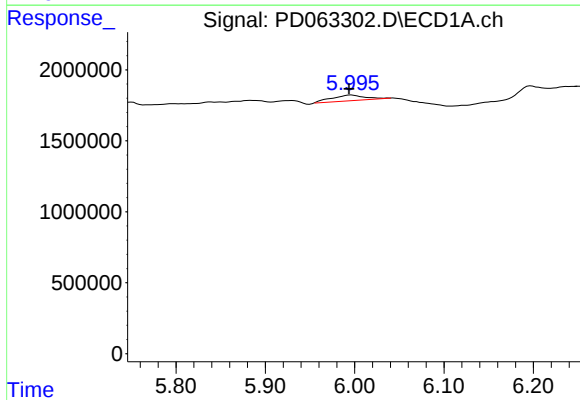


#14 Endrin

R.T.: 5.996 min
Delta R.T.: 0.002 min
Response: 1070950
Conc: 0.80 ng/ml

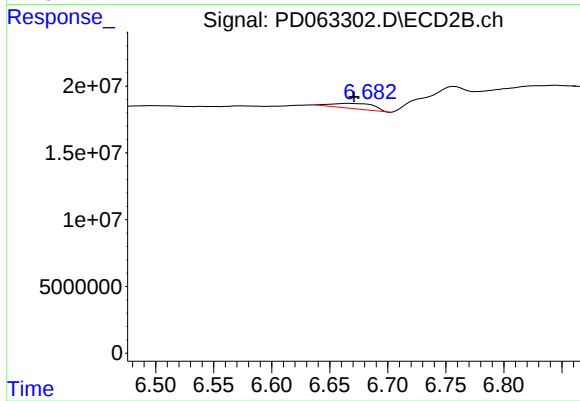

#14 Endrin


R.T.: 6.666 min
Delta R.T.: -0.005 min
Response: 9826247
Conc: 0.77 ng/ml

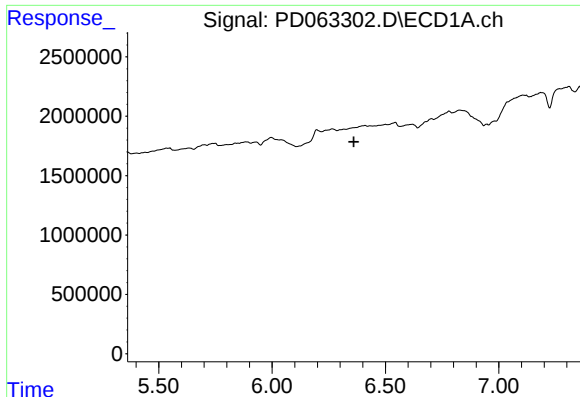

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.361 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

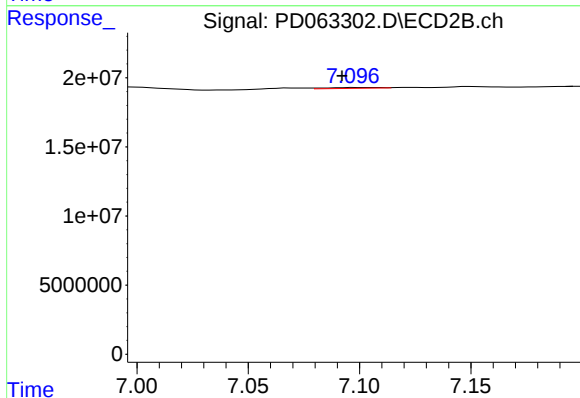


#17 4,4'-DDT

R.T.: 7.098 min
Delta R.T.: 0.005 min
Response: 940401
Conc: 0.08 ng/ml

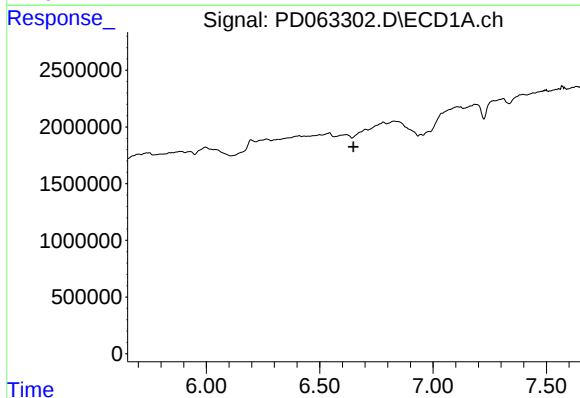


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.649 min
Response: 0
Conc: N.D.

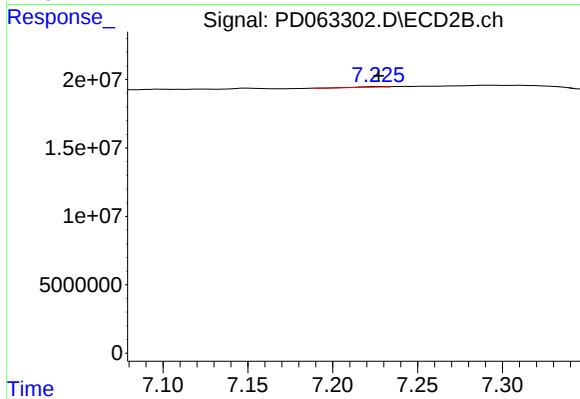

#19 Endosulfan Sulfate


R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 325493
Conc: 0.03 ng/ml

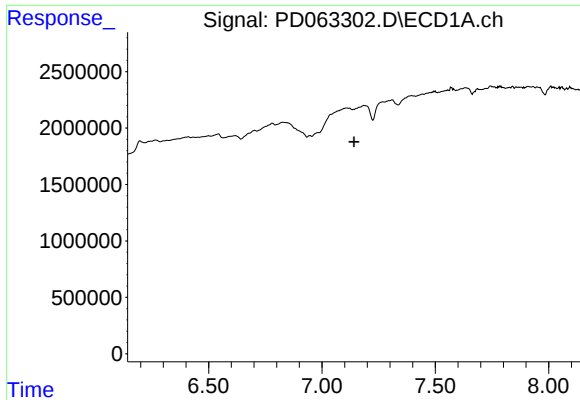

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

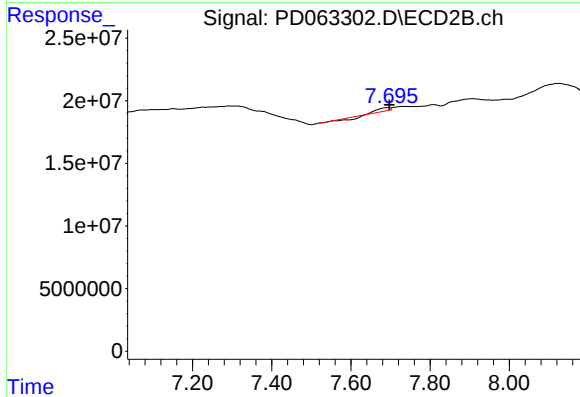


#21 Endrin ketone

R.T.: 7.697 min
Delta R.T.: 0.000 min
Response: 923361
Conc: 0.08 ng/ml

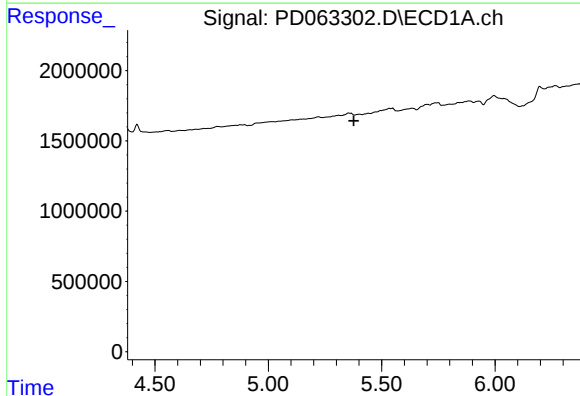


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.377 min
Response: 0
Conc: N.D.

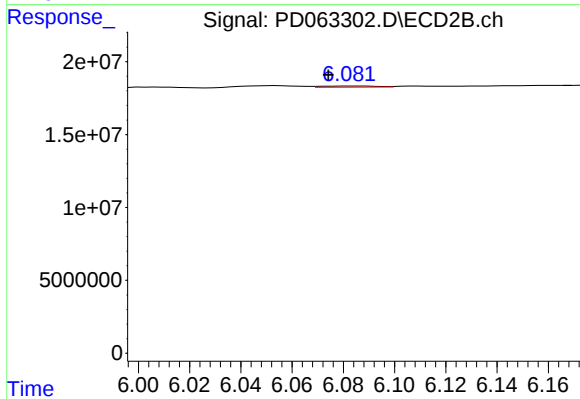

#25 Chlordane-3


R.T.: 6.083 min
Delta R.T.: 0.009 min
Response: 1299513
Conc: 0.55 ng/ml

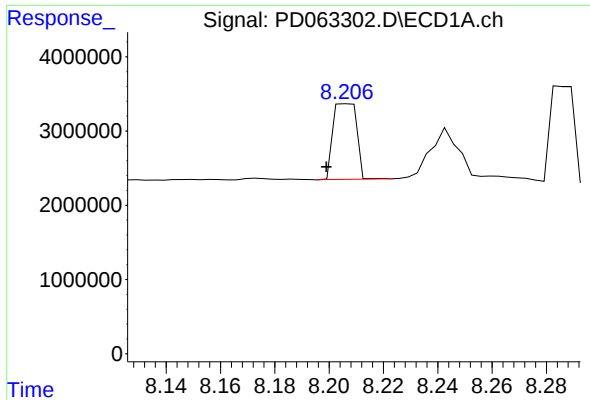

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.008 min
Response: 6133352
Conc: 4.87 ng/ml

Instrument :
ECD_D
ClientSampleId :

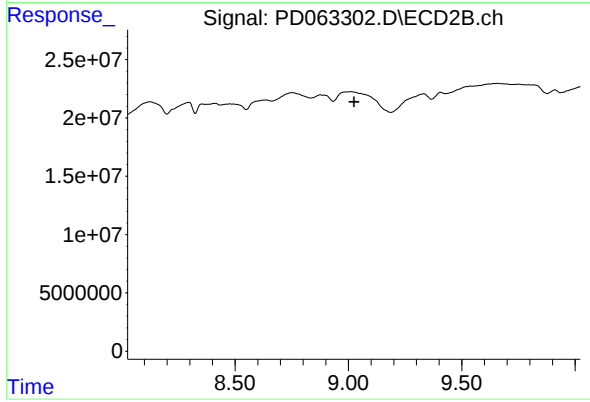

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.025 min
Response: 0
Conc: N.D.