

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052721\
 Data File : PD063316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2021 17:18
 Operator : AR\AJ
 Sample : M2539-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 FK-PS-01-073

Manual Integrations
 APPROVED

Ankita
 5/28/2021 8:59:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 17:59:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Mon May 24 14:48:18 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.971	15995760	181.0E6	14.522	15.618
28)	SA Decachlor...	8.197	9.027	16640583	154.0E6	13.222	15.099
Target Compounds							
10)	B gamma-Chl...	5.378	6.074	475267	10815244	0.324m	0.694m#
11)	B alpha-Chl...	5.435	6.148	887760	24857781	0.615m	1.677m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052721\
Data File : PD063316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2021 17:18
Operator : AR\AJ
Sample : M2539-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleID :
FK-PS-01-073


Manual Integrations
APPROVED

Ankita
5/28/2021 8:59:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 17:59:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Mon May 24 14:48:18 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

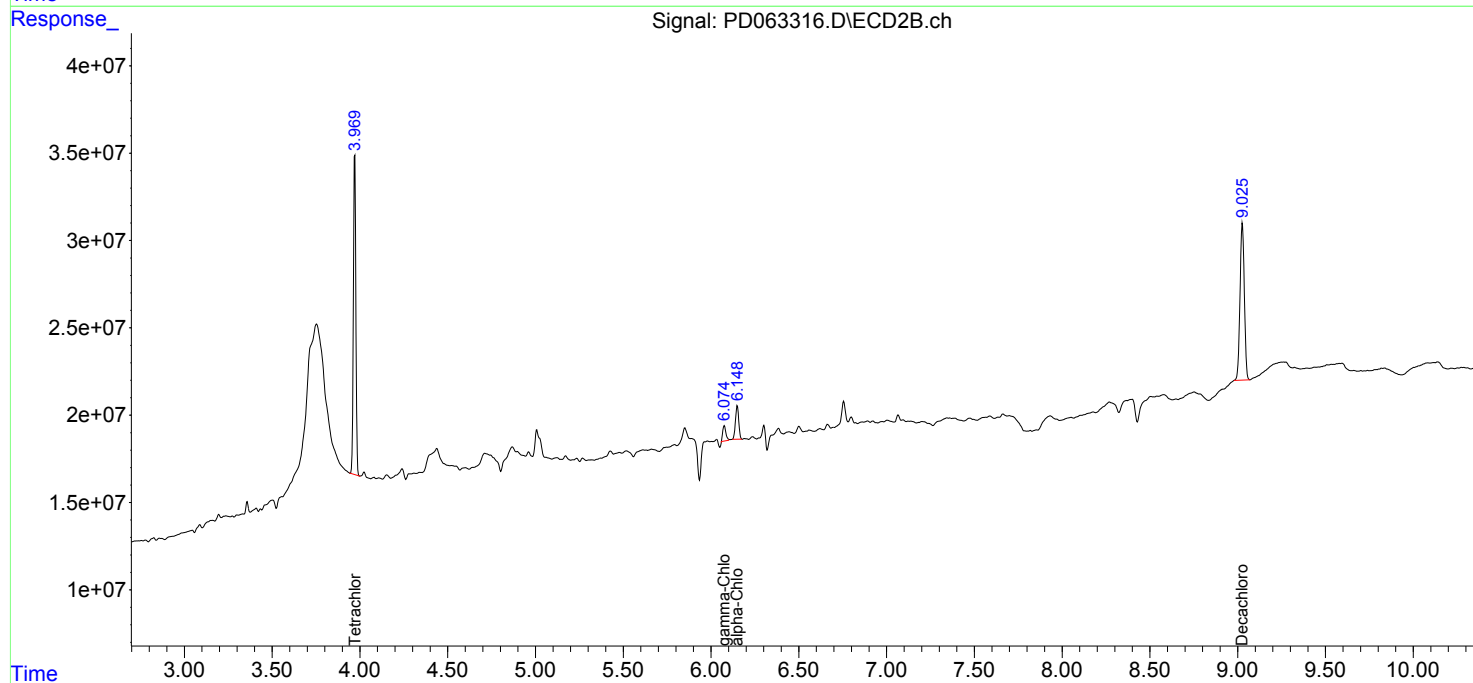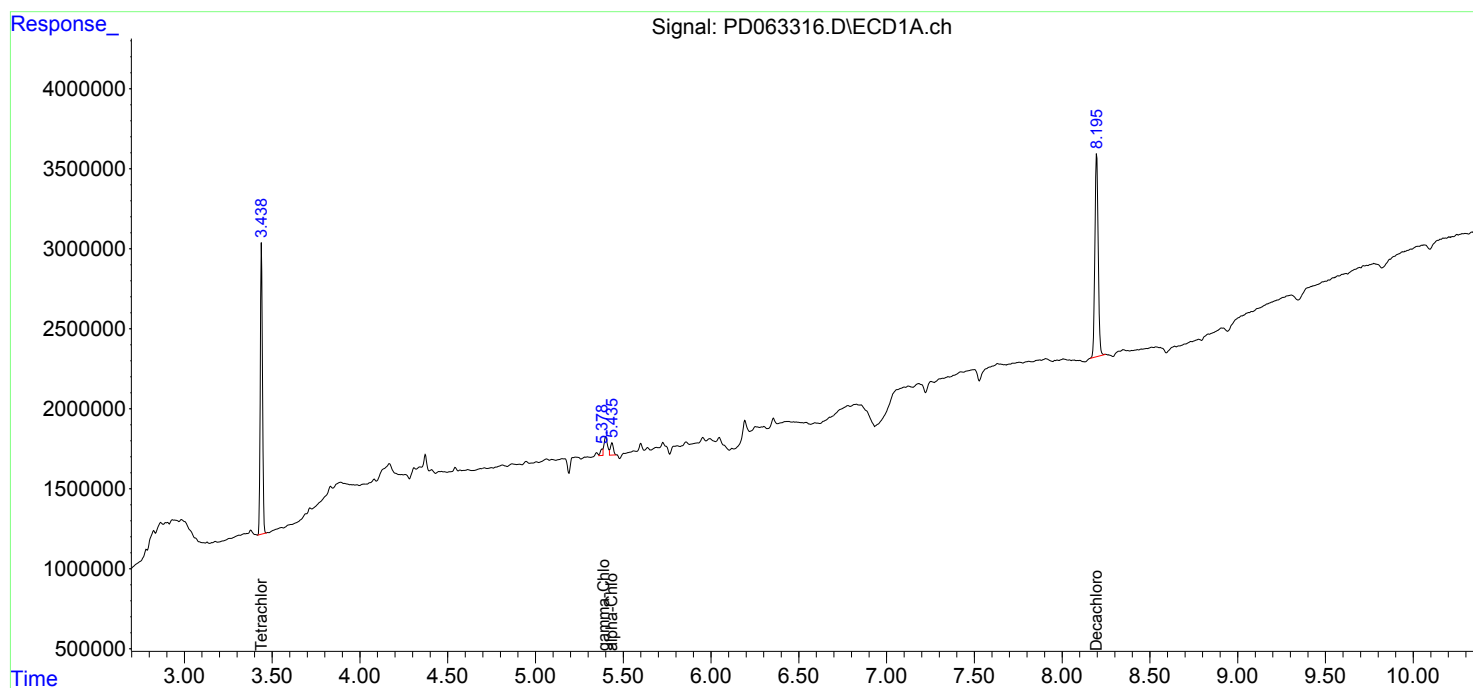

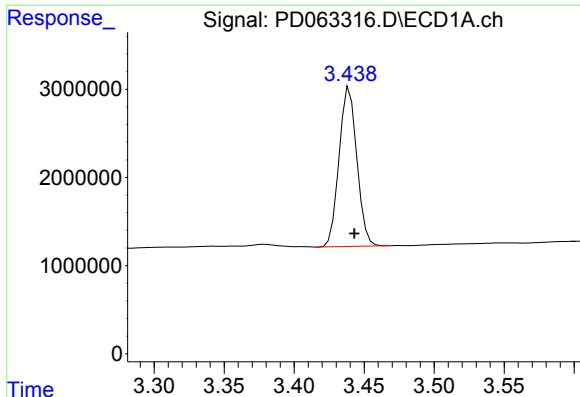


#1 Tetrachloro-m-xylene

R.T.: 3.440 min
Delta R.T.: -0.003 min
Response: 15995760
Conc: 14.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
FK-PS-01-073


Manual Integrations
APPROVED

Ankita
5/28/2021 8:59:51 AM

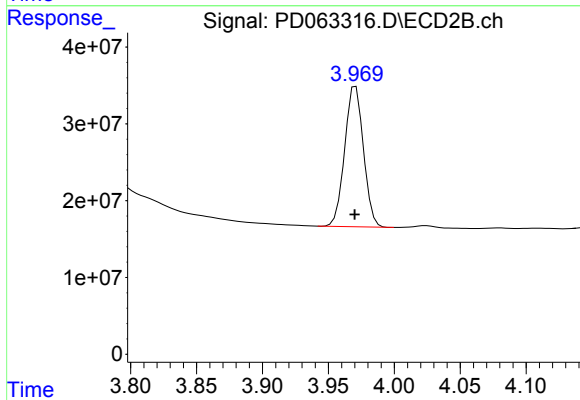


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 180978660
Conc: 15.62 ng/ml

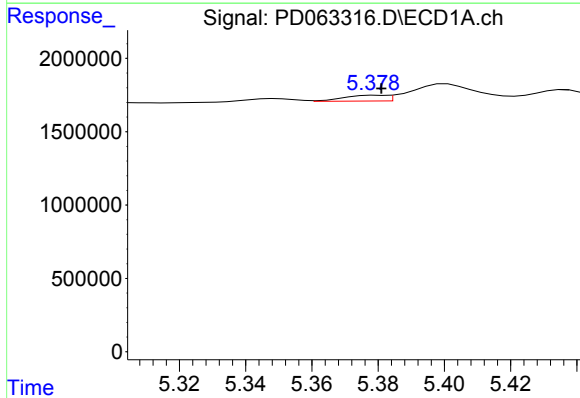


#10 gamma-Chlordane

R.T.: 5.378 min
Delta R.T.: -0.003 min
Response: 475267
Conc: 0.32 ng/ml m

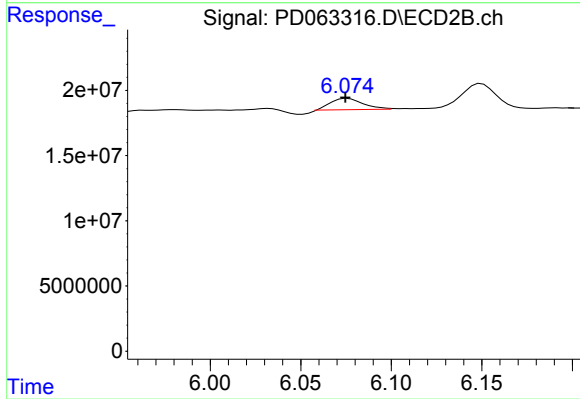

#10 gamma-Chlordane

R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 10815244
Conc: 0.69 ng/ml m

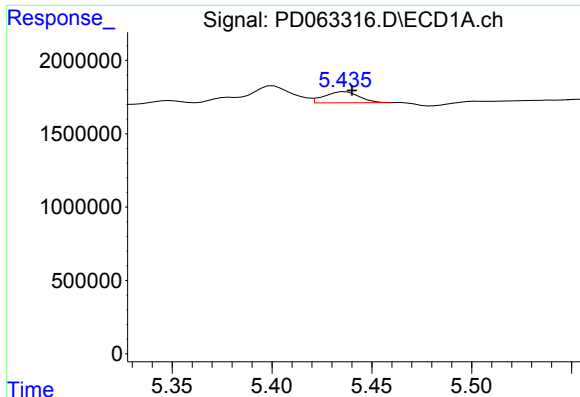


#11 alpha-Chlordane

R.T.: 5.435 min
Delta R.T.: -0.005 min
Response: 887760
Conc: 0.61 ng/ml m

Instrument :
ECD_D
ClientSampleId :
FK-PS-01-073


Manual Integrations
APPROVED

Ankita
5/28/2021 8:59:51 AM

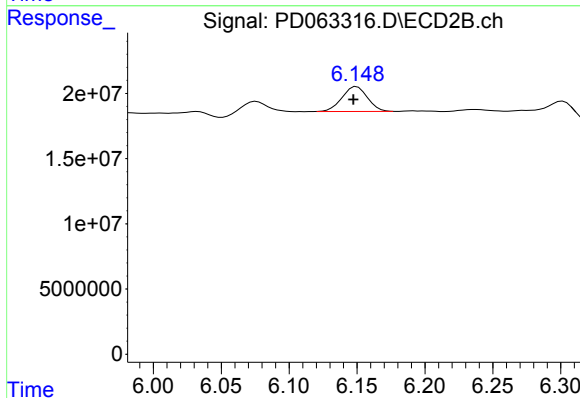


#11 alpha-Chlordane

R.T.: 6.148 min
Delta R.T.: 0.001 min
Response: 24857781
Conc: 1.68 ng/ml m

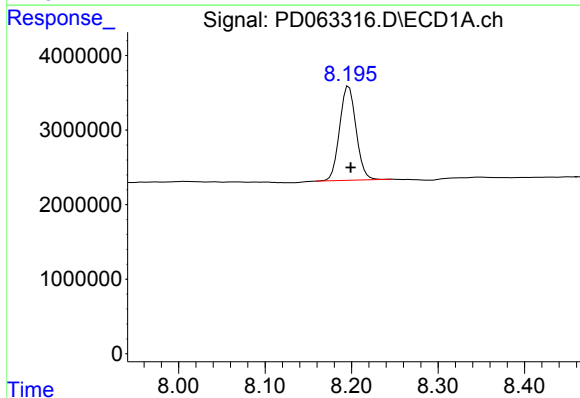

#28 Decachlorobiphenyl

R.T.: 8.197 min
Delta R.T.: -0.002 min
Response: 16640583
Conc: 13.22 ng/ml

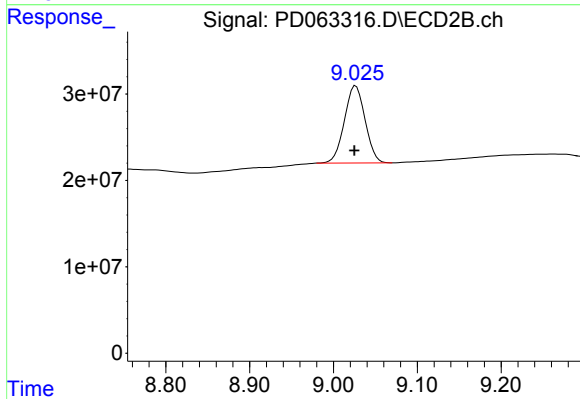

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: 0.002 min
Response: 154037106
Conc: 15.10 ng/ml