

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052722\
 Data File : PD069878.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2022 14:31
 Operator : AR\AJ
 Sample : N2883-11MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4K8MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/27/2022
 Supervised By :Ankita Jodhani 05/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 03:26:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050722CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed May 18 23:46:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	4.168	20504083	239.7E6	16.867	18.904
27)	SA Decachlor...	8.193	9.361	39088293	222.0E6	31.514	30.396
Target Compounds							
2)	A alpha-BHC	3.881	4.565	69020517	619.2E6	40.463	33.905
3)	MA gamma-BHC...	4.164	4.856	68820969	613.5E6	41.101	37.682
4)	MA Heptachlor	4.461	5.382	71379999	629.5E6	44.120	39.781
5)	MB Aldrin	4.708	5.695	71195468	616.9E6	48.518	42.983
6)	B beta-BHC	4.414	5.018	31889512	355.4E6	44.705	52.154m
7)	B delta-BHC	4.618	5.246	10511073	35375714	6.964	3.122 #
8)	B Heptachlo...	5.152	6.083	66310676	414.1E6	47.743	38.402
9)	A Endosulfan I	5.490	6.445	60457359	487.8E6	43.958	38.604
10)	B trans-Chl...	5.376	6.319	67278998	526.0E6	47.349m	40.058
11)	B cis-Chlor...	5.435	6.394	64954430	519.2E6	46.625m	40.735
12)	B 4,4'-DDE	5.602	6.544	134.2E6	1012.2E6	103.054	87.611
13)	MA Dieldrin	5.734	6.703	139.8E6	1032.9E6	94.248	81.137
14)	MA Endrin	5.991	6.924	123.3E6	814.7E6	94.706	80.557
15)	B Endosulfa...	6.266	7.129	110.8E6	856.4E6	94.994	89.499
16)	A 4,4'-DDD	6.119	7.035	105.9E6	813.8E6	90.370	82.230
17)	MA 4,4'-DDT	6.359	7.338	105.9E6	760.0E6	90.559	79.440
18)	B Endrin al...	6.435	7.253	92854462	638.3E6	89.316	77.289
19)	B Endosulfa...	6.647	7.478	82930503	573.7E6	67.672	61.328
20)	A Methoxychlor	6.908	7.791	288.1E6	1767.9E6	438.579	401.045
21)	B Endrin ke...	7.140	7.952	133.3E6	816.0E6	97.866	85.317

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052722\
Data File : PD069878.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2022 14:31
Operator : AR\AJ
Sample : N2883-11MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 03:26:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050722CLP.M
Quant Title : GC Extractables
QLast Update : Wed May 18 23:46:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

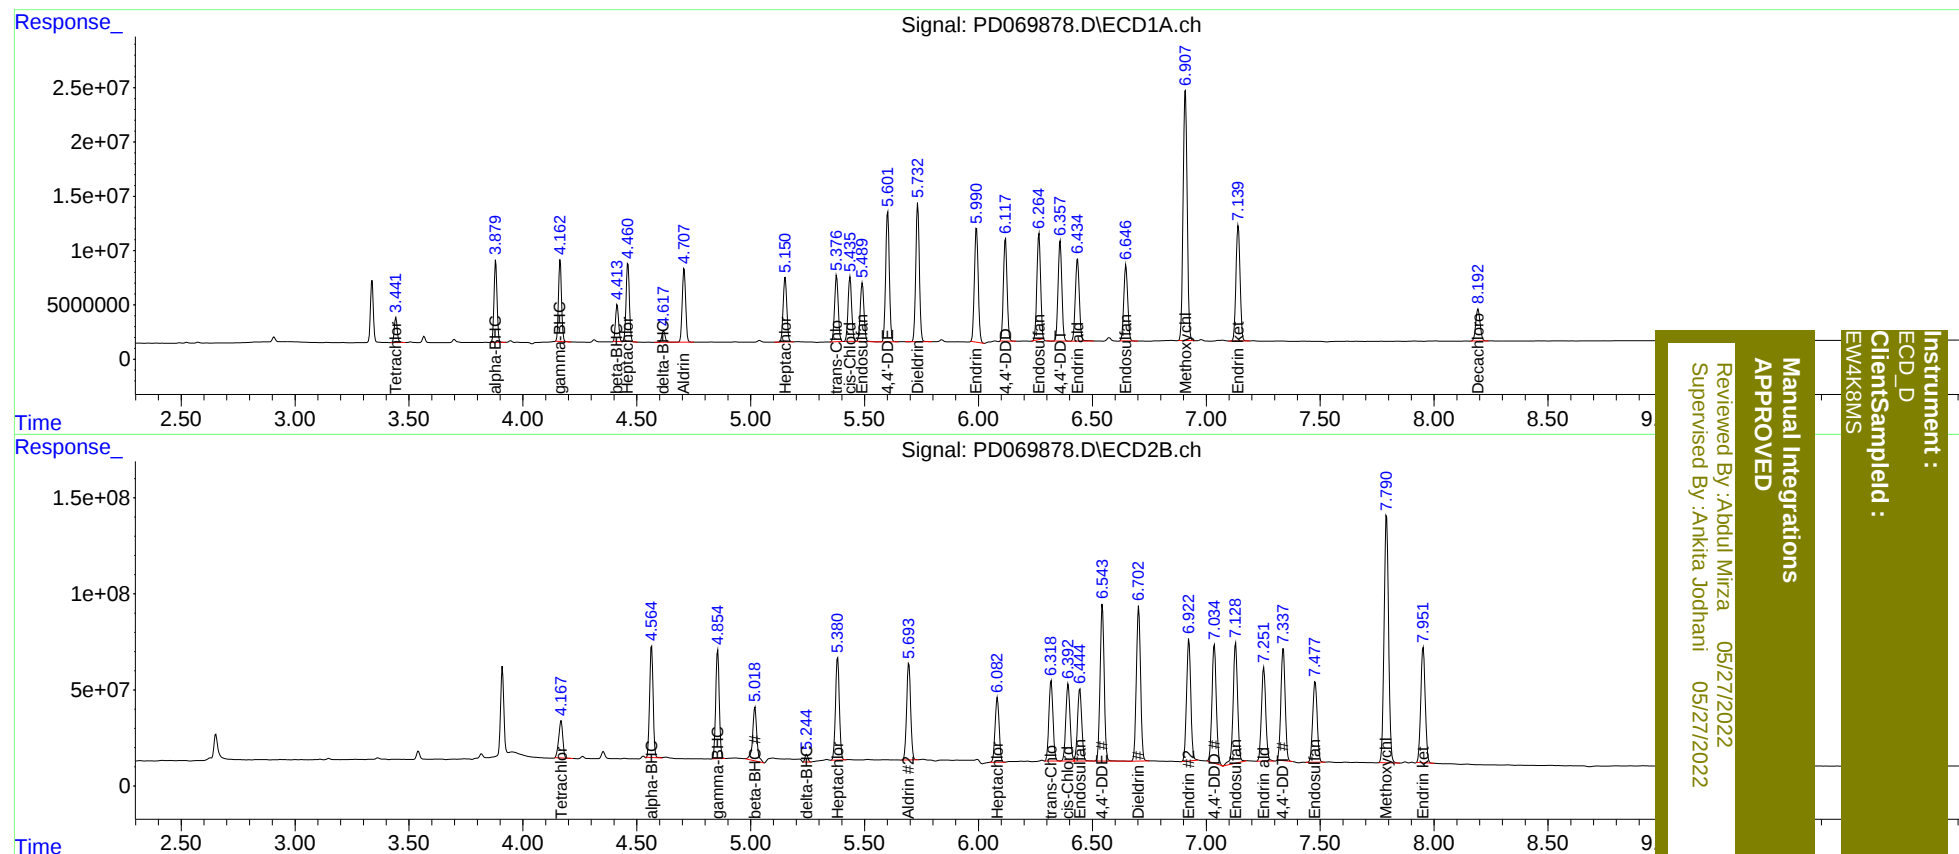

Reviewed By: Abdul Mirza 05/27/2022
Supervised By: Ankita Jodhani 05/27/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
EW4K8MS