

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052722\
 Data File : PD069879.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2022 14:45
 Operator : AR\AJ
 Sample : N2883-12MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4K8MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/27/2022
 Supervised By : Ankita Jodhani 05/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 03:27:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050722CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed May 18 23:46:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.168	19733331	231.5E6	16.233	18.256
27)	SA Decachlor...	8.192	9.361	38054930	215.3E6	30.680	29.488
Target Compounds							
2)	A alpha-BHC	3.881	4.565	67650074	606.9E6	39.660	33.231
3)	MA gamma-BHC...	4.164	4.855	67383741	596.4E6	40.243	36.634
4)	MA Heptachlor	4.461	5.382	68901406	613.5E6	42.588	38.775
5)	MB Aldrin	4.708	5.695	69649704	601.7E6	47.465	41.923
6)	B beta-BHC	4.413	5.018	31958650	342.7E6	44.801m	50.299m
7)	B delta-BHC	4.617	5.246	10288605	33291993	6.817	2.938 #
8)	B Heptachlo...	5.151	6.083	64983873	395.6E6	46.788	36.682
9)	A Endosulfan I	5.489	6.445	59152998	474.0E6	43.010	37.515
10)	B trans-Chl...	5.375	6.319	66122971	512.9E6	46.536m	39.063
11)	B cis-Chlor...	5.434	6.394	63905022	506.5E6	45.872m	39.735
12)	B 4,4'-DDE	5.601	6.544	131.2E6	982.1E6	100.798	85.000
13)	MA Dieldrin	5.733	6.703	136.7E6	1003.7E6	92.186	78.843
14)	MA Endrin	5.991	6.924	121.0E6	794.2E6	92.917	78.530
15)	B Endosulfa...	6.264	7.129	109.7E6	834.4E6	94.078	87.205
16)	A 4,4'-DDD	6.118	7.035	103.1E6	791.6E6	87.935	79.982
17)	MA 4,4'-DDT	6.358	7.338	104.0E6	739.6E6	88.971	77.313
18)	B Endrin al...	6.434	7.253	91285514	625.4E6	87.807	75.726
19)	B Endosulfa...	6.647	7.478	81295114	559.3E6	66.337	59.782
20)	A Methoxychlor	6.908	7.791	283.3E6	1732.1E6	431.193	392.918
21)	B Endrin ke...	7.139	7.953	131.0E6	795.1E6	96.174	83.130

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052722\
Data File : PD069879.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2022 14:45
Operator : AR\AJ
Sample : N2883-12MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 03:27:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050722CLP.M
Quant Title : GC Extractables
QLast Update : Wed May 18 23:46:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

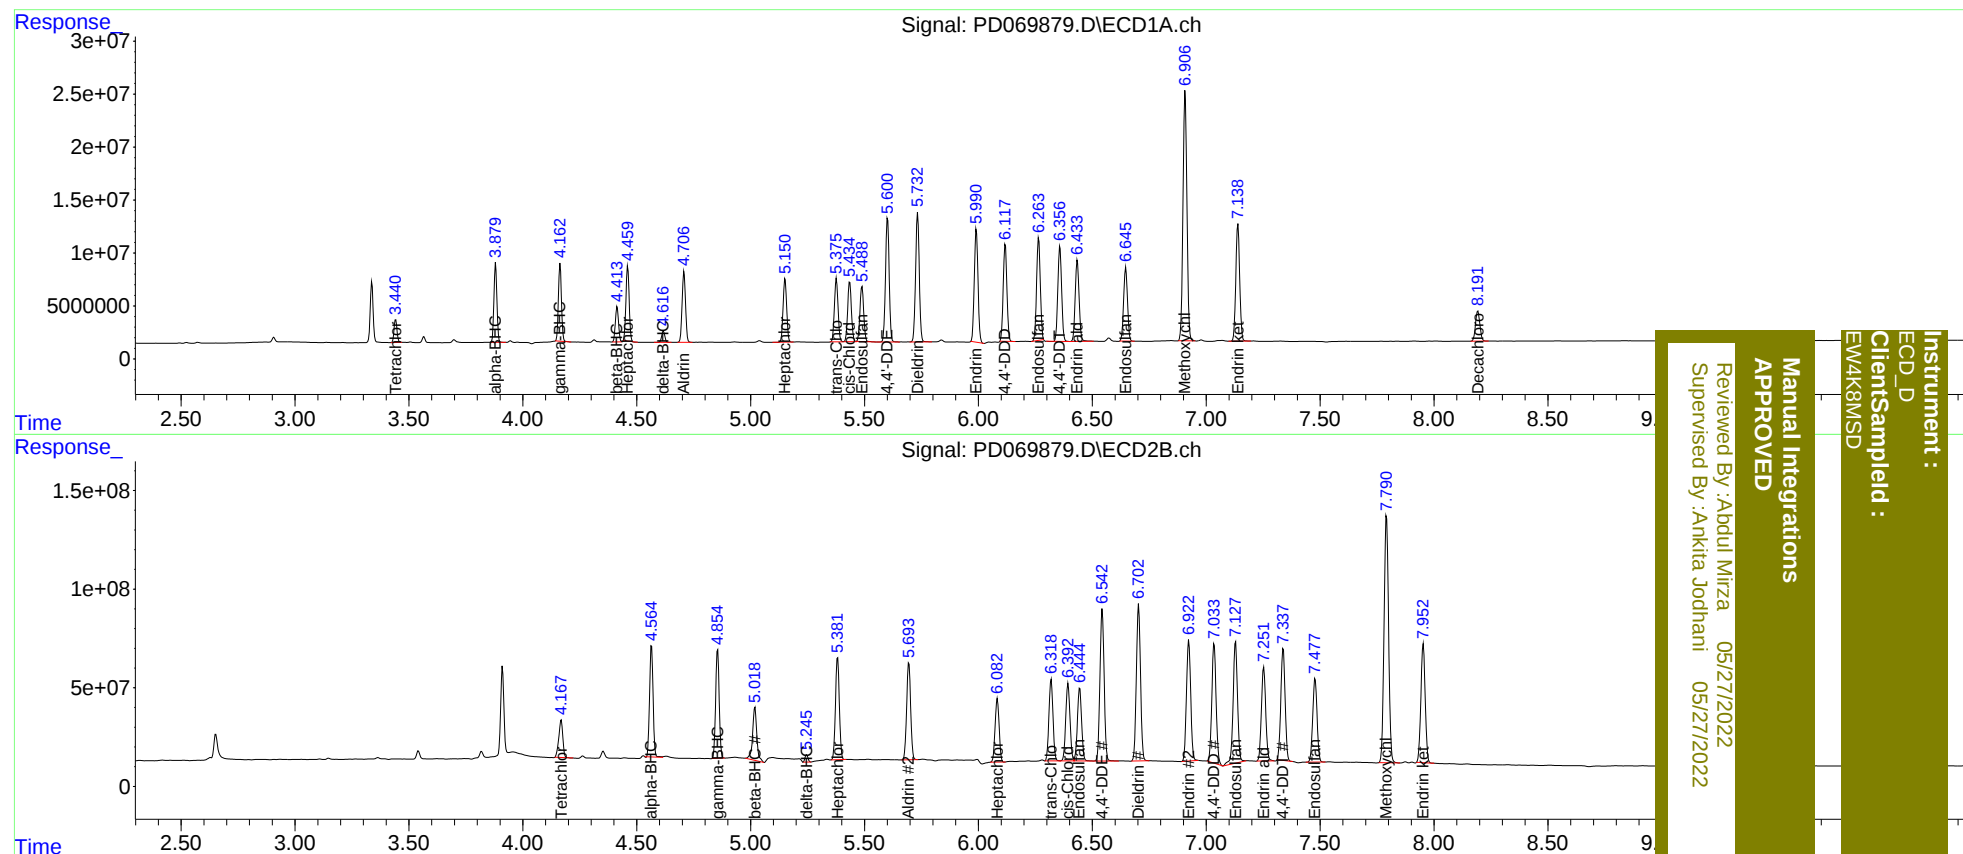

Reviewed By: Abdul Mirza 05/27/2022
Supervised By: Ankita Jodhani 05/27/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
EW4K8MSD