

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052724\
 Data File : PD083115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2024 00:51
 Operator : AR\AJ
 Sample : P2549-10MSD
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH625MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/28/2024
 Supervised By :Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 01:32:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.775	19579636	61526629	13.090m	15.822
27)	SA Decachlor...	9.110	7.901	42571264	102.2E6	21.239m	25.833
Target Compounds							
2)	A alpha-BHC	4.021	3.274	160.3E6	391.5E6	62.821	62.974
3)	MA gamma-BHC...	4.354	3.603	147.6E6	370.2E6	59.819m	63.982
4)	MA Heptachlor	4.946	3.941	149.5E6	335.3E6	59.387m	60.208
5)	MB Aldrin	5.291	4.221	139.4E6	339.8E6	57.588	61.484
6)	B beta-BHC	4.551	3.898	49641148	136.9E6	45.757m	54.605
7)	B delta-BHC	4.800	4.128	142.7E6	368.4E6	58.270	62.269
8)	B Heptachlo...	5.717	4.721	127.3E6	313.5E6	57.025m	61.356
9)	A Endosulfan I	6.105	5.093	114.8E6	183.9E6	55.163	40.786 #
10)	B trans-Chl...	5.973	4.971	181.7E6	434.9E6	83.925m	87.330
11)	B cis-Chlor...	6.056	5.035	255.5E6	501.1E6	114.401	98.667
12)	B 4,4'-DDE	6.226	5.223	373.7E6	1045.5E6	171.375	219.233 #
13)	MA Dieldrin	6.382	5.353	262.7E6	743.8E6	119.507	148.855m
14)	MA Endrin	6.612	5.631	186.4E6	652.2E6	104.540	149.111 #
15)	B Endosulfa...	6.832	5.923	201.2E6	598.6E6	104.457	142.046 #
16)	A 4,4'-DDD	6.744	5.777	209.4E6	429.4E6	135.040m	114.119
17)	MA 4,4'-DDT	7.061	6.026	375.8E6	803.7E6	233.637	209.317
18)	B Endrin al...	6.960	6.100	148.8E6	330.2E6	107.091m	104.691m
19)	B Endosulfa...	7.197	6.324	198.3E6	470.5E6	112.332	117.035
20)	A Methoxychlor	7.537	6.601	485.6E6	1055.3E6	561.285	537.824
21)	B Endrin ke...	7.685	6.829	189.0E6	429.9E6	100.244	95.595

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052724\
Data File : PD083115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2024 00:51
Operator : AR\AJ
Sample : P2549-10MSD
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 01:32:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

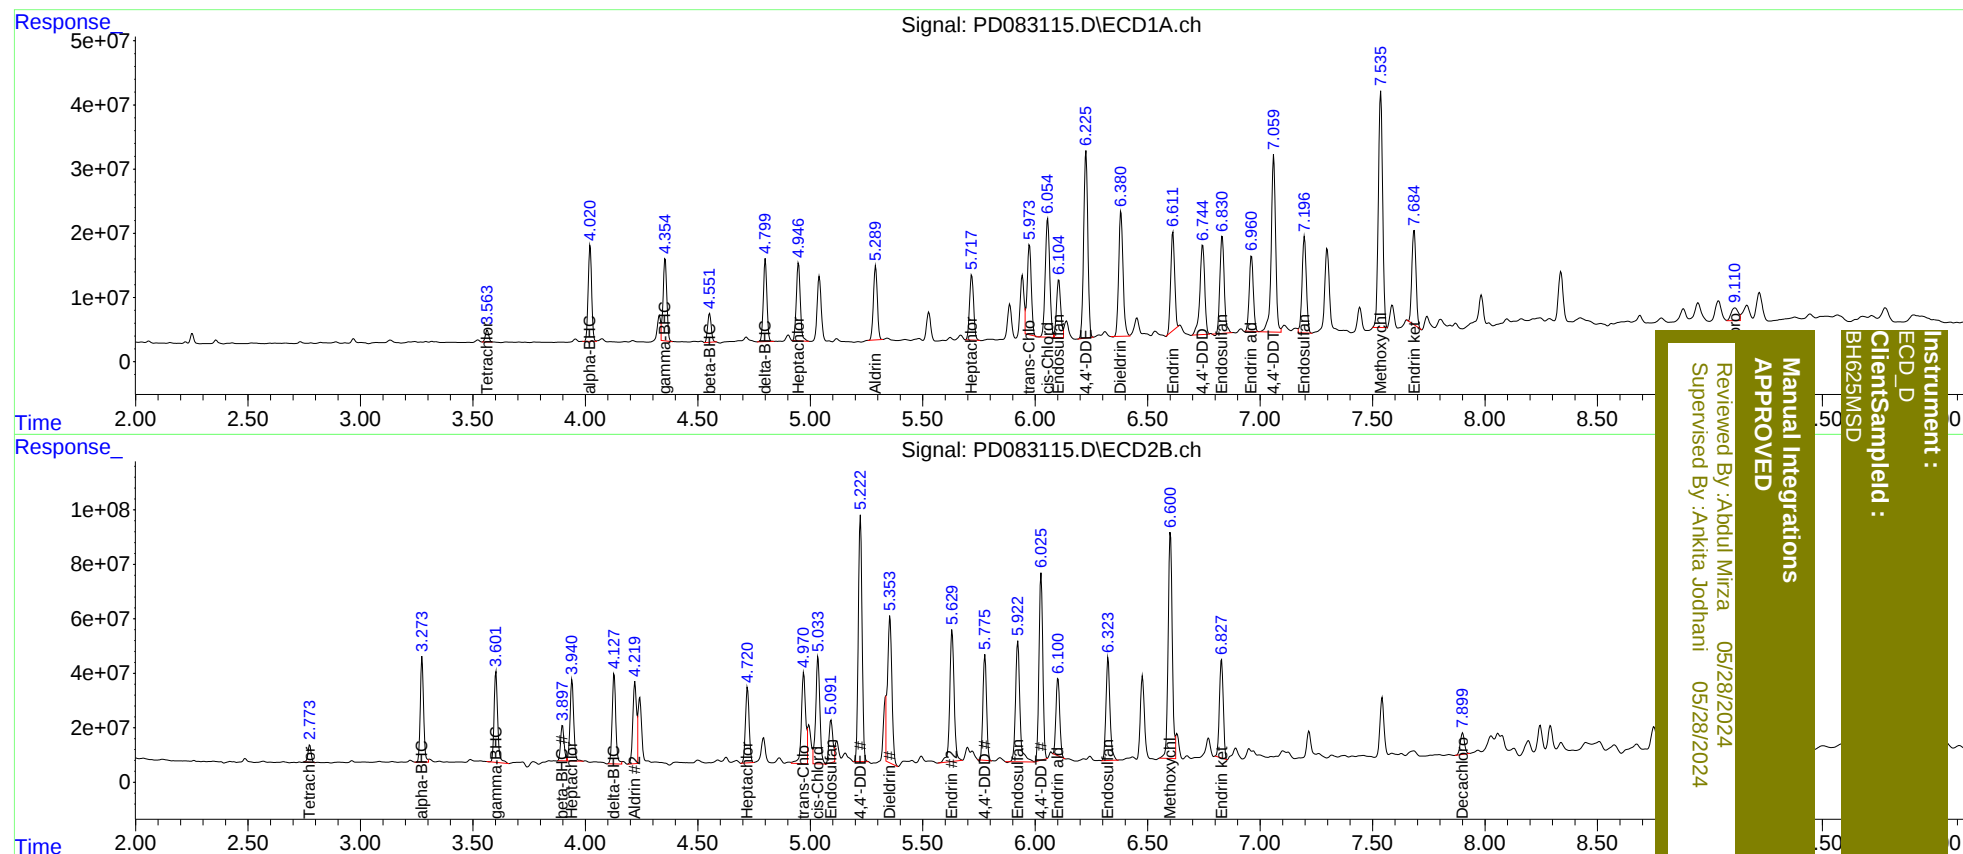

Instrument :
ECD_D
Client Sampled :
BH625MSD

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/28/2024
Supervised By :Ankita Jodhani 05/28/2024