

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052724\
 Data File : PD083120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2024 03:05
 Operator : AR\AJ
 Sample : P2549-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH629

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/28/2024
 Supervised By : Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 07:07:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.775	12814324	62545881	8.567m	16.084 #
27)	SA Decachlor...	9.104	7.900	55102328	126.5E6	27.491m	31.976
Target Compounds							
12)	B 4,4'-DDE	6.227	5.224	2151.0E6	4951.8E6	986.358	1038.381
13)	MA Dieldrin	6.402	5.361	36813587	177.8E6	16.750	35.585m#
16)	A 4,4'-DDD	6.733	5.777	54543498	77803310	35.169m	20.677m#
17)	MA 4,4'-DDT	7.061	6.028	1800.4E6	3384.2E6	1119.383	881.371

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052724\
Data File : PD083120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2024 03:05
Operator : AR\AJ
Sample : P2549-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 07:07:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

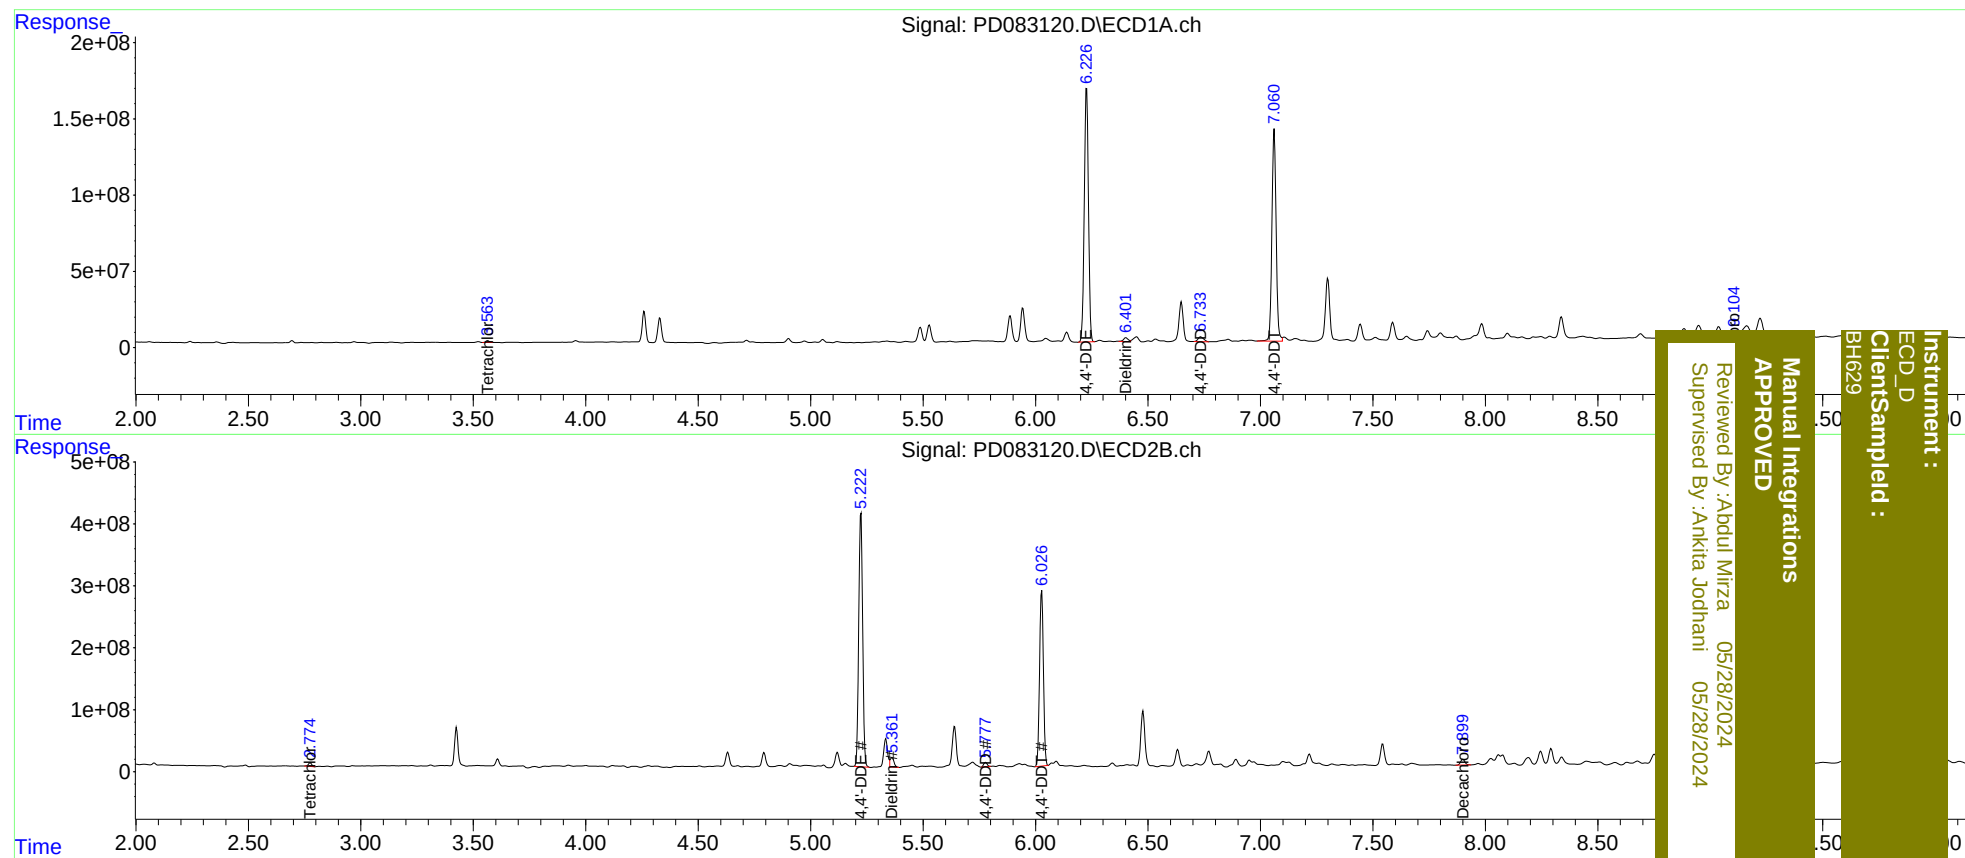

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/28/2024
Supervised By: Ankita Jodhani 05/28/2024

Instrument :
ECD_D
Client Sampled :
BH629